

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018407.D
 Acq On : 27 Nov 2023 18:55
 Operator : MA/JU
 Sample : 05341-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	39	rVB	99681	125429	1.24%	0.149%
2	3.687	98	102	114	rBV	441494	629218	6.20%	0.749%
3	3.928	140	143	149	rVB2	21700	32065	0.32%	0.038%
4	4.022	156	159	166	rVB	27888	36066	0.36%	0.043%
5	7.022	663	669	677	rVB	307024	475242	4.68%	0.566%
6	7.193	692	698	709	rVB	1444348	2237942	22.04%	2.664%
7	7.387	725	731	740	rBV	1283445	1977647	19.48%	2.354%
8	7.487	745	748	754	rVB8	7542	12344	0.12%	0.015%
9	7.857	804	811	818	rBV	1581713	2518996	24.81%	2.999%
10	8.569	924	932	941	rBV	922488	1430918	14.09%	1.704%
11	9.022	1001	1009	1020	rBV	1486077	2403778	23.67%	2.862%
12	9.457	1079	1083	1087	rVB3	16265	23751	0.23%	0.028%
13	9.740	1122	1131	1142	rBV	953984	1578051	15.54%	1.879%
14	10.275	1211	1222	1235	rBV	1662620	2732338	26.91%	3.253%
15	10.657	1280	1287	1297	rVB	1989068	3335611	32.85%	3.971%
16	10.798	1303	1311	1324	rBV	1424909	2435181	23.98%	2.899%
17	11.469	1422	1425	1432	rVB8	7096	12693	0.13%	0.015%
18	11.945	1503	1506	1513	rVB6	15715	26629	0.26%	0.032%
19	12.245	1551	1557	1562	rBV2	34826	55246	0.54%	0.066%
20	13.398	1749	1753	1758	rBV5	15651	25246	0.25%	0.030%
21	13.910	1833	1840	1851	rBV	3014109	4195627	41.32%	4.995%
22	14.187	1880	1887	1899	rBV	3603085	5214599	51.36%	6.208%
23	14.492	1933	1939	1950	rVV	2593343	3777241	37.20%	4.497%
24	14.569	1950	1952	1958	rVB7	6762	11190	0.11%	0.013%
25	14.686	1966	1972	1982	rBV	129828	232338	2.29%	0.277%
26	14.910	2007	2010	2017	rVB7	17053	24586	0.24%	0.029%
27	15.486	2101	2108	2121	rBV	4618695	6469704	63.72%	7.702%
28	15.598	2121	2127	2138	rVV	733645	1009916	9.95%	1.202%
29	15.728	2144	2149	2155	rVB2	24832	37150	0.37%	0.044%
30	16.263	2238	2240	2245	rBV5	7663	12217	0.12%	0.015%
31	16.745	2318	2322	2328	rVB7	6373	11222	0.11%	0.013%
32	16.928	2349	2353	2357	rBV7	7591	10846	0.11%	0.013%
33	17.022	2366	2369	2373	rBV6	6928	12273	0.12%	0.015%
34	17.245	2400	2407	2417	rBV	2837191	3976818	39.17%	4.734%
35	17.345	2417	2424	2438	rBV	4941370	7064048	69.57%	8.410%
36	18.145	2555	2560	2568	rBV2	147543	215593	2.12%	0.257%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018407.D
Acq On : 27 Nov 2023 18:55
Operator : MA/JU
Sample : 05341-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	19.163	2729	2733	2738	rBV	65647	87733	0.86%	0.104%
38	19.233	2741	2745	2750	rBV	60760	93977	0.93%	0.112%
39	19.392	2768	2772	2781	rBV	150162	190707	1.88%	0.227%
40	19.592	2800	2806	2815	rBV	6694428	8787756	86.55%	10.462%
41	21.374	3104	3109	3118	rBV	3548840	4919024	48.44%	5.856%
42	23.721	3500	3508	3524	rVB2	4399905	10153950	100.00%	12.088%
43	23.892	3529	3537	3549	rVB	2275534	5385382	53.04%	6.411%




Sum of corrected areas: 83998288

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018407.D
Acq On : 27 Nov 2023 18:55
Operator : MA/JU
Sample : 05341-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

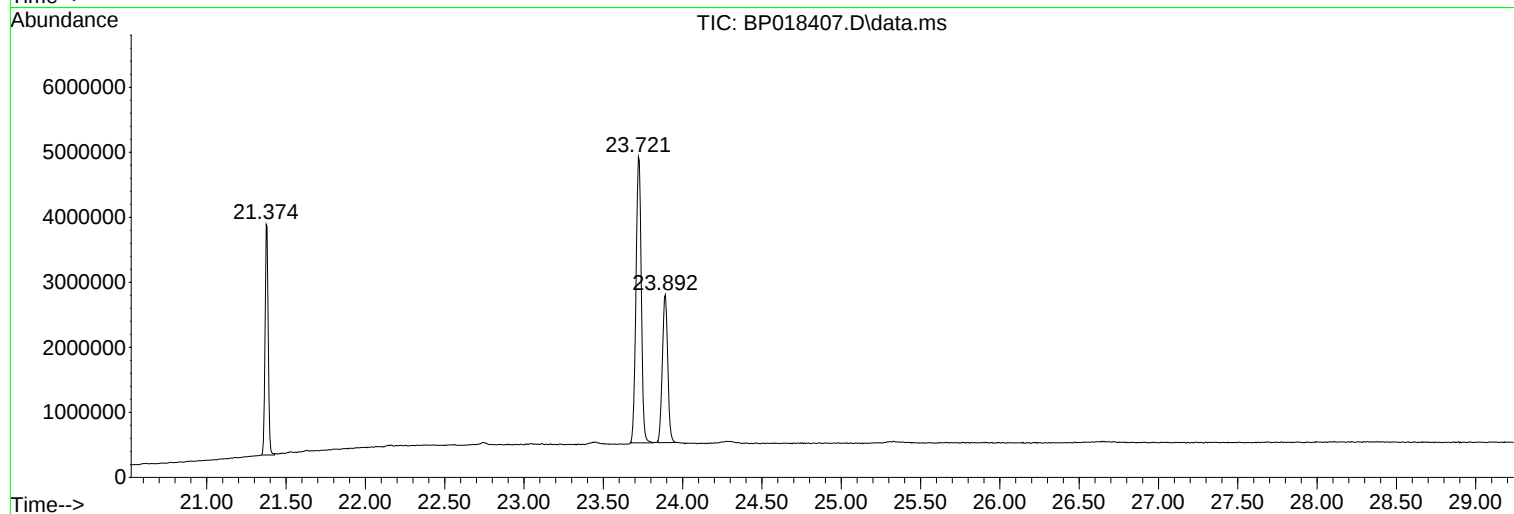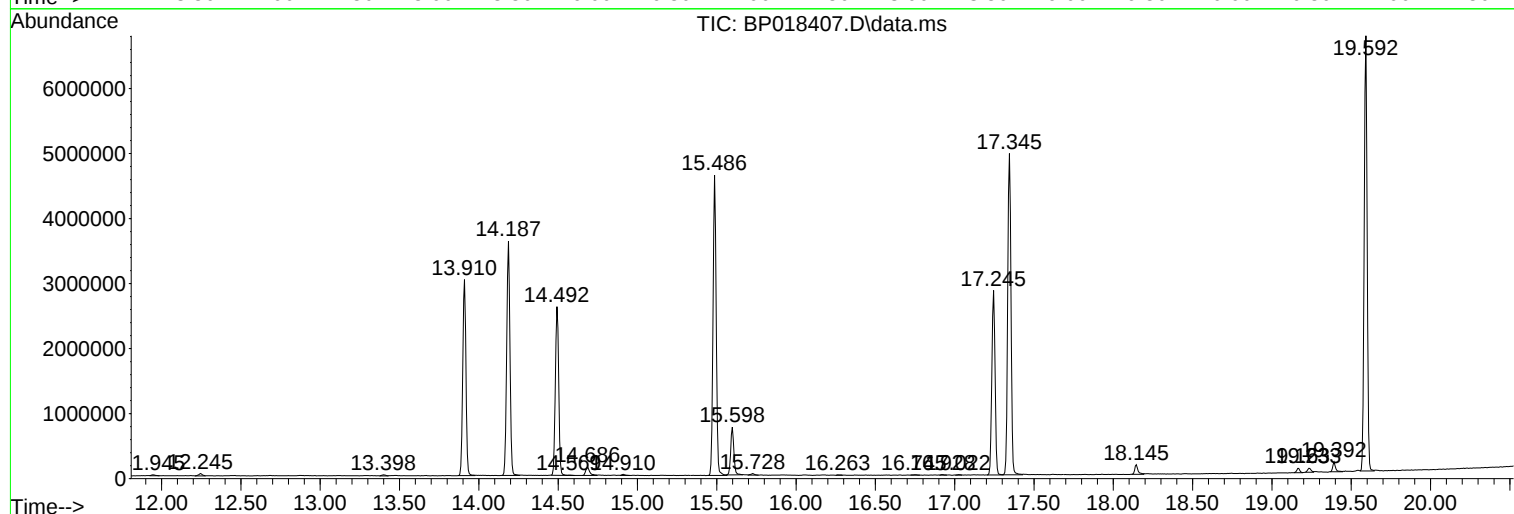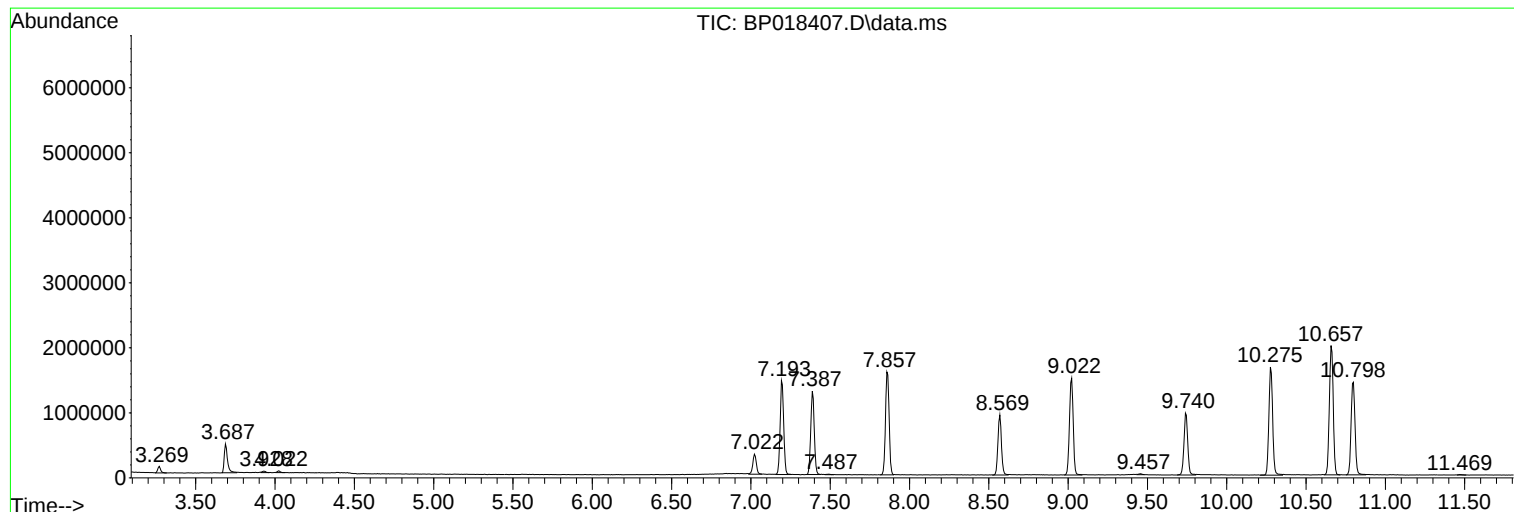

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018407.D
Acq On : 27 Nov 2023 18:55
Operator : MA/JU
Sample : 05341-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018407.D
Acq On : 27 Nov 2023 18:55
Operator : MA/JU
Sample : 05341-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc