

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018408.D
 Acq On : 27 Nov 2023 19:29
 Operator : MA/JU
 Sample : 05341-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	36	rVB	94234	110436	1.28%	0.150%
2	3.687	98	102	113	rBV	463970	669294	7.77%	0.909%
3	3.928	141	143	151	rVB2	23200	30280	0.35%	0.041%
4	4.023	156	159	163	rVB2	24290	30114	0.35%	0.041%
5	6.840	635	638	641	rBV5	5445	8649	0.10%	0.012%
6	7.022	663	669	678	rVB	298691	454699	5.28%	0.618%
7	7.193	692	698	710	rVB	1318394	2033006	23.60%	2.762%
8	7.387	725	731	738	rBV	1197324	1846696	21.44%	2.509%
9	7.487	747	748	757	rVB9	9180	12326	0.14%	0.017%
10	7.858	805	811	818	rBV	1380928	2179119	25.30%	2.960%
11	8.569	925	932	941	rBV	835470	1334102	15.49%	1.812%
12	9.022	999	1009	1019	rBV	1317372	2173221	25.23%	2.952%
13	9.452	1078	1082	1088	rVB7	14402	26929	0.31%	0.037%
14	9.740	1124	1131	1146	rBV	863873	1409713	16.36%	1.915%
15	10.275	1215	1222	1242	rBV	1470588	2480842	28.80%	3.370%
16	10.658	1280	1287	1295	rVB	1765302	2890802	33.56%	3.927%
17	10.799	1302	1311	1319	rBV	1371153	2369459	27.51%	3.219%
18	11.463	1421	1424	1431	rVB9	4379	9428	0.11%	0.013%
19	11.946	1500	1506	1510	rBV6	9274	16064	0.19%	0.022%
20	12.246	1552	1557	1563	rVB2	33517	47098	0.55%	0.064%
21	12.881	1657	1665	1669	rBV10	6330	15782	0.18%	0.021%
22	13.399	1749	1753	1759	rVB4	18248	28173	0.33%	0.038%
23	13.463	1759	1764	1770	rBV9	6711	11727	0.14%	0.016%
24	13.910	1833	1840	1854	rBV	2619311	3567474	41.41%	4.846%
25	14.187	1878	1887	1899	rBV	3246901	4586465	53.24%	6.230%
26	14.493	1930	1939	1950	rBV	2292844	3300487	38.31%	4.483%
27	14.687	1965	1972	1982	rBV	118467	217831	2.53%	0.296%
28	14.910	2005	2010	2015	rBV8	10012	17997	0.21%	0.024%
29	15.145	2048	2050	2057	rVB8	7275	13160	0.15%	0.018%
30	15.210	2057	2061	2066	rBV7	5060	8738	0.10%	0.012%
31	15.487	2101	2108	2120	rBV	3947142	5694433	66.10%	7.735%
32	15.598	2121	2127	2139	rVV	608458	857353	9.95%	1.165%
33	15.728	2145	2149	2153	rBV3	14849	19882	0.23%	0.027%
34	16.216	2229	2232	2235	rVV5	6760	10630	0.12%	0.014%
35	16.916	2349	2351	2357	rVB7	6283	9569	0.11%	0.013%
36	17.016	2365	2368	2373	rBV7	9402	16520	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018408.D
 Acq On : 27 Nov 2023 19:29
 Operator : MA/JU
 Sample : 05341-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	17.116	2382	2385	2390	rVB7	7220	11058	0.13%	0.015%
38	17.245	2400	2407	2417	rBV	2421208	3403922	39.51%	4.624%
39	17.345	2417	2424	2437	rBV	4230052	6213188	72.12%	8.440%
40	17.928	2521	2523	2528	rVB5	8030	10334	0.12%	0.014%
41	18.145	2555	2560	2566	rBV	126318	183015	2.12%	0.249%
42	19.163	2729	2733	2738	rBV3	57092	77040	0.89%	0.105%
43	19.234	2741	2745	2750	rBV	50069	80813	0.94%	0.110%
44	19.392	2768	2772	2776	rBV2	127682	155262	1.80%	0.211%
45	19.592	2800	2806	2813	rBV	5563992	7635665	88.64%	10.372%
46	21.375	3104	3109	3119	rBV	3051055	4171698	48.43%	5.667%
47	23.722	3500	3508	3522	rVB2	3697004	8614567	100.00%	11.702%
48	23.892	3529	3537	3551	rVB2	1865063	4551452	52.83%	6.183%




Sum of corrected areas: 73616512

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018408.D
Acq On : 27 Nov 2023 19:29
Operator : MA/JU
Sample : 05341-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

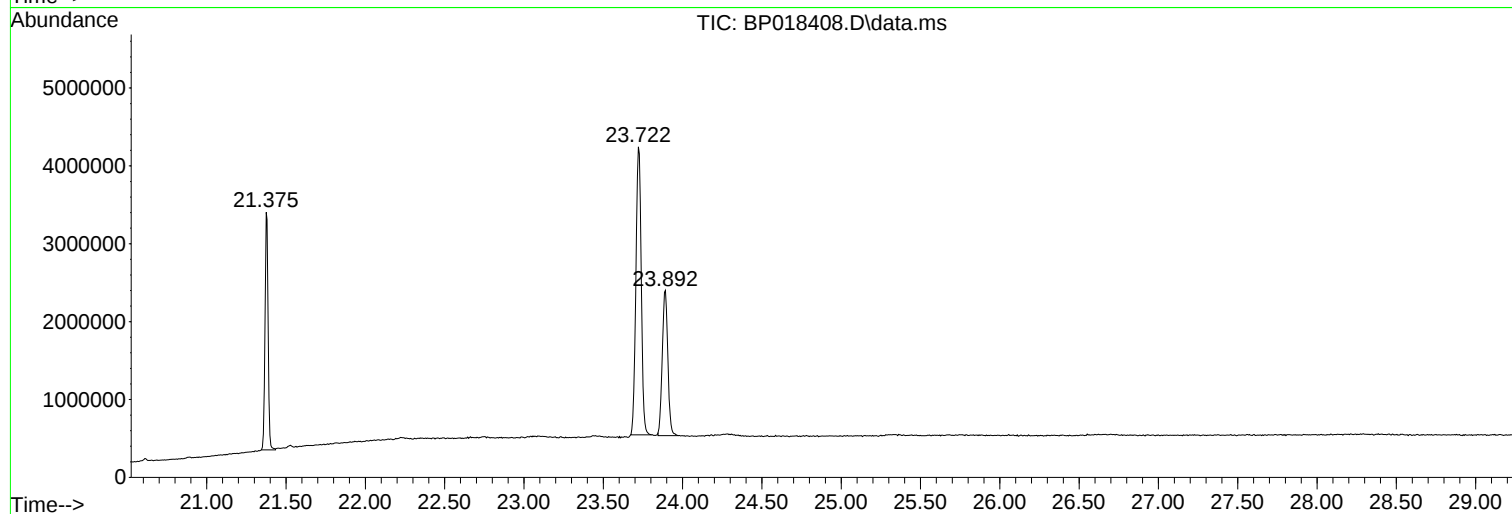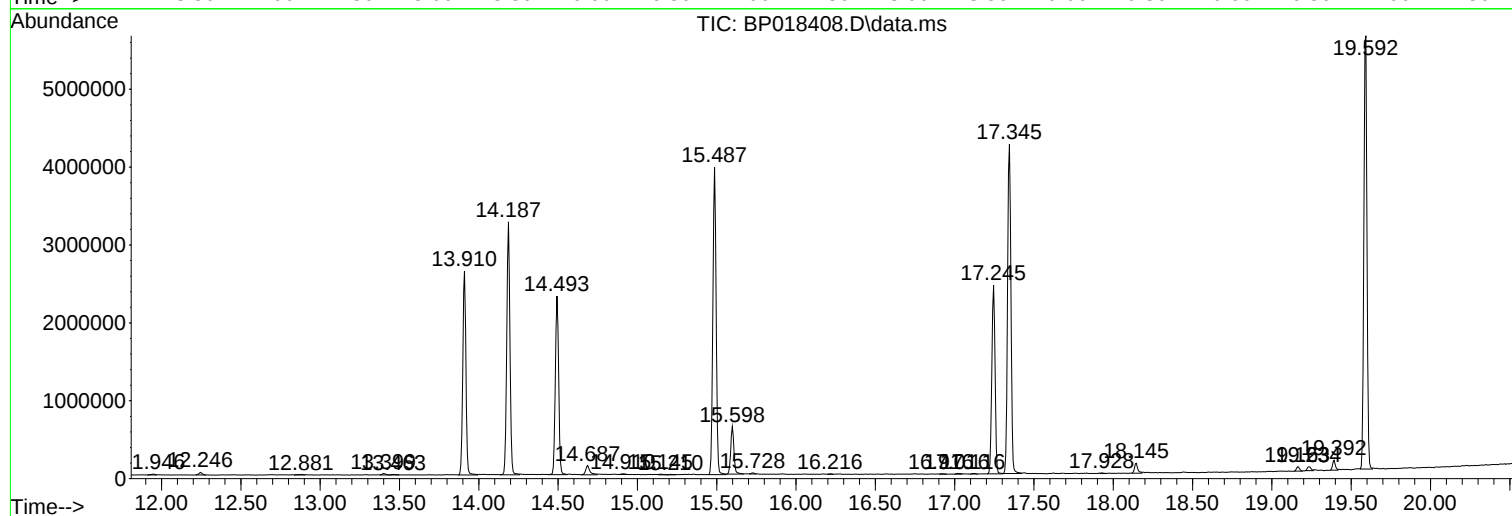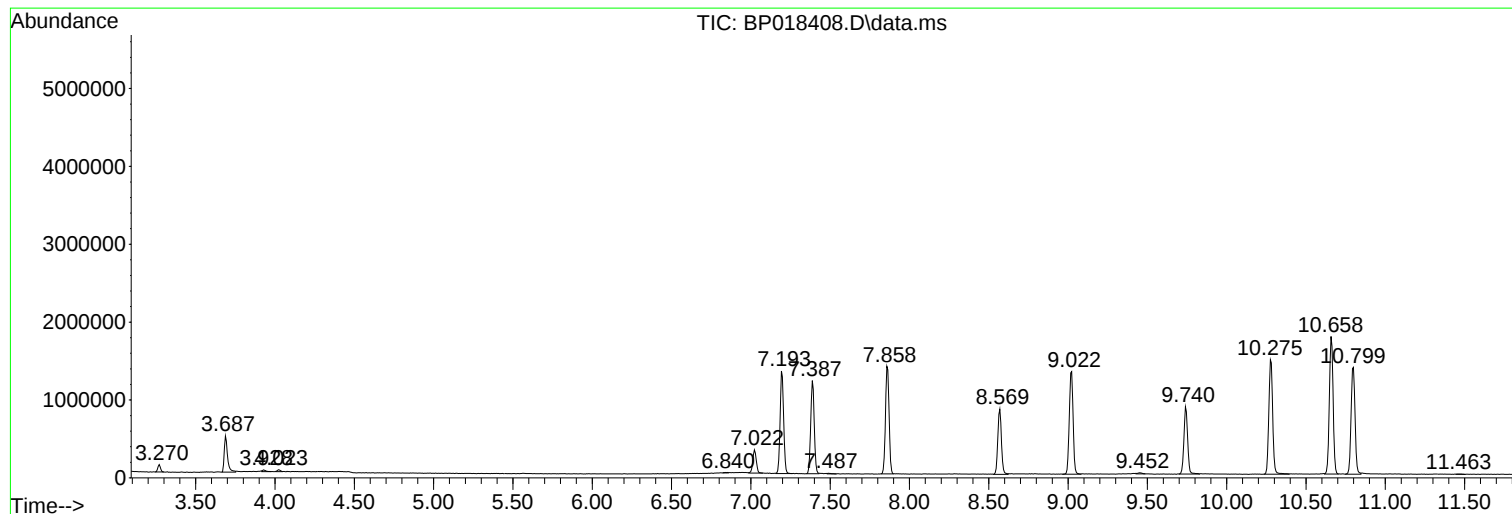

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018408.D
Acq On : 27 Nov 2023 19:29
Operator : MA/JU
Sample : 05341-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018408.D
Acq On : 27 Nov 2023 19:29
Operator : MA/JU
Sample : 05341-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc