

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018410.D
 Acq On : 27 Nov 2023 20:37
 Operator : MA/JU
 Sample : 05332-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	42	rVB	90271	128977	1.23%	0.152%
2	3.687	98	102	113	rBV	389018	568546	5.41%	0.668%
3	3.928	140	143	147	rVB3	24647	31679	0.30%	0.037%
4	4.022	155	159	165	rVB	68560	86849	0.83%	0.102%
5	4.969	317	320	325	rVB5	9277	13325	0.13%	0.016%
6	7.022	663	669	680	rVB	333792	531002	5.05%	0.624%
7	7.193	691	698	706	rBV	1411702	2183041	20.77%	2.566%
8	7.387	721	731	744	rBV	1285980	2009626	19.12%	2.362%
9	7.487	744	748	754	rVB6	10486	17920	0.17%	0.021%
10	7.857	803	811	819	rBV	1558451	2471558	23.52%	2.905%
11	7.934	820	824	831	rVB3	14522	25027	0.24%	0.029%
12	8.569	925	932	945	rBV	965829	1520871	14.47%	1.787%
13	9.022	1001	1009	1018	rBV	1466070	2363032	22.49%	2.777%
14	9.410	1068	1075	1076	rBV7	6728	12043	0.11%	0.014%
15	9.457	1077	1083	1089	rVB2	39853	73201	0.70%	0.086%
16	9.740	1124	1131	1142	rBV	927418	1523976	14.50%	1.791%
17	9.957	1166	1168	1175	rVB8	6073	10562	0.10%	0.012%
18	10.275	1215	1222	1235	rBV	1633128	2697095	25.66%	3.170%
19	10.657	1280	1287	1295	rBV	1970134	3260504	31.03%	3.832%
20	10.793	1302	1310	1325	rBV	1187623	2089027	19.88%	2.455%
21	11.945	1499	1506	1511	rBV4	26848	46222	0.44%	0.054%
22	12.245	1551	1557	1563	rVB	36361	56421	0.54%	0.066%
23	12.687	1626	1632	1634	rBV7	6610	12241	0.12%	0.014%
24	13.116	1700	1705	1710	rVB7	7976	11506	0.11%	0.014%
25	13.334	1737	1742	1746	rVV3	22695	34918	0.33%	0.041%
26	13.398	1748	1753	1759	rVB	48685	78718	0.75%	0.093%
27	13.469	1759	1765	1770	rBV8	7473	15088	0.14%	0.018%
28	13.910	1833	1840	1852	rBV	2906611	4011313	38.17%	4.714%
29	14.187	1878	1887	1897	rBV	3511195	5109185	48.62%	6.004%
30	14.492	1932	1939	1948	rBV	2561787	3783183	36.00%	4.446%
31	14.686	1966	1972	1982	rBV	144233	255793	2.43%	0.301%
32	14.910	2004	2010	2015	rVB10	11322	22067	0.21%	0.026%
33	15.486	2100	2108	2121	rBV	4462559	6268124	59.65%	7.366%
34	15.598	2121	2127	2141	rVV	781615	1108224	10.55%	1.302%
35	15.722	2145	2148	2159	rVB4	21791	44179	0.42%	0.052%
36	16.745	2316	2322	2327	rBV9	7989	17408	0.17%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018410.D
Acq On : 27 Nov 2023 20:37
Operator : MA/JU
Sample : 05332-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	17.128	2381	2387	2392	rBV8	8925	17916	0.17%	0.021%
38	17.245	2400	2407	2417	rBV	2891535	4058615	38.62%	4.770%
39	17.345	2417	2424	2436	rBV	5130242	7272575	69.20%	8.547%
40	17.933	2520	2524	2529	rVB8	11712	17162	0.16%	0.020%
41	18.145	2555	2560	2568	rBV	230581	323979	3.08%	0.381%
42	19.163	2729	2733	2740	rBV2	69264	96093	0.91%	0.113%
43	19.233	2741	2745	2750	rBV	65444	91266	0.87%	0.107%
44	19.392	2768	2772	2778	rBV	98035	127260	1.21%	0.150%
45	19.592	2800	2806	2814	rBV	7195202	9146014	87.03%	10.748%
46	21.139	3064	3069	3081	rBV2	226314	479813	4.57%	0.564%
47	21.380	3104	3110	3119	rBV	3715227	5010935	47.68%	5.889%
48	23.727	3501	3509	3527	rVB2	4418215	10508951	100.00%	12.350%
49	23.898	3530	3538	3553	rVB	2224982	5448091	51.84%	6.403%




Sum of corrected areas: 85091121

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018410.D
Acq On : 27 Nov 2023 20:37
Operator : MA/JU
Sample : 05332-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

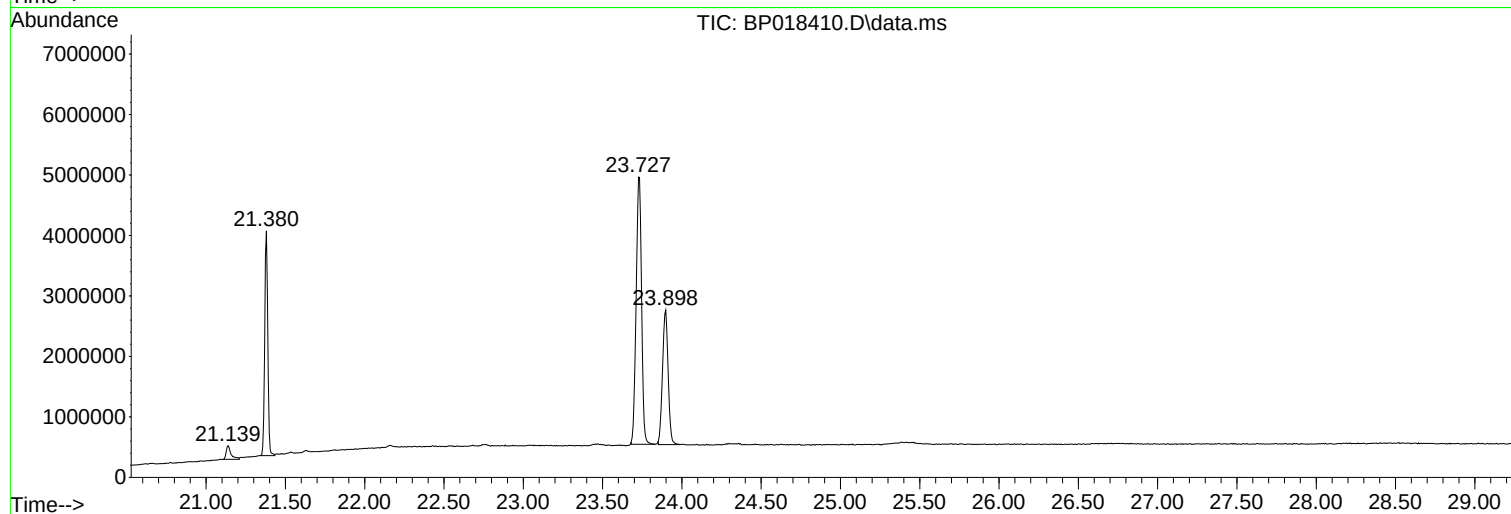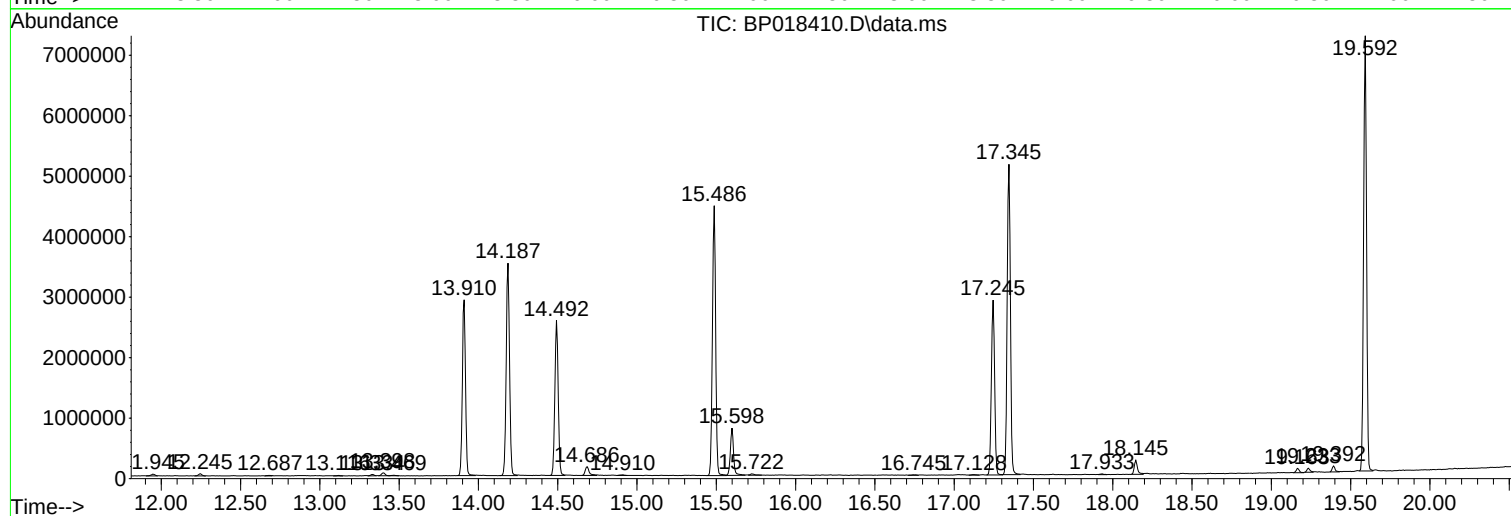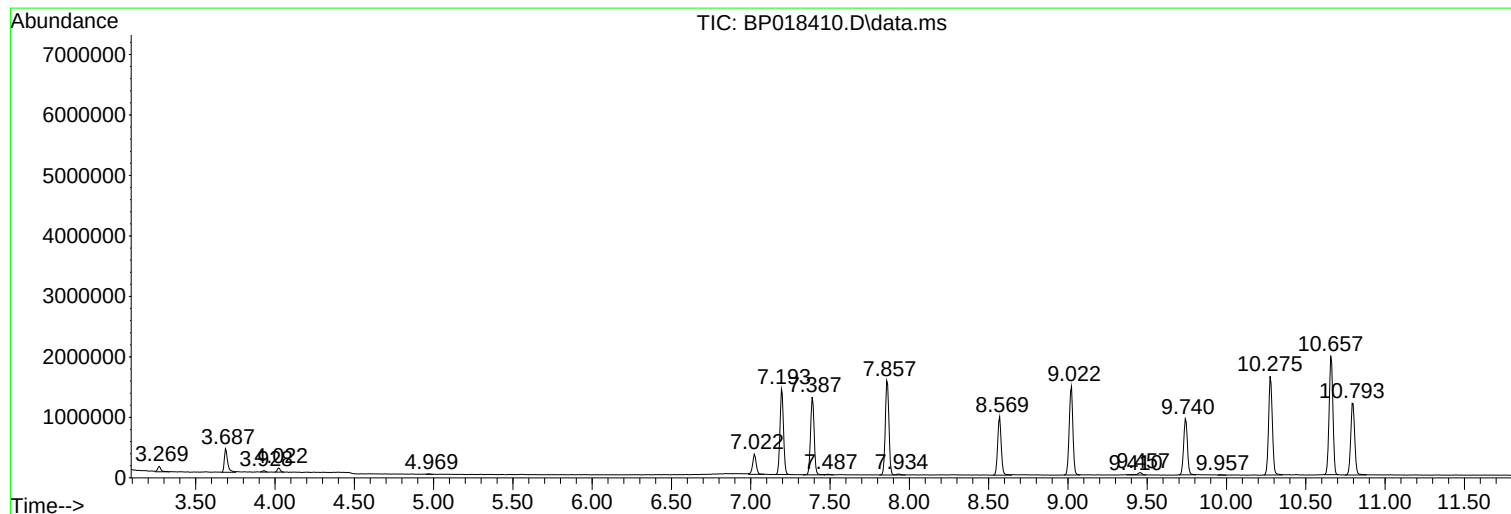

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018410.D
Acq On : 27 Nov 2023 20:37
Operator : MA/JU
Sample : 05332-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018410.D
Acq On : 27 Nov 2023 20:37
Operator : MA/JU
Sample : 05332-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------