

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018415.D
 Acq On : 28 Nov 2023 00:00
 Operator : MA/JU
 Sample : PB157280BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	40	rBV	133285	167170	1.87%	0.177%
2	3.687	97	102	118	rBV	1587027	2332450	26.09%	2.471%
3	4.022	155	159	167	rVB2	23947	44503	0.50%	0.047%
4	7.022	662	669	681	rVB	1804550	2776020	31.05%	2.941%
5	7.193	691	698	711	rVB	1562019	2417189	27.03%	2.561%
6	7.387	723	731	745	rBV	1903810	2961754	33.12%	3.138%
7	7.858	803	811	819	rVB	1514633	2367997	26.48%	2.509%
8	8.569	924	932	943	rBV	2240046	3573202	39.96%	3.786%
9	9.022	1000	1009	1018	rBV	1612883	2659233	29.74%	2.817%
10	9.740	1120	1131	1144	rBV	1221983	1981879	22.16%	2.100%
11	10.275	1214	1222	1236	rBV	2216329	3592308	40.18%	3.806%
12	10.657	1279	1287	1297	rVB	2007404	3338513	37.34%	3.537%
13	10.793	1303	1310	1322	rBV	2108076	3633538	40.64%	3.849%
14	11.946	1500	1506	1512	rBV	7704	19227	0.22%	0.020%
15	12.246	1551	1557	1563	rBV	43087	74141	0.83%	0.079%
16	12.463	1587	1594	1598	rVB10	4847	11988	0.13%	0.013%
17	13.398	1748	1753	1758	rBV7	14664	23708	0.27%	0.025%
18	13.463	1758	1764	1771	rVB8	6973	14254	0.16%	0.015%
19	13.910	1832	1840	1851	rBV	3560355	4899682	54.80%	5.191%
20	14.187	1880	1887	1898	rBV	4296873	6189895	69.23%	6.558%
21	14.493	1932	1939	1949	rBV	2899179	4141148	46.31%	4.387%
22	14.687	1965	1972	1994	rBV	1027383	1601229	17.91%	1.696%
23	15.487	2101	2108	2117	rBV	5145565	7226859	80.82%	7.656%
24	15.598	2121	2127	2142	rVV	755444	1051834	11.76%	1.114%
25	15.728	2142	2149	2154	rVB3	24817	42704	0.48%	0.045%
26	16.269	2238	2241	2246	rVB6	7143	11469	0.13%	0.012%
27	16.745	2318	2322	2328	rBV8	6676	11397	0.13%	0.012%
28	16.922	2348	2352	2357	rBV8	8224	14007	0.16%	0.015%
29	17.028	2366	2370	2373	rBV5	7228	10829	0.12%	0.011%
30	17.116	2381	2385	2392	rBV10	6178	14196	0.16%	0.015%
31	17.245	2398	2407	2417	rBV	2841477	4041635	45.20%	4.282%
32	17.345	2417	2424	2438	rVV	4897006	6835533	76.45%	7.242%
33	18.145	2555	2560	2563	rBV5	10736	17980	0.20%	0.019%
34	19.163	2730	2733	2739	rVB3	55912	72956	0.82%	0.077%
35	19.233	2741	2745	2749	rBV	54560	68928	0.77%	0.073%
36	19.592	2800	2806	2816	rBV	5901736	7734968	86.50%	8.195%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018415.D
Acq On : 28 Nov 2023 00:00
Operator : MA/JU
Sample : PB157280BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK280

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	21.386	3105	3111	3120	rBV	3369917	4488637	50.20%	4.755%
38	23.751	3504	3513	3528	rVB2	3647057	8941647	100.00%	9.473%
39	23.916	3533	3541	3558	rVB	1976790	4983895	55.74%	5.280%


Sum of corrected areas: 94390502

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018415.D
Acq On : 28 Nov 2023 00:00
Operator : MA/JU
Sample : PB157280BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK280

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

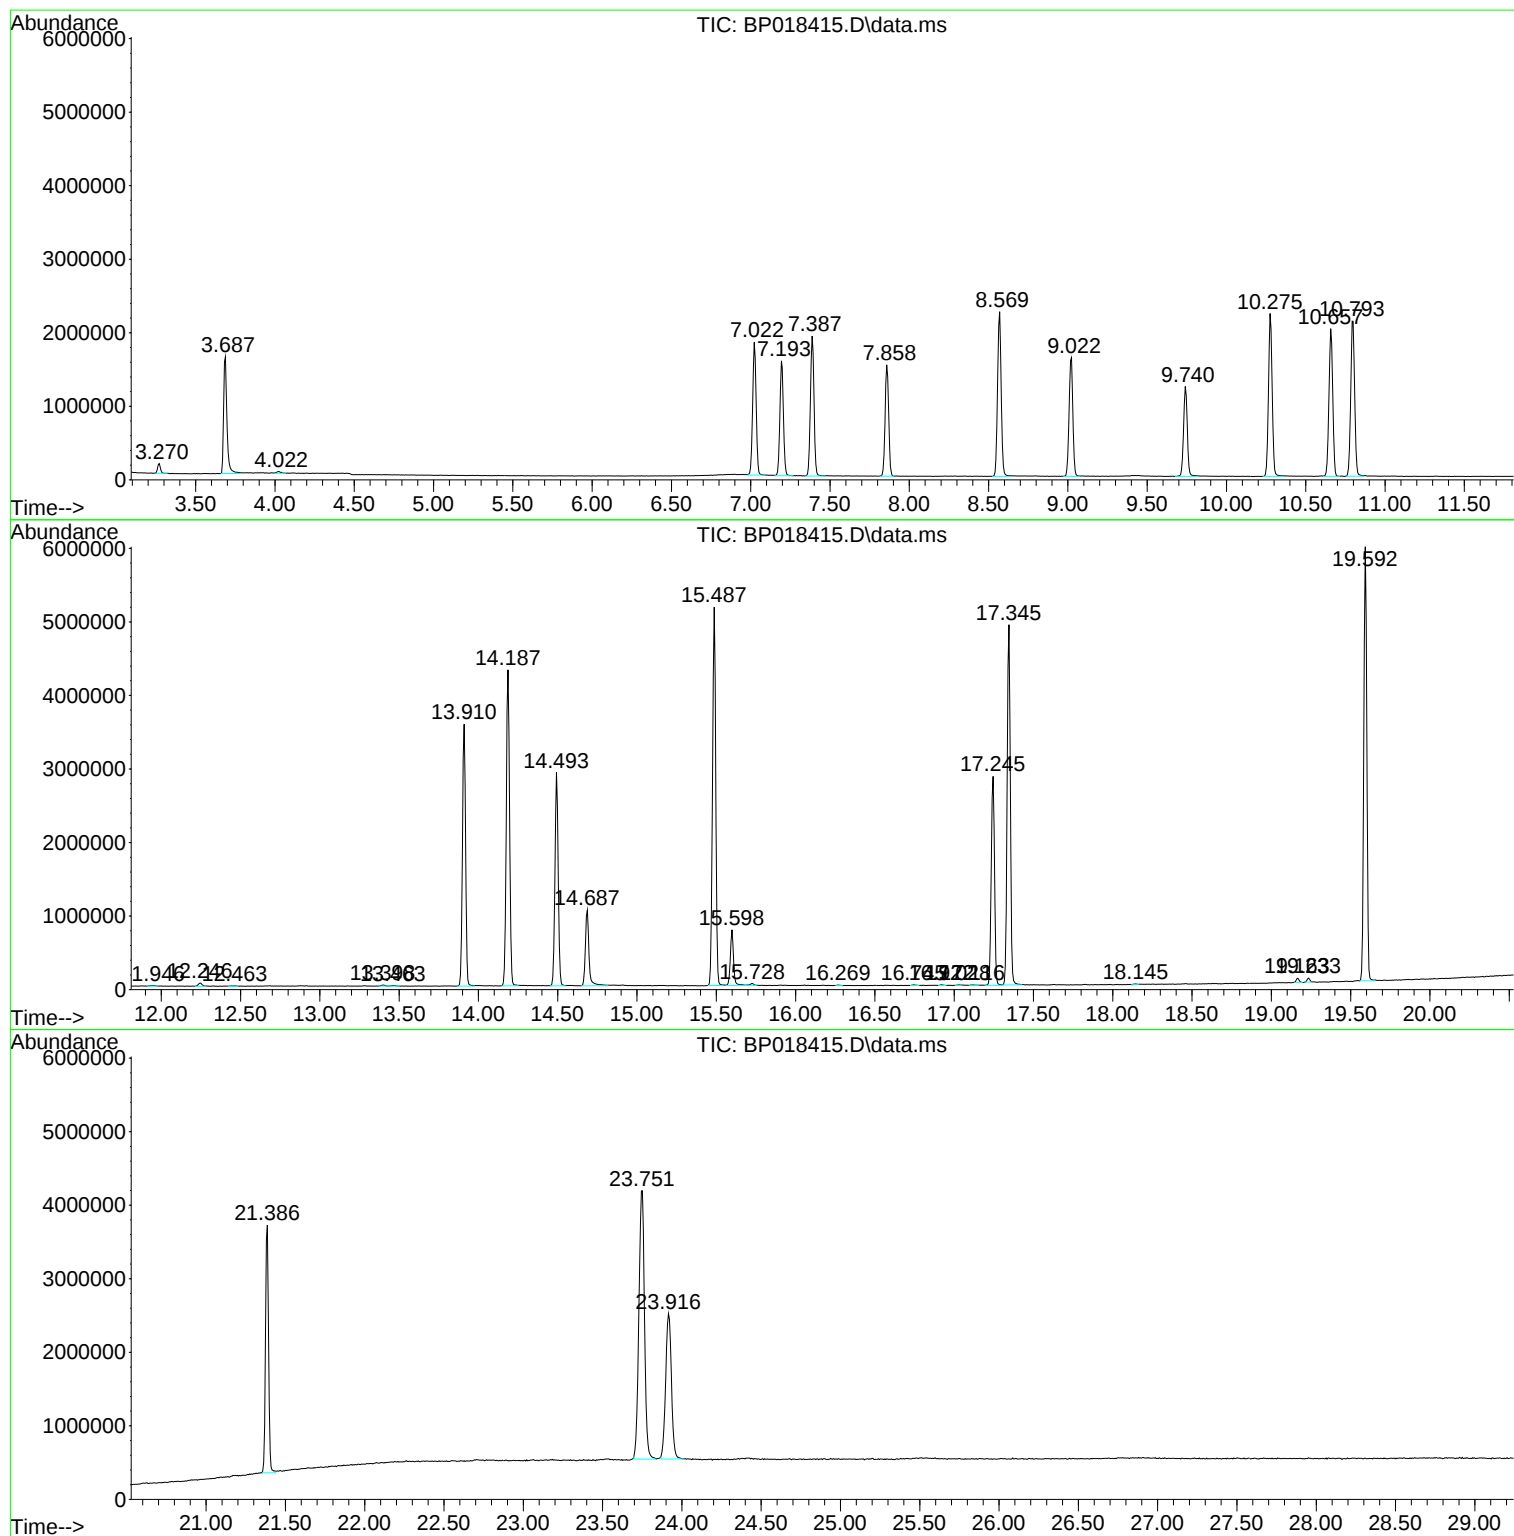

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018415.D
Acq On : 28 Nov 2023 00:00
Operator : MA/JU
Sample : PB157280BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK280

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018415.D
Acq On : 28 Nov 2023 00:00
Operator : MA/JU
Sample : PB157280BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK280

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------