

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018416.D
 Acq On : 28 Nov 2023 00:34
 Operator : MA/JU
 Sample : PB157281BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK281

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	41	rVB	182775	240215	1.96%	0.198%
2	3.687	97	102	117	rBV	2080962	2991439	24.43%	2.460%
3	4.022	156	159	164	rVB	27578	38419	0.31%	0.032%
4	7.022	662	669	681	rVB	2282358	3581192	29.25%	2.944%
5	7.193	692	698	709	rVB	1983183	3101995	25.33%	2.550%
6	7.387	724	731	741	rBV	2440044	3791478	30.96%	3.117%
7	7.857	801	811	820	rBV	1747916	2713861	22.16%	2.231%
8	8.569	924	932	943	rBV	2930074	4601592	37.58%	3.783%
9	9.022	1001	1009	1022	rBV	2149274	3444079	28.13%	2.832%
10	9.440	1075	1080	1086	rVB10	9894	22907	0.19%	0.019%
11	9.740	1122	1131	1142	rBV	1619474	2593140	21.18%	2.132%
12	10.275	1213	1222	1233	rBV	2850876	4658012	38.04%	3.830%
13	10.657	1279	1287	1295	rVB	2350549	3843082	31.38%	3.160%
14	10.798	1302	1311	1326	rBV	2774618	4737869	38.69%	3.895%
15	11.951	1498	1507	1509	rBV7	7622	14448	0.12%	0.012%
16	12.245	1551	1557	1564	rBV	54974	95437	0.78%	0.078%
17	13.398	1749	1753	1758	rVB3	19457	26997	0.22%	0.022%
18	13.469	1760	1765	1769	rBV7	9441	18370	0.15%	0.015%
19	13.910	1832	1840	1851	rBV	4803856	6330168	51.70%	5.205%
20	14.187	1880	1887	1897	rBV	5498842	8071597	65.92%	6.637%
21	14.492	1932	1939	1949	rBV	3303606	4776887	39.01%	3.928%
22	14.687	1965	1972	1984	rBV	1505617	2269997	18.54%	1.866%
23	14.898	2006	2008	2015	rVB7	8090	13799	0.11%	0.011%
24	15.486	2101	2108	2121	rBV	6655209	9469906	77.34%	7.786%
25	15.598	2121	2127	2141	rVV	1132534	1568295	12.81%	1.289%
26	15.728	2144	2149	2156	rVB	33227	57935	0.47%	0.048%
27	16.739	2317	2321	2328	rBV10	6390	13347	0.11%	0.011%
28	17.028	2364	2370	2375	rBV5	10309	20639	0.17%	0.017%
29	17.245	2400	2407	2417	rBV	3521620	4820789	39.37%	3.964%
30	17.345	2417	2424	2441	rVV	6607982	9299908	75.95%	7.646%
31	19.169	2729	2734	2740	rBV3	76639	108336	0.88%	0.089%
32	19.233	2741	2745	2752	rBV	75181	108249	0.88%	0.089%
33	19.592	2800	2806	2816	rBV	8158411	10655705	87.02%	8.761%
34	21.386	3105	3111	3119	rBV	4205169	5374396	43.89%	4.419%
35	23.751	3504	3513	3527	rVB2	4877560	12244994	100.00%	10.068%
36	23.915	3533	3541	3554	rVB	2299328	5904821	48.22%	4.855%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018416.D
Acq On : 28 Nov 2023 00:34
Operator : MA/JU
Sample : PB157281BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK281

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 121624300

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018416.D
Acq On : 28 Nov 2023 00:34
Operator : MA/JU
Sample : PB157281BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK281

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

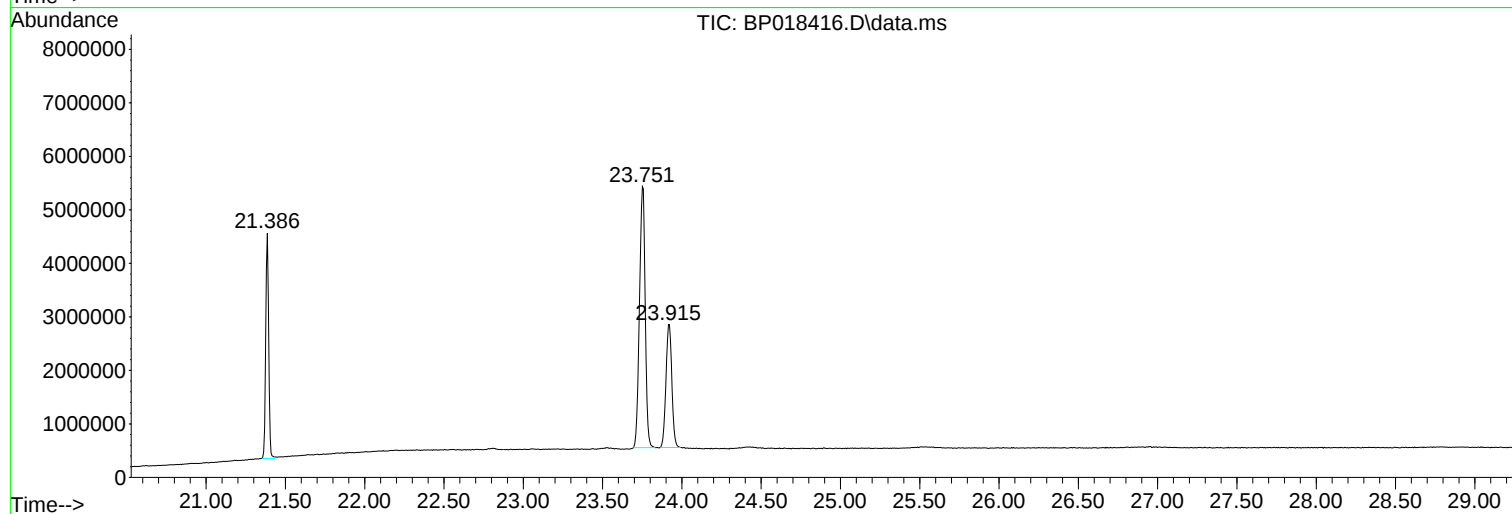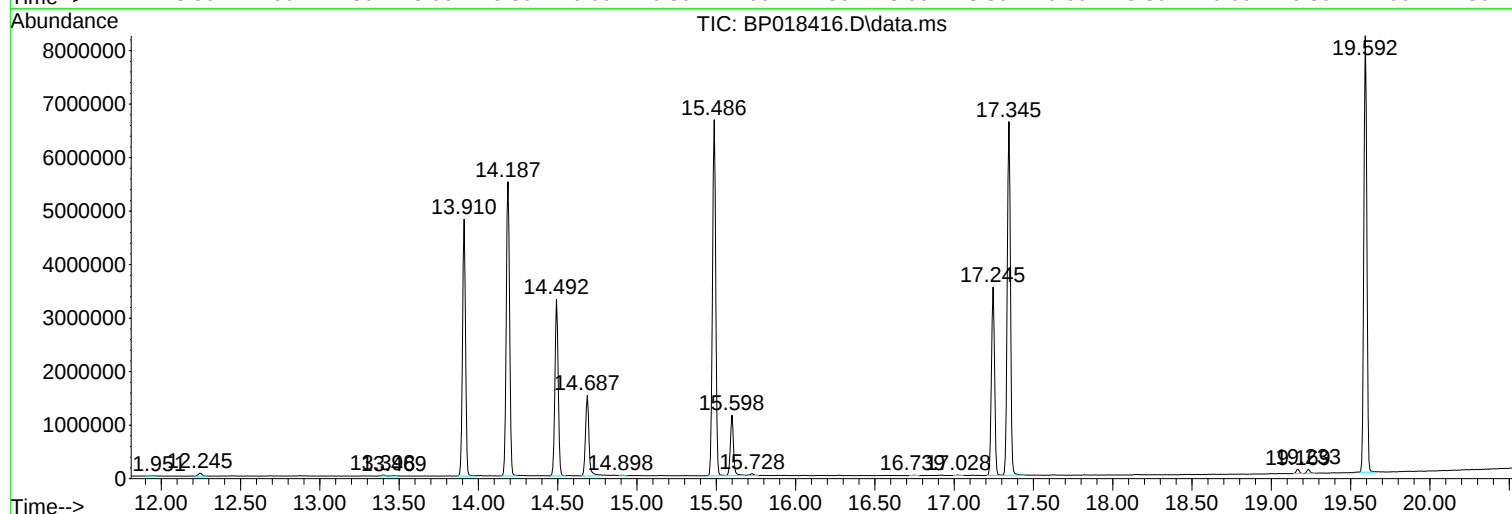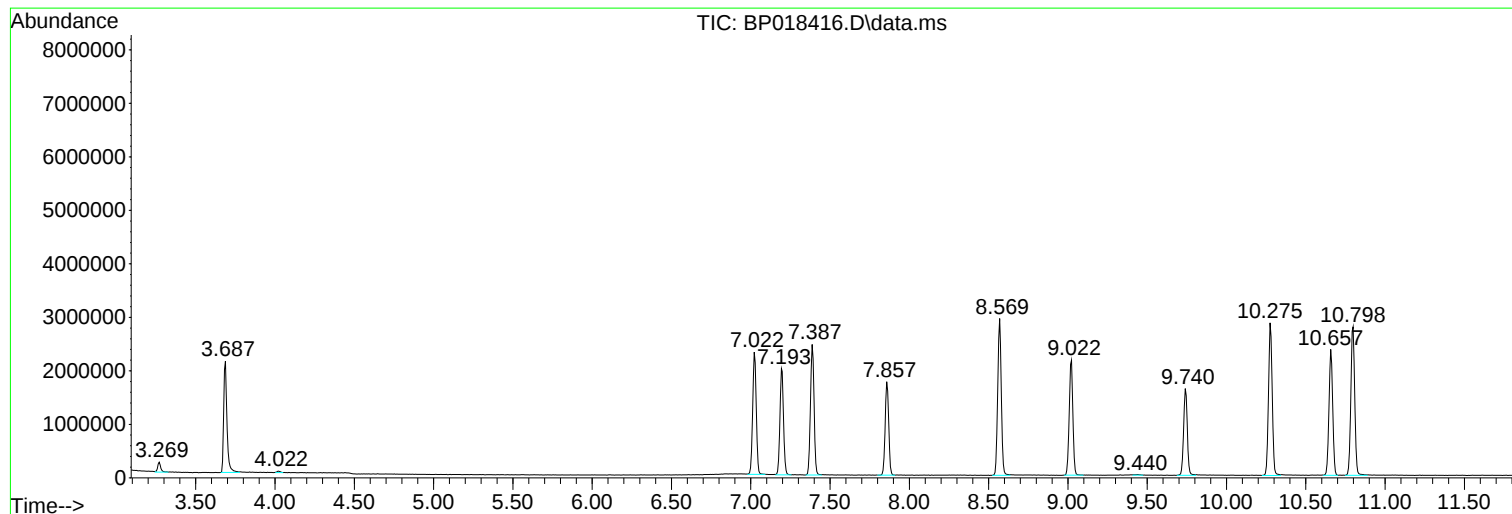

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018416.D
Acq On : 28 Nov 2023 00:34
Operator : MA/JU
Sample : PB157281BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK281

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018416.D
Acq On : 28 Nov 2023 00:34
Operator : MA/JU
Sample : PB157281BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK281

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc