

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018420.D
 Acq On : 28 Nov 2023 02:50
 Operator : MA/JU
 Sample : 05332-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	39	rVB	98672	133425	1.30%	0.124%
2	3.687	98	102	112	rBV	347881	510389	4.97%	0.473%
3	4.022	156	159	164	rVB2	25910	38204	0.37%	0.035%
4	6.852	634	640	644	rBV8	6880	14832	0.14%	0.014%
5	7.022	663	669	682	rVB	452592	722389	7.03%	0.669%
6	7.193	691	698	710	rVB	1721194	2665424	25.94%	2.470%
7	7.387	724	731	743	rBV	1659959	2557532	24.89%	2.370%
8	7.857	804	811	819	rBV	1719009	2685851	26.14%	2.489%
9	7.928	819	823	828	rVB3	13698	19043	0.19%	0.018%
10	8.281	876	883	893	rBV6	12132	33699	0.33%	0.031%
11	8.569	925	932	942	rBV	1316845	2113027	20.56%	1.958%
12	9.022	1000	1009	1017	rBV	1872052	3130403	30.46%	2.901%
13	9.451	1073	1082	1089	rVB	148302	255893	2.49%	0.237%
14	9.740	1122	1131	1144	rBV	1419513	2288722	22.27%	2.121%
15	9.899	1152	1158	1162	rBV4	13265	22067	0.21%	0.020%
16	10.275	1213	1222	1238	rBV	2445610	4060547	39.51%	3.763%
17	10.604	1272	1278	1280	rBV3	11667	18823	0.18%	0.017%
18	10.657	1280	1287	1296	rVB	2404862	4015517	39.08%	3.721%
19	10.793	1302	1310	1322	rBV	1392194	2389878	23.26%	2.215%
20	11.945	1499	1506	1515	rBV	77678	132325	1.29%	0.123%
21	12.175	1540	1545	1550	rBV7	9506	18001	0.18%	0.017%
22	12.245	1550	1557	1562	rVV2	49500	84606	0.82%	0.078%
23	12.692	1627	1633	1635	rBV6	7306	12852	0.13%	0.012%
24	12.857	1652	1661	1667	rBV5	23019	46531	0.45%	0.043%
25	12.904	1667	1669	1672	rVV4	9130	11785	0.11%	0.011%
26	12.969	1675	1680	1685	rVB9	7157	13769	0.13%	0.013%
27	13.110	1700	1704	1708	rVB3	25317	35484	0.35%	0.033%
28	13.287	1726	1734	1736	rBV8	5524	10611	0.10%	0.010%
29	13.334	1736	1742	1748	rVV2	27158	47789	0.47%	0.044%
30	13.398	1748	1753	1759	rVV	68927	115842	1.13%	0.107%
31	13.463	1760	1764	1771	rVB4	11270	20255	0.20%	0.019%
32	13.910	1833	1840	1851	rBV	5144381	6814609	66.31%	6.315%
33	14.004	1852	1856	1866	rVB	13526	33632	0.33%	0.031%
34	14.187	1878	1887	1897	rBV	5464761	8097090	78.79%	7.503%
35	14.398	1919	1923	1929	rVB8	12065	17495	0.17%	0.016%
36	14.492	1932	1939	1950	rVV	3686209	5426764	52.81%	5.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018420.D
 Acq On : 28 Nov 2023 02:50
 Operator : MA/JU
 Sample : 05332-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	14.569	1950	1952	1957	rVB6	9424	12729	0.12%	0.012%
38	14.686	1966	1972	1985	rBV	231216	386991	3.77%	0.359%
39	14.851	1995	2000	2004	rVB6	10439	18354	0.18%	0.017%
40	14.910	2004	2010	2018	rVB6	16750	33460	0.33%	0.031%
41	15.439	2095	2100	2101	rBV5	6747	11237	0.11%	0.010%
42	15.486	2101	2108	2120	rVV	6987167	10067463	97.97%	9.329%
43	15.598	2121	2127	2137	rVV	1330949	1814327	17.66%	1.681%
44	15.722	2145	2148	2152	rBV	27510	31995	0.31%	0.030%
45	16.216	2229	2232	2236	rBV6	8039	13707	0.13%	0.013%
46	16.281	2239	2243	2248	rVB8	14295	25891	0.25%	0.024%
47	16.539	2284	2287	2291	rBV6	8313	14411	0.14%	0.013%
48	17.022	2367	2369	2373	rBV4	9048	15263	0.15%	0.014%
49	17.122	2384	2386	2389	rVB2	11355	11468	0.11%	0.011%
50	17.245	2400	2407	2414	rBV	3983606	5579077	54.29%	5.170%
51	17.345	2417	2424	2435	rVV	7055914	9986128	97.18%	9.254%
52	17.557	2457	2460	2465	rVB5	17095	26356	0.26%	0.024%
53	18.145	2555	2560	2570	rBV	256785	388846	3.78%	0.360%
54	18.439	2608	2610	2618	rVB6	17524	34579	0.34%	0.032%
55	19.169	2730	2734	2738	rVB2	87949	118402	1.15%	0.110%
56	19.233	2741	2745	2750	rBV	83207	120426	1.17%	0.112%
57	19.398	2769	2773	2778	rBV2	96029	119732	1.17%	0.111%
58	19.592	2800	2806	2814	rBV	7760903	10276165	100.00%	9.523%
59	21.157	3068	3072	3079	rBV3	141931	269798	2.63%	0.250%
60	21.386	3106	3111	3120	rBV	3374883	4619702	44.96%	4.281%
61	23.762	3505	3515	3531	rVB2	4041310	10185020	99.11%	9.438%
62	23.933	3535	3544	3557	rVB	1967221	5116988	49.79%	4.742%



Sum of corrected areas: 107913620

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018420.D
Acq On : 28 Nov 2023 02:50
Operator : MA/JU
Sample : 05332-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

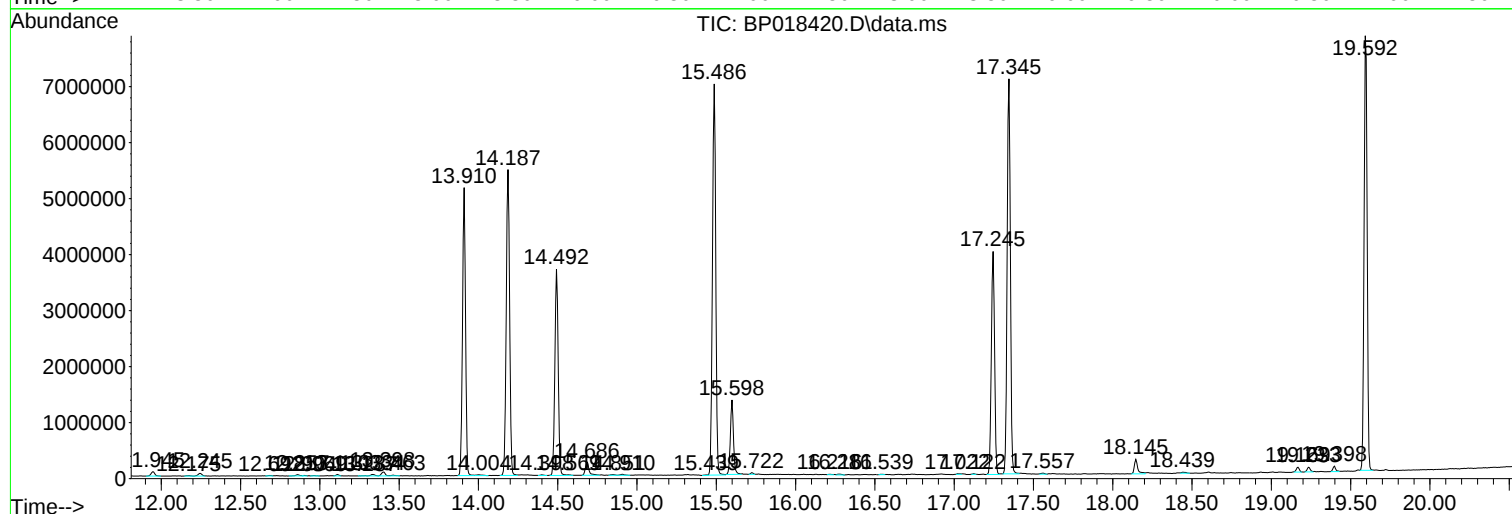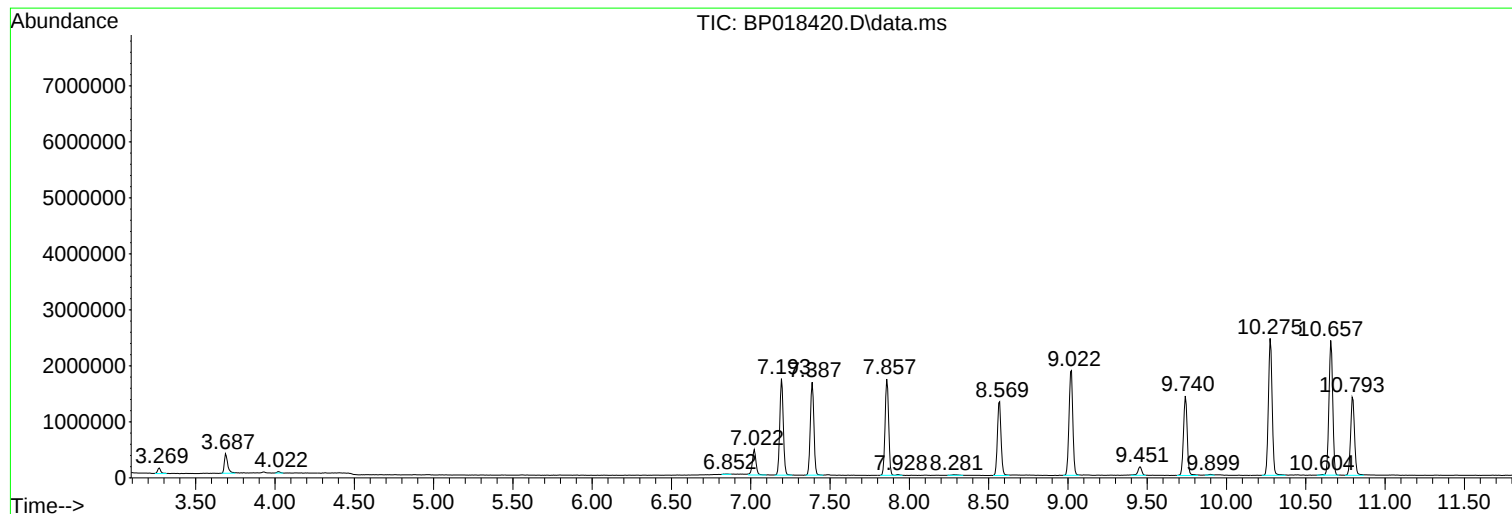

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018420.D
Acq On : 28 Nov 2023 02:50
Operator : MA/JU
Sample : 05332-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018420.D
Acq On : 28 Nov 2023 02:50
Operator : MA/JU
Sample : 05332-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc