

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018421.D
 Acq On : 28 Nov 2023 03:24
 Operator : MA/JU
 Sample : 05332-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	38	rVB	83921	116626	1.18%	0.112%
2	3.687	98	102	114	rBV	455917	674272	6.83%	0.647%
3	3.928	140	143	149	rVB2	20985	30754	0.31%	0.030%
4	4.023	155	159	166	rVB2	25337	38128	0.39%	0.037%
5	6.834	635	637	644	rBV8	8441	15712	0.16%	0.015%
6	7.022	662	669	681	rVB	396336	638871	6.47%	0.613%
7	7.193	691	698	705	rBV	1609318	2447164	24.77%	2.349%
8	7.246	705	707	713	rVB2	19880	23022	0.23%	0.022%
9	7.387	723	731	740	rBV	1469079	2291719	23.20%	2.200%
10	7.858	802	811	818	rBV	1741081	2680028	27.13%	2.572%
11	7.928	818	823	827	rVV3	15467	23210	0.23%	0.022%
12	8.228	868	874	880	rVB	46794	76998	0.78%	0.074%
13	8.358	892	896	900	rVB6	12620	18616	0.19%	0.018%
14	8.563	924	931	940	rBV	1206838	1906783	19.30%	1.830%
15	8.799	968	971	977	rVB8	7369	12612	0.13%	0.012%
16	9.016	1001	1008	1019	rVV	1806286	2904226	29.40%	2.788%
17	9.216	1034	1042	1050	rBV2	46696	83115	0.84%	0.080%
18	9.299	1050	1056	1057	rVV5	8470	12076	0.12%	0.012%
19	9.328	1057	1061	1065	rVV6	11552	27888	0.28%	0.027%
20	9.399	1069	1073	1078	rVV	40499	74912	0.76%	0.072%
21	9.452	1078	1082	1095	rVB2	60564	111967	1.13%	0.107%
22	9.669	1114	1119	1122	rBV7	5986	11942	0.12%	0.011%
23	9.740	1122	1131	1139	rVV	1268597	2040615	20.66%	1.959%
24	9.799	1139	1141	1146	rVV6	11593	15110	0.15%	0.015%
25	10.069	1180	1187	1193	rVB5	35145	69655	0.71%	0.067%
26	10.152	1195	1201	1206	rBV	45543	77826	0.79%	0.075%
27	10.199	1206	1209	1213	rVB5	19877	27338	0.28%	0.026%
28	10.275	1215	1222	1234	rBV	2190207	3576576	36.21%	3.433%
29	10.510	1256	1262	1270	rVB2	32672	59076	0.60%	0.057%
30	10.657	1279	1287	1294	rBV	2411901	3985904	40.35%	3.826%
31	10.710	1294	1296	1301	rVB4	16668	22386	0.23%	0.021%
32	10.793	1301	1310	1316	rBV	1788594	3052044	30.90%	2.929%
33	10.846	1316	1319	1325	rVV	135948	253127	2.56%	0.243%
34	10.905	1325	1329	1333	rVV	89637	142492	1.44%	0.137%
35	10.952	1333	1337	1344	rVB2	52012	90207	0.91%	0.087%
36	11.028	1346	1350	1353	rBV	21641	33214	0.34%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018421.D
 Acq On : 28 Nov 2023 03:24
 Operator : MA/JU
 Sample : 05332-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGB5

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	11.081	1354	1359	1365	rVV2	32575	60651	0.61%	0.058%
38	11.134	1365	1368	1373	rVV2	18635	27734	0.28%	0.027%
39	11.175	1373	1375	1380	rVV5	9939	13428	0.14%	0.013%
40	11.246	1382	1387	1395	rVB4	16675	31903	0.32%	0.031%
41	11.322	1395	1400	1404	rBV8	6156	12647	0.13%	0.012%
42	11.422	1411	1417	1424	rBV4	23118	44897	0.45%	0.043%
43	11.575	1437	1443	1451	rBV10	11326	25052	0.25%	0.024%
44	11.704	1458	1465	1468	rBV8	8223	13942	0.14%	0.013%
45	11.769	1471	1476	1479	rBV6	11206	16037	0.16%	0.015%
46	11.852	1485	1490	1497	rVB6	14821	23899	0.24%	0.023%
47	11.946	1502	1506	1512	rVB3	19107	28611	0.29%	0.027%
48	12.210	1546	1551	1554	rVV	88037	138659	1.40%	0.133%
49	12.246	1554	1557	1564	rVB2	59217	101945	1.03%	0.098%
50	12.369	1573	1578	1583	rVB9	7795	14781	0.15%	0.014%
51	12.510	1595	1602	1610	rVB	41032	94869	0.96%	0.091%
52	12.846	1652	1659	1666	rBV9	14933	39209	0.40%	0.038%
53	12.899	1666	1668	1676	rVB7	8680	14490	0.15%	0.014%
54	12.963	1676	1679	1685	rBV7	9725	16773	0.17%	0.016%
55	13.328	1736	1741	1746	rBV2	35886	55191	0.56%	0.053%
56	13.399	1748	1753	1760	rVV	77848	121495	1.23%	0.117%
57	13.457	1760	1763	1766	rVV4	7969	14510	0.15%	0.014%
58	13.499	1768	1770	1775	rVV6	8604	14766	0.15%	0.014%
59	13.546	1775	1778	1784	rVB8	7915	13935	0.14%	0.013%
60	13.910	1833	1840	1850	rBV	4230514	5910595	59.84%	5.673%
61	14.081	1866	1869	1874	rVB7	11941	21214	0.21%	0.020%
62	14.187	1877	1887	1897	rBV	4850991	7241055	73.31%	6.950%
63	14.398	1919	1923	1928	rVB7	13402	21579	0.22%	0.021%
64	14.493	1932	1939	1948	rBV	3680394	5447289	55.15%	5.228%
65	14.622	1957	1961	1964	rVB6	9145	12546	0.13%	0.012%
66	14.687	1966	1972	1982	rBV	198170	340435	3.45%	0.327%
67	14.893	2003	2007	2016	rVB	34865	69975	0.71%	0.067%
68	15.316	2074	2079	2084	rBV7	16272	29550	0.30%	0.028%
69	15.487	2101	2108	2120	rBV	6383698	8855323	89.65%	8.499%
70	15.598	2121	2127	2137	rBV	1215870	1661158	16.82%	1.594%
71	15.728	2145	2149	2158	rVB2	26500	57763	0.58%	0.055%
72	15.845	2164	2169	2173	rBV4	24951	41264	0.42%	0.040%
73	15.928	2180	2183	2188	rVV6	10735	16152	0.16%	0.016%
74	15.981	2188	2192	2195	rVB4	23842	29096	0.29%	0.028%
75	16.051	2200	2204	2208	rBV7	14003	24410	0.25%	0.023%
76	16.216	2229	2232	2236	rVV5	12735	17603	0.18%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018421.D
 Acq On : 28 Nov 2023 03:24
 Operator : MA/JU
 Sample : 05332-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	16.275	2238	2242	2245	rVB6	13938	18338	0.19%	0.018%
78	16.510	2276	2282	2286	rBV9	10142	20206	0.20%	0.019%
79	16.740	2317	2321	2324	rBV6	8863	15585	0.16%	0.015%
80	16.916	2349	2351	2356	rVB6	15133	17106	0.17%	0.016%
81	17.034	2365	2371	2374	rBV5	26139	50251	0.51%	0.048%
82	17.181	2392	2396	2398	rBV4	13765	16556	0.17%	0.016%
83	17.245	2399	2407	2417	rVV	4151797	5722514	57.93%	5.493%
84	17.345	2417	2424	2433	rVV	6574670	9296920	94.12%	8.923%
85	17.422	2433	2437	2448	rVB4	49840	101538	1.03%	0.097%
86	17.545	2454	2458	2465	rBV4	9424	19218	0.19%	0.018%
87	17.616	2468	2470	2473	rBV2	10565	13206	0.13%	0.013%
88	17.934	2521	2524	2526	rBV3	13999	20990	0.21%	0.020%
89	18.145	2553	2560	2568	rBV2	302081	523386	5.30%	0.502%
90	18.416	2601	2606	2619	rBV	78272	162142	1.64%	0.156%
91	18.604	2636	2638	2643	rVB4	19593	19351	0.20%	0.019%
92	19.075	2715	2718	2722	rVB5	44417	56491	0.57%	0.054%
93	19.169	2730	2734	2738	rBV2	86041	111092	1.12%	0.107%
94	19.233	2741	2745	2750	rVV	74370	103140	1.04%	0.099%
95	19.392	2769	2772	2777	rBV3	83768	105572	1.07%	0.101%
96	19.592	2800	2806	2815	rBV	7023475	9877941	100.00%	9.481%
97	21.157	3069	3072	3082	rVB5	128385	239372	2.42%	0.230%
98	21.386	3106	3111	3119	rBV	3532492	4737188	47.96%	4.547%
99	23.763	3506	3515	3531	rVB	3725468	9414144	95.30%	9.036%
100	23.933	3536	3544	3557	rVB	1915558	5122434	51.86%	4.917%


Sum of corrected areas: 104187323

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018421.D
Acq On : 28 Nov 2023 03:24
Operator : MA/JU
Sample : 05332-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

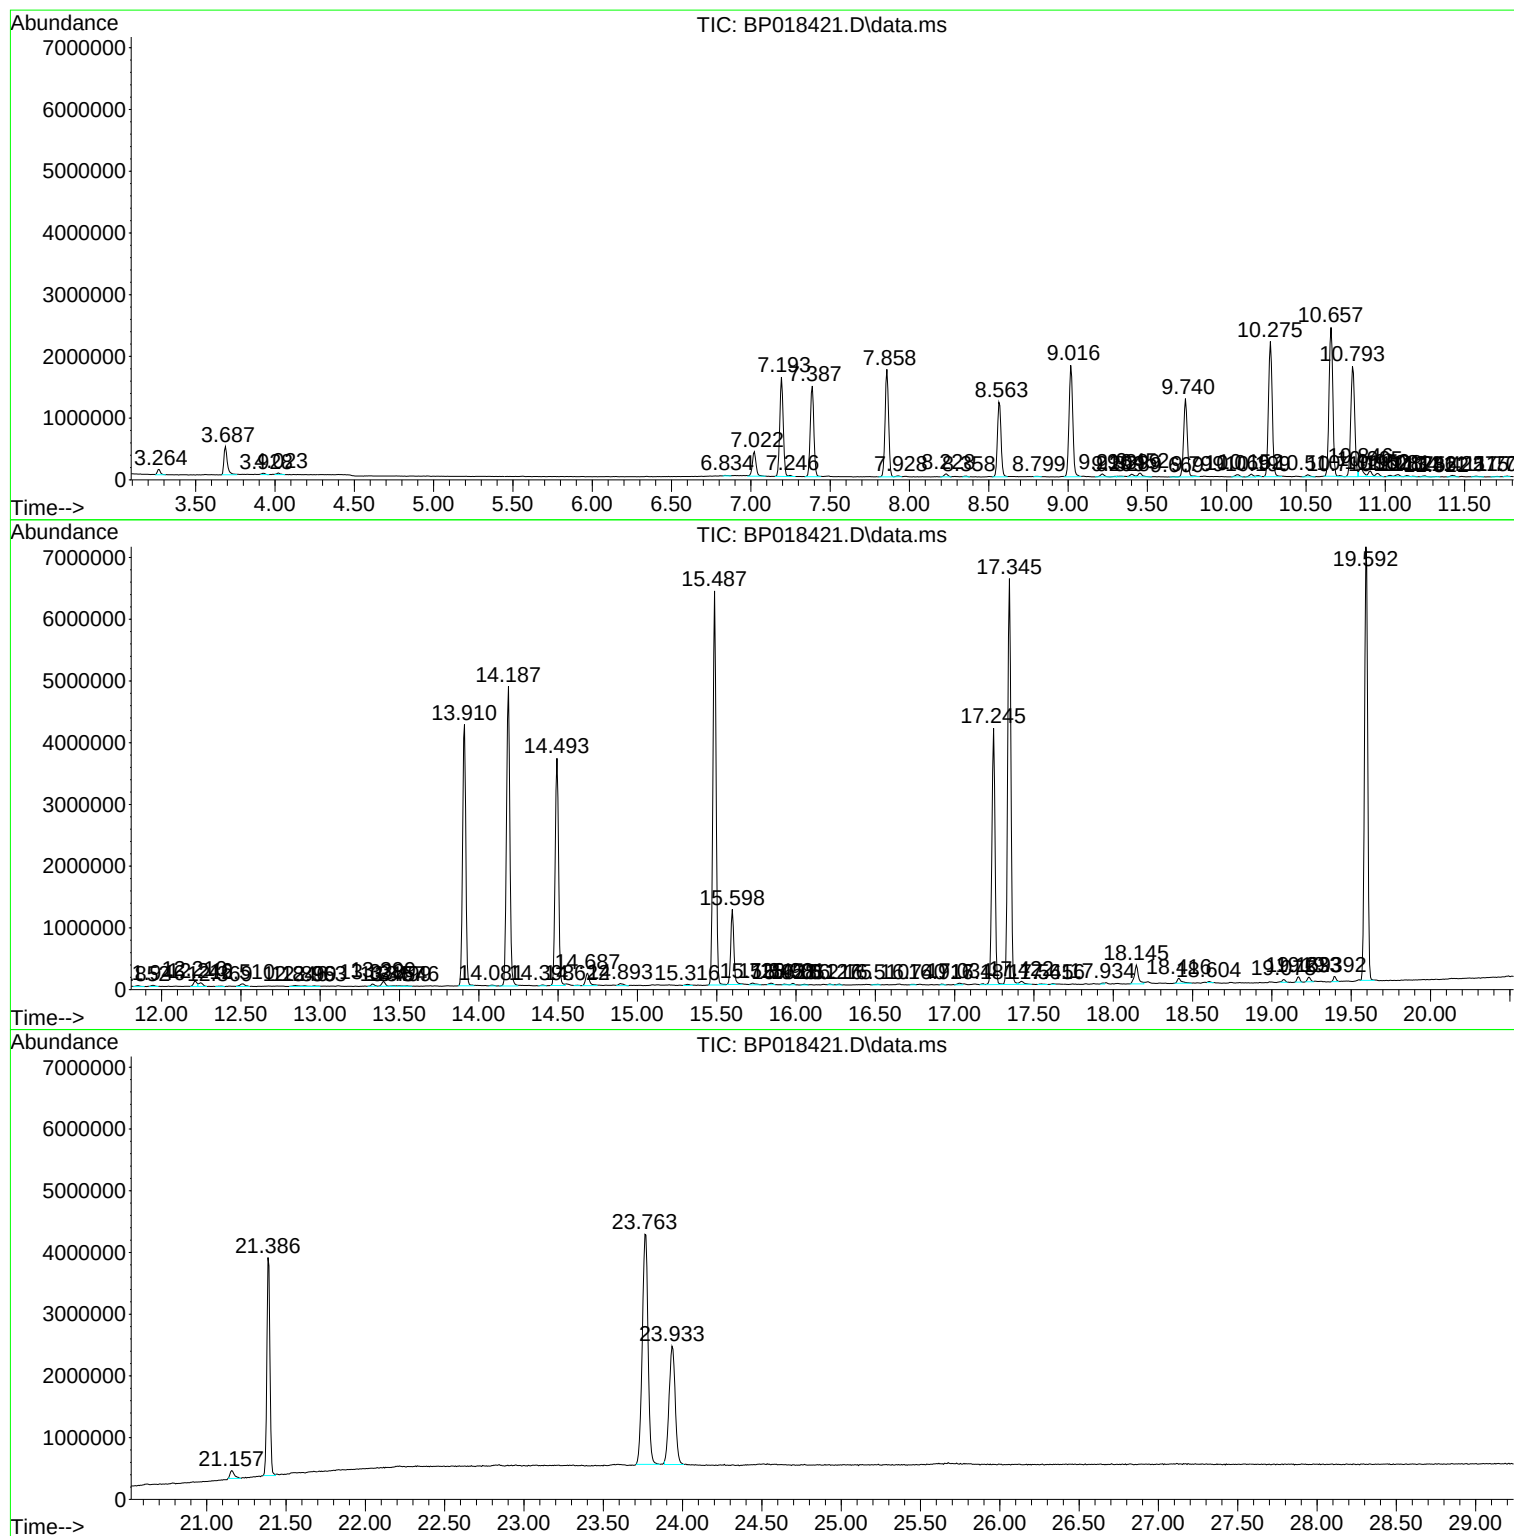

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018421.D
Acq On : 28 Nov 2023 03:24
Operator : MA/JU
Sample : 05332-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018421.D
Acq On : 28 Nov 2023 03:24
Operator : MA/JU
Sample : 05332-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
