

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018422.D
 Acq On : 28 Nov 2023 03:57
 Operator : MA/JU
 Sample : 05332-20
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	36	rVB	90584	120577	1.22%	0.120%
2	3.687	98	102	118	rBV	474241	697402	7.08%	0.694%
3	3.928	140	143	148	rVB	20893	30687	0.31%	0.031%
4	4.016	156	158	164	rVB2	22627	31193	0.32%	0.031%
5	4.957	316	318	322	rVB4	7945	10706	0.11%	0.011%
6	5.557	417	420	425	rVB7	6291	10372	0.11%	0.010%
7	6.269	536	541	544	rBV7	7039	12600	0.13%	0.013%
8	6.851	634	640	643	rBV8	8842	19605	0.20%	0.019%
9	7.022	662	669	678	rVB	392769	624751	6.34%	0.621%
10	7.193	691	698	710	rVB	1700439	2611150	26.51%	2.597%
11	7.387	724	731	741	rBV	1515062	2357073	23.93%	2.344%
12	7.487	743	748	755	rVB9	10819	24151	0.25%	0.024%
13	7.857	803	811	818	rBV	1668699	2581328	26.20%	2.567%
14	7.928	818	823	829	rVB4	11447	23694	0.24%	0.024%
15	8.563	924	931	941	rBV	1103078	1778877	18.06%	1.769%
16	9.016	1001	1008	1016	rBV	1824014	2971331	30.16%	2.955%
17	9.451	1070	1082	1092	rVB	68265	138228	1.40%	0.137%
18	9.739	1122	1131	1143	rBV	1331885	2135644	21.68%	2.124%
19	10.275	1214	1222	1235	rBV	2243362	3686454	37.42%	3.666%
20	10.610	1272	1279	1280	rBV5	6111	11511	0.12%	0.011%
21	10.657	1280	1287	1298	rVB	2288639	3780352	38.38%	3.759%
22	10.792	1302	1310	1326	rBV	1548408	2660316	27.01%	2.646%
23	11.945	1500	1506	1514	rVB2	35756	61845	0.63%	0.062%
24	12.151	1536	1541	1549	rBV10	4340	11339	0.12%	0.011%
25	12.245	1551	1557	1563	rVB2	45500	76310	0.77%	0.076%
26	12.680	1626	1631	1634	rBV6	5514	10193	0.10%	0.010%
27	13.122	1701	1706	1711	rVB4	12658	22142	0.22%	0.022%
28	13.333	1738	1742	1748	rVB4	16926	25155	0.26%	0.025%
29	13.398	1748	1753	1759	rBV	67118	108018	1.10%	0.107%
30	13.463	1759	1764	1768	rBV6	9161	14486	0.15%	0.014%
31	13.910	1833	1840	1850	rBV	4512597	6249314	63.44%	6.215%
32	14.022	1858	1859	1866	rVB7	6126	9903	0.10%	0.010%
33	14.186	1876	1887	1899	rBV	5107822	7475729	75.89%	7.434%
34	14.404	1921	1924	1929	rVB7	8523	11343	0.12%	0.011%
35	14.492	1929	1939	1951	rBV	3383498	4988106	50.64%	4.961%
36	14.686	1966	1972	1984	rBV	185981	321780	3.27%	0.320%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018422.D
 Acq On : 28 Nov 2023 03:57
 Operator : MA/JU
 Sample : 05332-20
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	14.851	1995	2000	2005	rVV8	9552	14451	0.15%	0.014%
38	14.904	2005	2009	2016	rVB10	14423	25418	0.26%	0.025%
39	15.486	2101	2108	2120	rBV	6441148	9353074	94.95%	9.301%
40	15.598	2121	2127	2137	rVV	1165761	1588897	16.13%	1.580%
41	15.727	2145	2149	2153	rVB	27518	37139	0.38%	0.037%
42	16.269	2238	2241	2247	rVB7	12761	21177	0.21%	0.021%
43	17.021	2367	2369	2373	rBV4	10905	14247	0.14%	0.014%
44	17.245	2401	2407	2417	rVV	3550665	4988981	50.64%	4.961%
45	17.345	2417	2424	2436	rVV2	6439618	9165930	93.05%	9.115%
46	17.563	2457	2461	2466	rVB6	14036	24349	0.25%	0.024%
47	17.927	2520	2523	2528	rVB7	9904	11491	0.12%	0.011%
48	18.145	2555	2560	2570	rBV	229256	333083	3.38%	0.331%
49	18.457	2608	2613	2618	rBV7	17275	34031	0.35%	0.034%
50	18.604	2635	2638	2642	rBV3	18550	22830	0.23%	0.023%
51	19.168	2730	2734	2739	rVB	89318	112221	1.14%	0.112%
52	19.233	2741	2745	2750	rBV	76055	116024	1.18%	0.115%
53	19.398	2769	2773	2779	rBV	116471	143338	1.46%	0.143%
54	19.592	2801	2806	2815	rBV	7334059	9694722	98.41%	9.641%
55	21.162	3069	3073	3080	rBV6	111861	221465	2.25%	0.220%
56	21.392	3107	3112	3118	rBV	3214218	4249627	43.14%	4.226%
57	23.774	3507	3517	3530	rVB2	3862194	9850920	100.00%	9.796%
58	23.939	3537	3545	3564	rVB	1778876	4829347	49.02%	4.803%




Sum of corrected areas: 100556427

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018422.D
Acq On : 28 Nov 2023 03:57
Operator : MA/JU
Sample : 05332-20
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

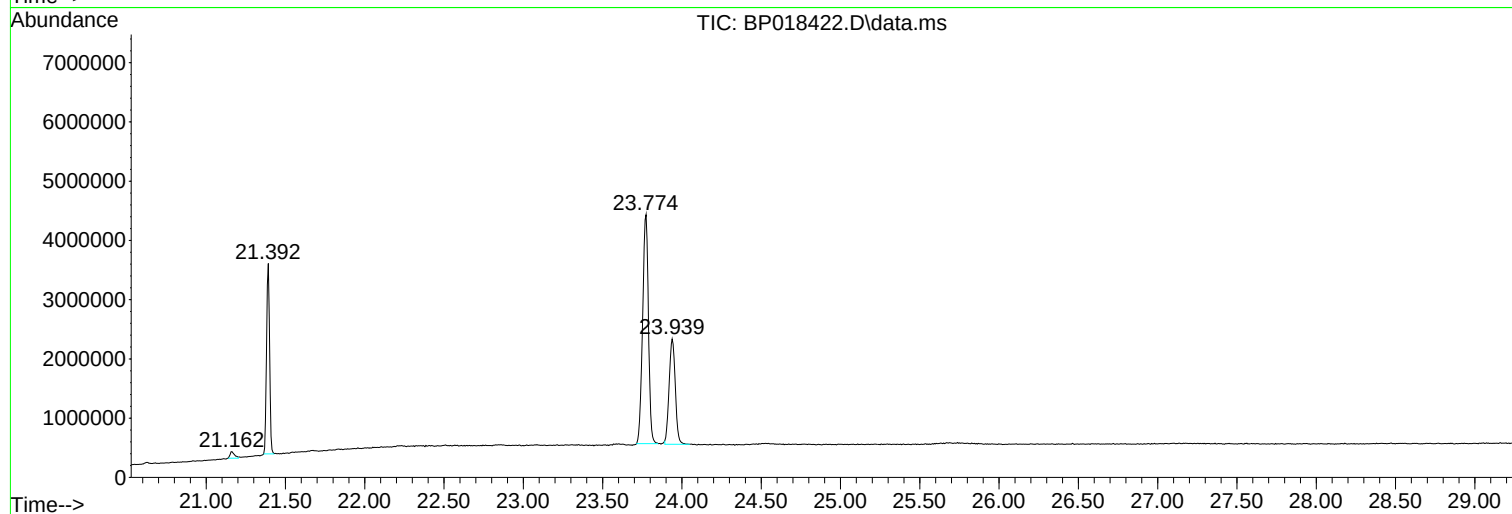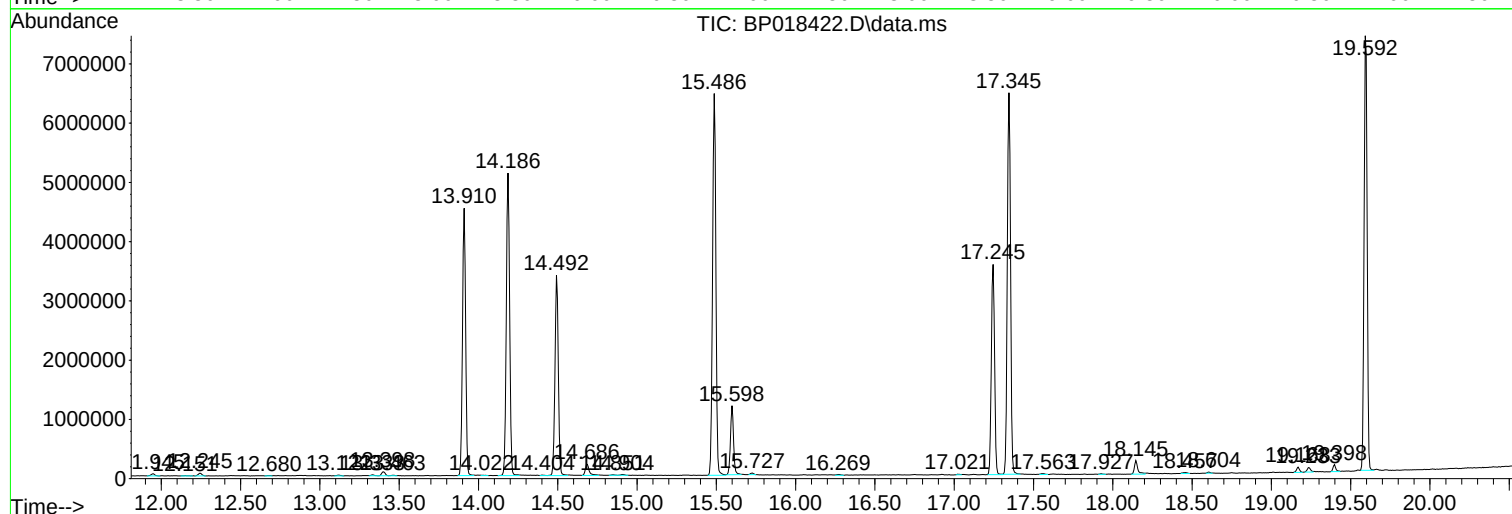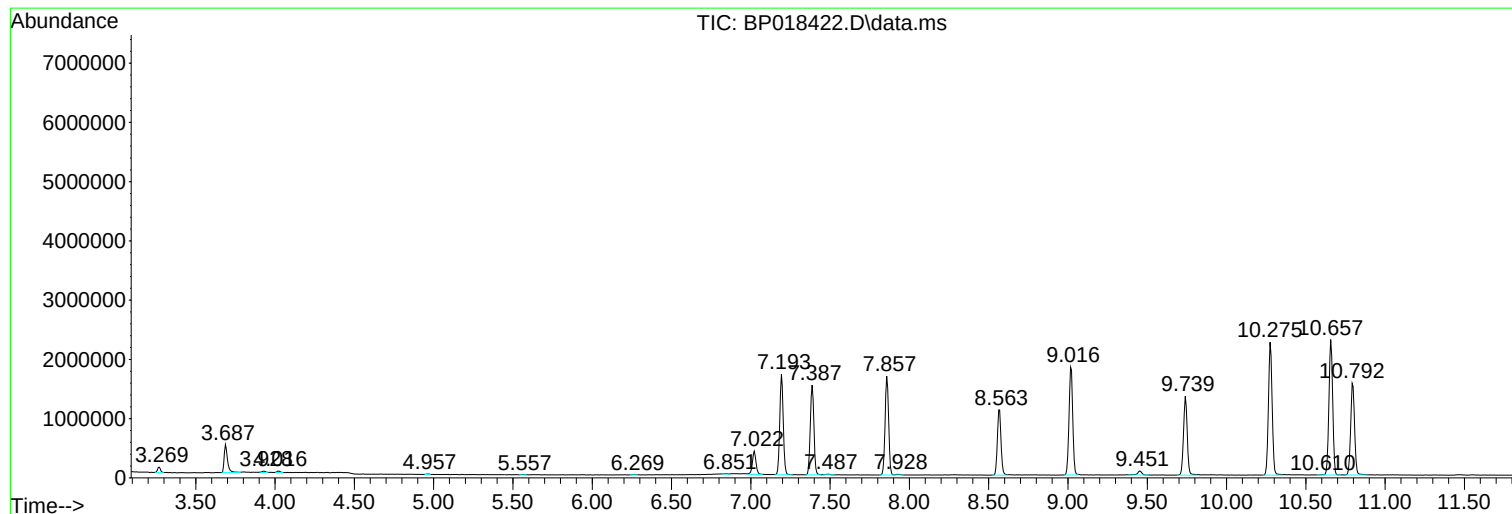

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018422.D
Acq On : 28 Nov 2023 03:57
Operator : MA/JU
Sample : 05332-20
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018422.D
Acq On : 28 Nov 2023 03:57
Operator : MA/JU
Sample : 05332-20
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc