

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018423.D
 Acq On : 28 Nov 2023 04:31
 Operator : MA/JU
 Sample : 05332-21
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018423.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	38	rVB	92810	120858	1.15%	0.137%
2	3.687	98	102	115	rBV	499341	732550	6.99%	0.828%
3	3.928	139	143	148	rVB2	26867	45896	0.44%	0.052%
4	4.023	155	159	163	rBV2	20711	28626	0.27%	0.032%
5	4.964	315	319	324	rVB6	9343	17347	0.17%	0.020%
6	5.558	414	420	426	rBV10	7330	13978	0.13%	0.016%
7	6.840	630	638	640	rBV9	9760	21870	0.21%	0.025%
8	7.022	663	669	680	rVB	374290	603170	5.76%	0.682%
9	7.193	690	698	707	rBV	1571347	2401402	22.92%	2.716%
10	7.387	724	731	741	rBV	1429800	2212299	21.11%	2.502%
11	7.481	744	747	755	rVB9	9695	20197	0.19%	0.023%
12	7.858	803	811	818	rBV	1287679	1992794	19.02%	2.254%
13	7.934	820	824	828	rVB5	7460	12805	0.12%	0.014%
14	8.563	925	931	943	rBV	1057088	1674536	15.98%	1.894%
15	9.016	1001	1008	1016	rBV	1667445	2718025	25.94%	3.074%
16	9.452	1076	1082	1089	rVB2	45843	84075	0.80%	0.095%
17	9.740	1120	1131	1142	rBV	1172947	1924286	18.37%	2.176%
18	10.275	1212	1222	1241	rBV	2004442	3308143	31.57%	3.741%
19	10.657	1279	1287	1294	rBV	1714812	2817710	26.89%	3.187%
20	10.793	1303	1310	1327	rBV	1397728	2398539	22.89%	2.713%
21	11.475	1416	1426	1430	rBV	7453	16670	0.16%	0.019%
22	11.946	1502	1506	1513	rVB2	27068	47824	0.46%	0.054%
23	12.246	1550	1557	1564	rBV	40493	66620	0.64%	0.075%
24	13.122	1701	1706	1710	rVB4	10446	15759	0.15%	0.018%
25	13.281	1728	1733	1738	rBV9	6382	11758	0.11%	0.013%
26	13.334	1738	1742	1746	rVV6	12952	18848	0.18%	0.021%
27	13.399	1746	1753	1760	rVV	45808	74338	0.71%	0.084%
28	13.463	1760	1764	1769	rVV7	6621	10953	0.10%	0.012%
29	13.910	1833	1840	1854	rBV	3870595	5403492	51.57%	6.111%
30	14.187	1877	1887	1897	rBV	4496336	6490707	61.95%	7.340%
31	14.493	1932	1939	1950	rBV	2444553	3556069	33.94%	4.022%
32	14.687	1966	1972	1982	rBV	185433	311598	2.97%	0.352%
33	14.840	1995	1998	2005	rVB9	6747	12705	0.12%	0.014%
34	14.910	2005	2010	2017	rVB9	14475	25379	0.24%	0.029%
35	15.487	2101	2108	2121	rBV	5698045	8127401	77.57%	9.191%
36	15.598	2121	2127	2137	rVV	1023875	1367937	13.06%	1.547%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018423.D
 Acq On : 28 Nov 2023 04:31
 Operator : MA/JU
 Sample : 05332-21
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGC9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	15.722	2145	2148	2161	rVB4	30409	55666	0.53%	0.063%
38	16.275	2238	2242	2245	rBV5	10196	15670	0.15%	0.018%
39	16.922	2348	2352	2357	rBV7	7467	11591	0.11%	0.013%
40	17.116	2382	2385	2389	rBV6	6793	11593	0.11%	0.013%
41	17.245	2400	2407	2417	rBV	2470789	3533033	33.72%	3.996%
42	17.345	2417	2424	2435	rVV	6086972	8159797	77.88%	9.228%
43	17.622	2468	2471	2474	rBV3	8508	11336	0.11%	0.013%
44	18.145	2555	2560	2570	rBV3	95559	146938	1.40%	0.166%
45	18.604	2635	2638	2643	rBV6	15398	22885	0.22%	0.026%
46	19.169	2730	2734	2739	rBV3	75126	100517	0.96%	0.114%
47	19.233	2741	2745	2750	rBV	69878	107007	1.02%	0.121%
48	19.398	2769	2773	2777	rBV4	54601	71297	0.68%	0.081%
49	19.592	2800	2806	2814	rBV	7087458	9278716	88.56%	10.494%
50	21.392	3107	3112	3119	rBV	2704123	3586854	34.23%	4.056%
51	23.774	3507	3517	3533	rVB2	4090297	10477615	100.00%	11.849%
52	23.945	3537	3546	3559	rVB	1518522	4125661	39.38%	4.666%




Sum of corrected areas: 88423340

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018423.D
Acq On : 28 Nov 2023 04:31
Operator : MA/JU
Sample : 05332-21
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

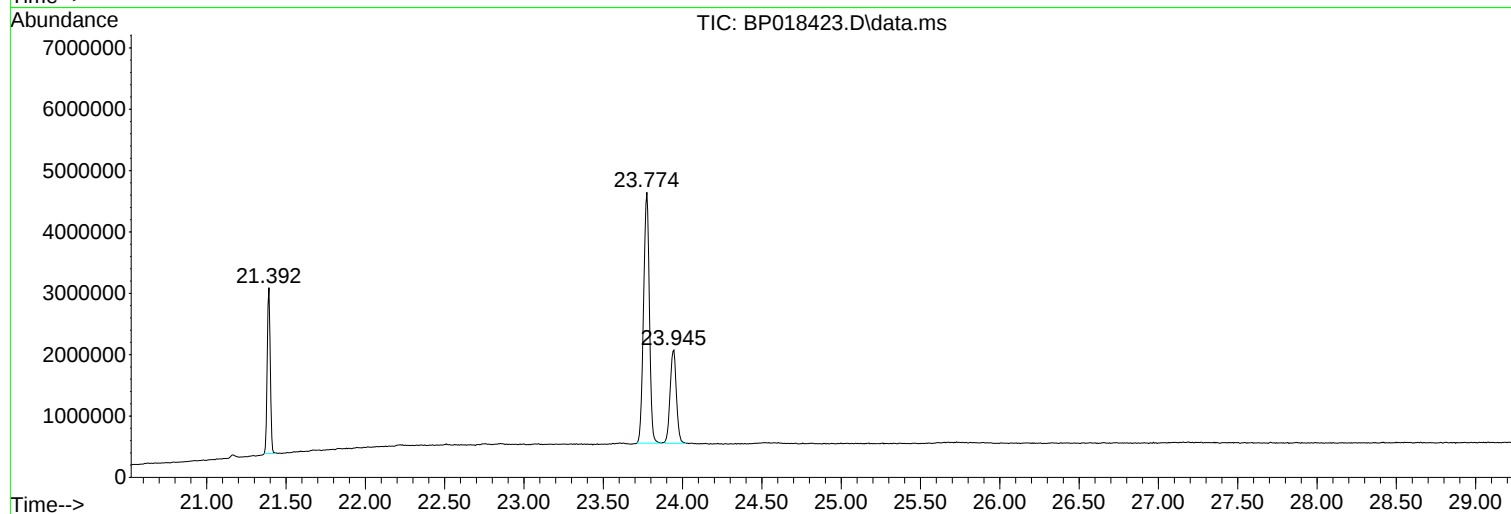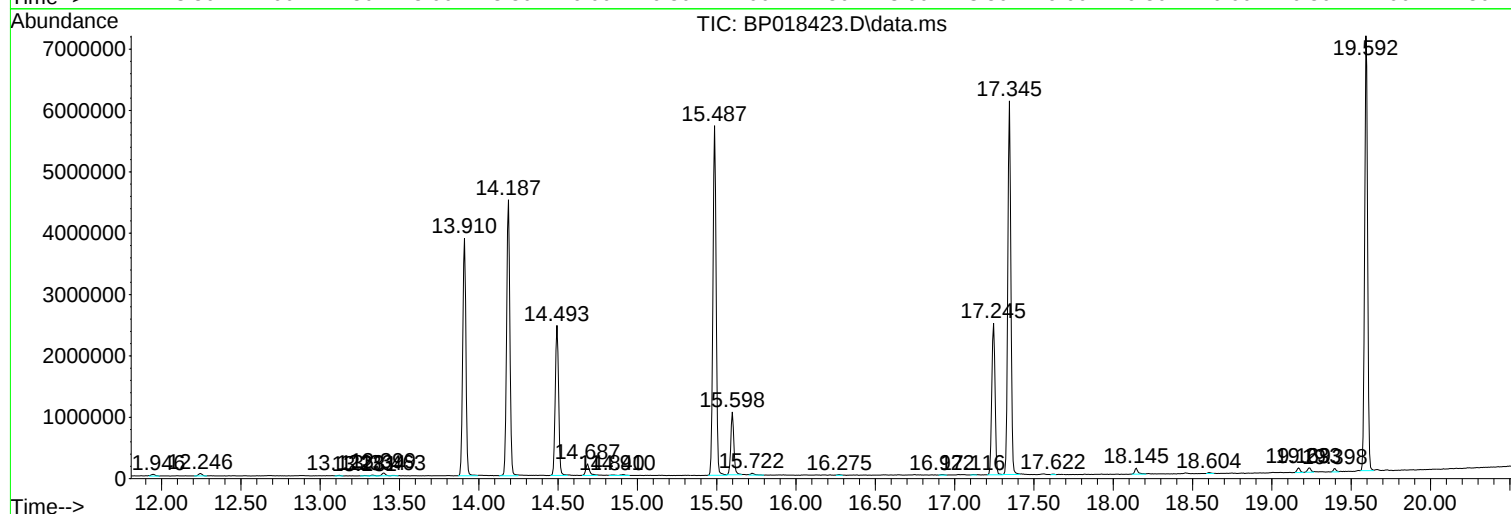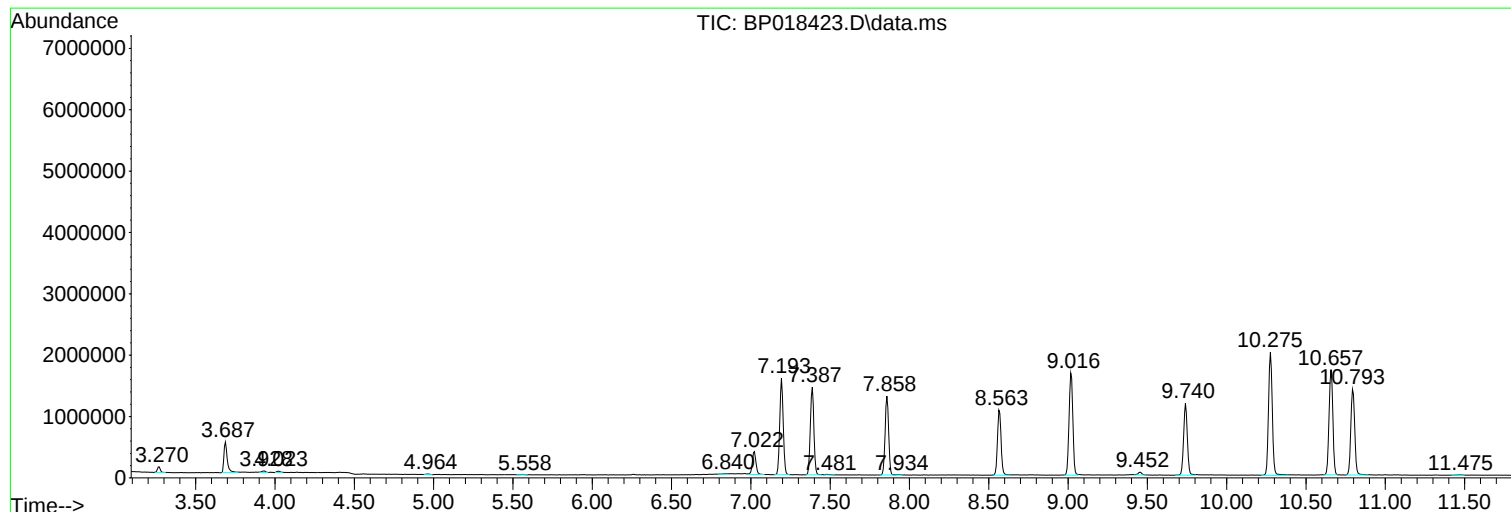

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018423.D
Acq On : 28 Nov 2023 04:31
Operator : MA/JU
Sample : 05332-21
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018423.D
Acq On : 28 Nov 2023 04:31
Operator : MA/JU
Sample : 05332-21
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
