

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018426.D
 Acq On : 28 Nov 2023 06:13
 Operator : MA/JU
 Sample : 05341-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	36	rBV	92995	120570	1.35%	0.127%
2	3.687	98	102	112	rBV	498410	715791	8.03%	0.751%
3	3.928	139	143	147	rVB	21239	34979	0.39%	0.037%
4	4.023	156	159	163	rVB	23400	31253	0.35%	0.033%
5	4.558	247	250	256	rVB8	8595	15248	0.17%	0.016%
6	7.022	661	669	680	rVB	376625	605012	6.78%	0.635%
7	7.193	691	698	709	rVB	1634525	2476440	27.76%	2.598%
8	7.387	724	731	742	rBV	1440353	2248367	25.21%	2.359%
9	7.487	742	748	754	rVB9	9933	21881	0.25%	0.023%
10	7.858	802	811	818	rBV	1697481	2598206	29.13%	2.726%
11	8.563	924	931	940	rBV	1145709	1781710	19.98%	1.869%
12	8.675	945	950	957	rVB7	9158	19791	0.22%	0.021%
13	9.016	1001	1008	1018	rBV	1761343	2813930	31.55%	2.952%
14	9.187	1033	1037	1041	rVB7	5974	9746	0.11%	0.010%
15	9.452	1078	1082	1092	rVB5	17867	38070	0.43%	0.040%
16	9.740	1119	1131	1139	rBV	1179356	1894945	21.25%	1.988%
17	10.275	1214	1222	1237	rBV	2080500	3431412	38.47%	3.600%
18	10.657	1279	1287	1295	rVB	2338178	3831734	42.96%	4.020%
19	10.793	1300	1310	1324	rBV	1759771	2971847	33.32%	3.118%
20	11.393	1409	1412	1415	rBV3	6741	9022	0.10%	0.009%
21	11.934	1499	1504	1507	rBV6	7714	12771	0.14%	0.013%
22	12.181	1541	1546	1550	rVB7	9150	15387	0.17%	0.016%
23	12.246	1552	1557	1564	rVB	42851	67186	0.75%	0.070%
24	12.875	1658	1664	1667	rBV8	4597	10662	0.12%	0.011%
25	13.122	1702	1706	1710	rVB4	5767	9593	0.11%	0.010%
26	13.398	1748	1753	1760	rBV4	24064	39223	0.44%	0.041%
27	13.910	1833	1840	1853	rBV	4059300	5626634	63.08%	5.903%
28	14.187	1878	1887	1901	rBV	4906517	7037060	78.90%	7.383%
29	14.493	1933	1939	1951	rVV	3538135	5171948	57.99%	5.426%
30	14.687	1965	1972	1984	rBV	142233	266322	2.99%	0.279%
31	14.845	1997	1999	2006	rVB8	5979	9472	0.11%	0.010%
32	14.910	2006	2010	2016	rVB8	9960	17449	0.20%	0.018%
33	15.487	2101	2108	2117	rBV	6106439	8780908	98.45%	9.213%
34	15.598	2121	2127	2141	rVV	927151	1302625	14.60%	1.367%
35	15.722	2145	2148	2156	rVB2	30678	51427	0.58%	0.054%
36	16.222	2230	2233	2239	rVB8	6168	9074	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018426.D
 Acq On : 28 Nov 2023 06:13
 Operator : MA/JU
 Sample : 05341-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	16.275	2239	2242	2245	rVB5	6928	9728	0.11%	0.010%
38	16.440	2266	2270	2273	rVB6	7173	10031	0.11%	0.011%
39	16.640	2301	2304	2311	rVV9	4360	9080	0.10%	0.010%
40	16.745	2316	2322	2326	rBV8	8215	17238	0.19%	0.018%
41	16.922	2347	2352	2356	rVB7	10472	14209	0.16%	0.015%
42	17.028	2367	2370	2374	rBV4	6668	9919	0.11%	0.010%
43	17.245	2400	2407	2417	rBV	3775248	5364305	60.14%	5.628%
44	17.345	2417	2424	2435	rVV	6373537	8804878	98.72%	9.238%
45	18.145	2554	2560	2567	rBV10	27942	58630	0.66%	0.062%
46	19.169	2729	2734	2738	rBV	72976	97776	1.10%	0.103%
47	19.233	2741	2745	2750	rBV	64283	92118	1.03%	0.097%
48	19.398	2770	2773	2776	rBV3	22156	25499	0.29%	0.027%
49	19.592	2800	2806	2816	rBV	6801616	8919425	100.00%	9.358%
50	21.392	3107	3112	3121	rBV	3349644	4447681	49.87%	4.666%
51	23.780	3508	3518	3533	rVB	3280212	8459943	94.85%	8.876%
52	23.951	3538	3547	3561	rVB2	1782096	4872783	54.63%	5.113%




Sum of corrected areas: 95310938

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018426.D
Acq On : 28 Nov 2023 06:13
Operator : MA/JU
Sample : 05341-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

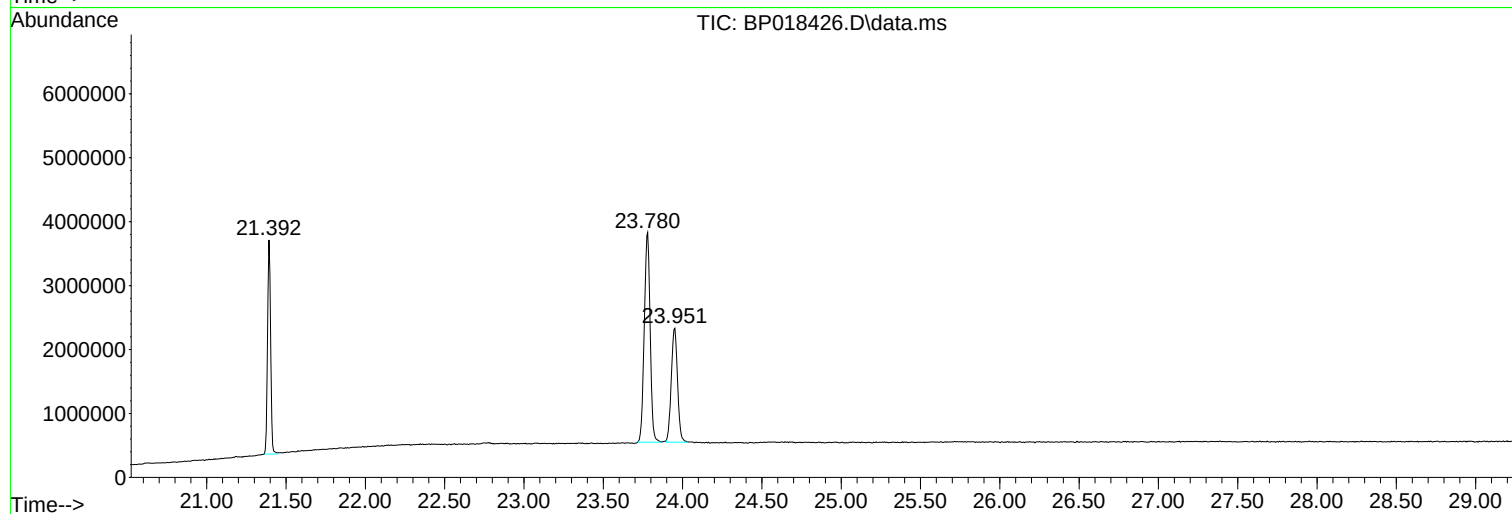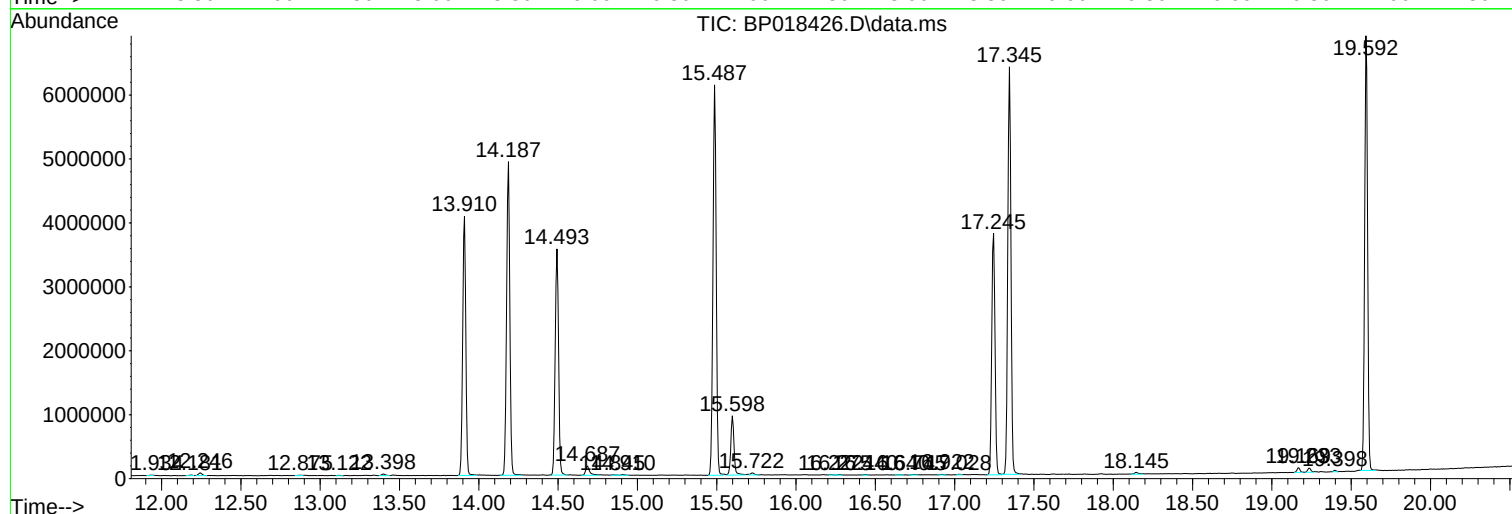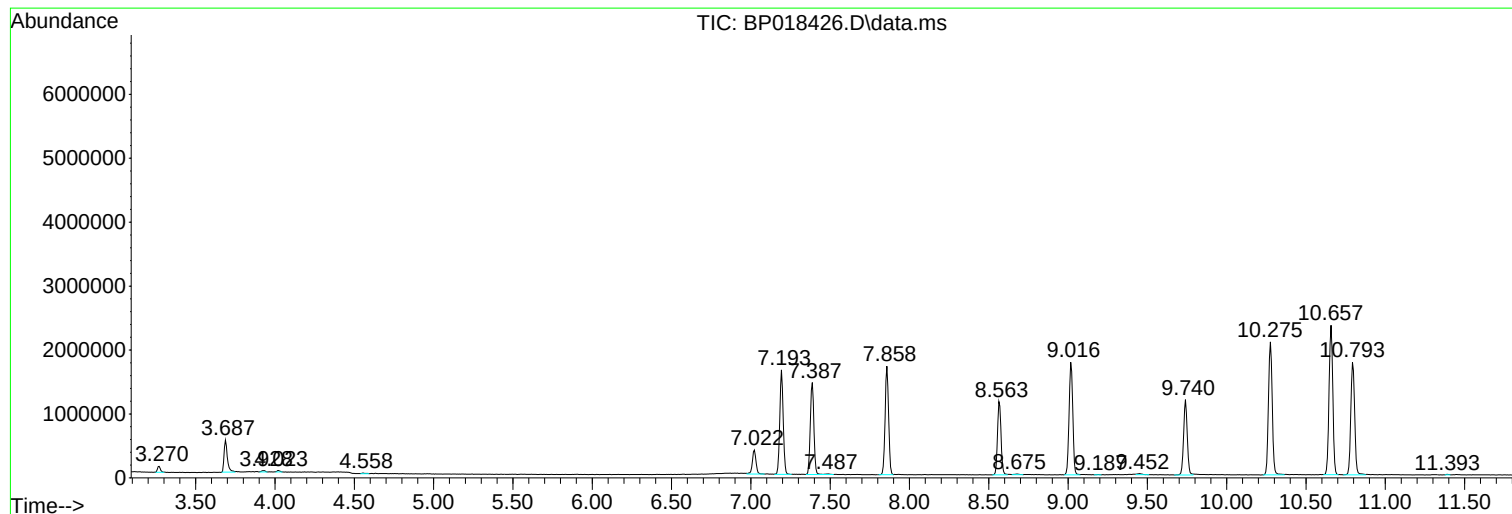

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018426.D
Acq On : 28 Nov 2023 06:13
Operator : MA/JU
Sample : 05341-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018426.D
Acq On : 28 Nov 2023 06:13
Operator : MA/JU
Sample : 05341-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc