

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018429.D
 Acq On : 28 Nov 2023 07:54
 Operator : MA/JU
 Sample : PB157282BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK282

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	39	rVB	152762	199489	1.81%	0.167%
2	3.681	97	101	118	rBV	1911794	2786197	25.26%	2.333%
3	4.022	155	159	164	rVB2	25617	35288	0.32%	0.030%
4	7.022	662	669	682	rVB	2211251	3388128	30.72%	2.837%
5	7.193	691	698	708	rVB	1901520	2880876	26.12%	2.412%
6	7.387	724	731	742	rBV	2244440	3548372	32.17%	2.971%
7	7.858	804	811	819	rVB	1514958	2355213	21.35%	1.972%
8	8.569	923	932	942	rBV	2820097	4475668	40.58%	3.748%
9	9.016	1001	1008	1021	rBV	2055829	3331347	30.21%	2.790%
10	9.740	1119	1131	1143	rBV	1633495	2592535	23.51%	2.171%
11	10.275	1213	1222	1240	rBV	2920286	4676957	42.41%	3.916%
12	10.657	1280	1287	1295	rVB	2114720	3485710	31.61%	2.919%
13	10.793	1302	1310	1329	rBV	2748980	4764545	43.20%	3.990%
14	11.940	1500	1505	1513	rBV9	7334	19955	0.18%	0.017%
15	12.240	1549	1556	1564	rVB	59077	101248	0.92%	0.085%
16	13.287	1728	1734	1737	rBV7	5797	12863	0.12%	0.011%
17	13.398	1745	1753	1759	rBV5	23087	44113	0.40%	0.037%
18	13.457	1759	1763	1772	rVB6	9409	19817	0.18%	0.017%
19	13.910	1833	1840	1850	rBV	5099740	6943962	62.96%	5.815%
20	14.010	1853	1857	1863	rVB6	8333	12837	0.12%	0.011%
21	14.187	1878	1887	1901	rBV2	5783401	8599140	77.97%	7.201%
22	14.492	1930	1939	1949	rBV	3286050	4734753	42.93%	3.965%
23	14.687	1965	1972	1988	rBV	1513111	2308311	20.93%	1.933%
24	14.904	2006	2009	2014	rBV7	9031	11723	0.11%	0.010%
25	15.487	2101	2108	2120	rBV	7255579	10244096	92.88%	8.578%
26	15.598	2121	2127	2140	rVV	1313311	1782179	16.16%	1.492%
27	15.728	2144	2149	2154	rVB	34196	57054	0.52%	0.048%
28	16.269	2239	2241	2246	rVB6	10329	14109	0.13%	0.012%
29	16.922	2349	2352	2356	rVB6	10942	15935	0.14%	0.013%
30	17.034	2367	2371	2379	rVB5	7432	15098	0.14%	0.013%
31	17.245	2401	2407	2414	rBV	3436986	4840006	43.88%	4.053%
32	17.345	2417	2424	2436	rVV2	6860325	9910948	89.86%	8.299%
33	17.622	2465	2471	2475	rBV4	11432	19024	0.17%	0.016%
34	17.828	2502	2506	2510	rBV6	7346	11346	0.10%	0.010%
35	18.145	2557	2560	2564	rBV6	21103	27117	0.25%	0.023%
36	19.169	2730	2734	2739	rBV2	82182	112215	1.02%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018429.D
Acq On : 28 Nov 2023 07:54
Operator : MA/JU
Sample : PB157282BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK282

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	19.233	2741	2745	2752	rBV	80333	125047	1.13%	0.105%
38	19.398	2770	2773	2779	rVB6	29032	37568	0.34%	0.031%
39	19.551	2797	2799	2801	rBV3	16231	12604	0.11%	0.011%
40	19.598	2801	2807	2816	rVB	7647461	10341376	93.77%	8.660%
41	21.398	3107	3113	3123	rBV	3269683	4509374	40.89%	3.776%
42	23.792	3510	3520	3533	rVB2	4110331	11028972	100.00%	9.236%
43	23.963	3540	3549	3563	rVB	1758109	4985880	45.21%	4.175%




Sum of corrected areas: 119418995

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018429.D
Acq On : 28 Nov 2023 07:54
Operator : MA/JU
Sample : PB157282BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK282

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

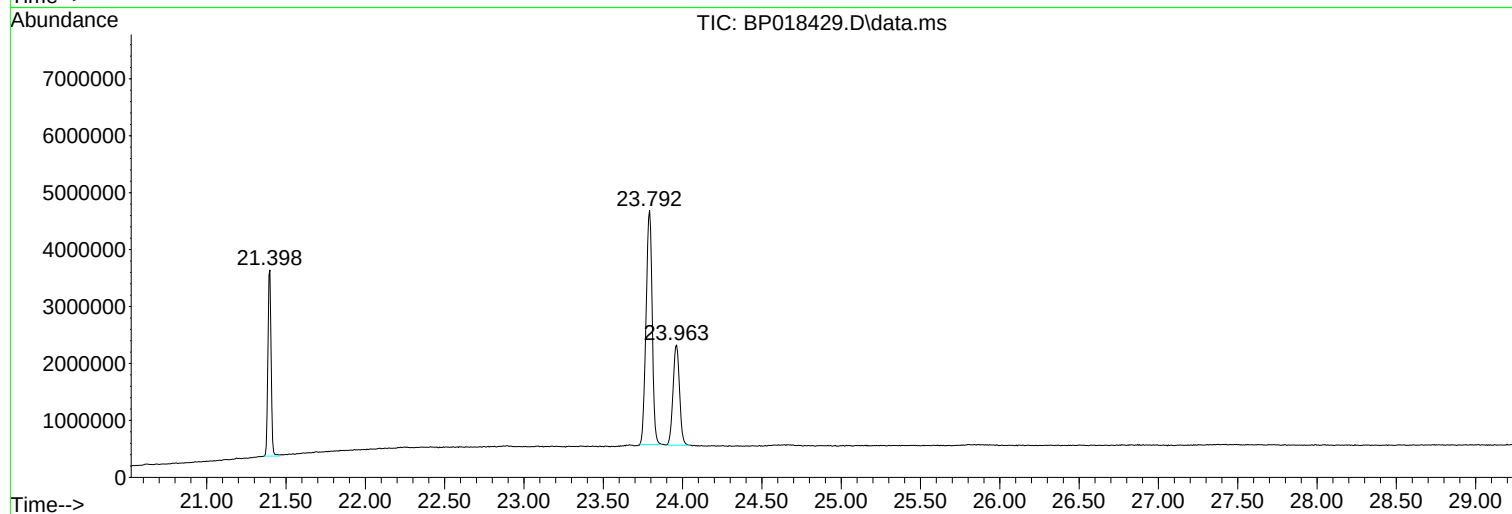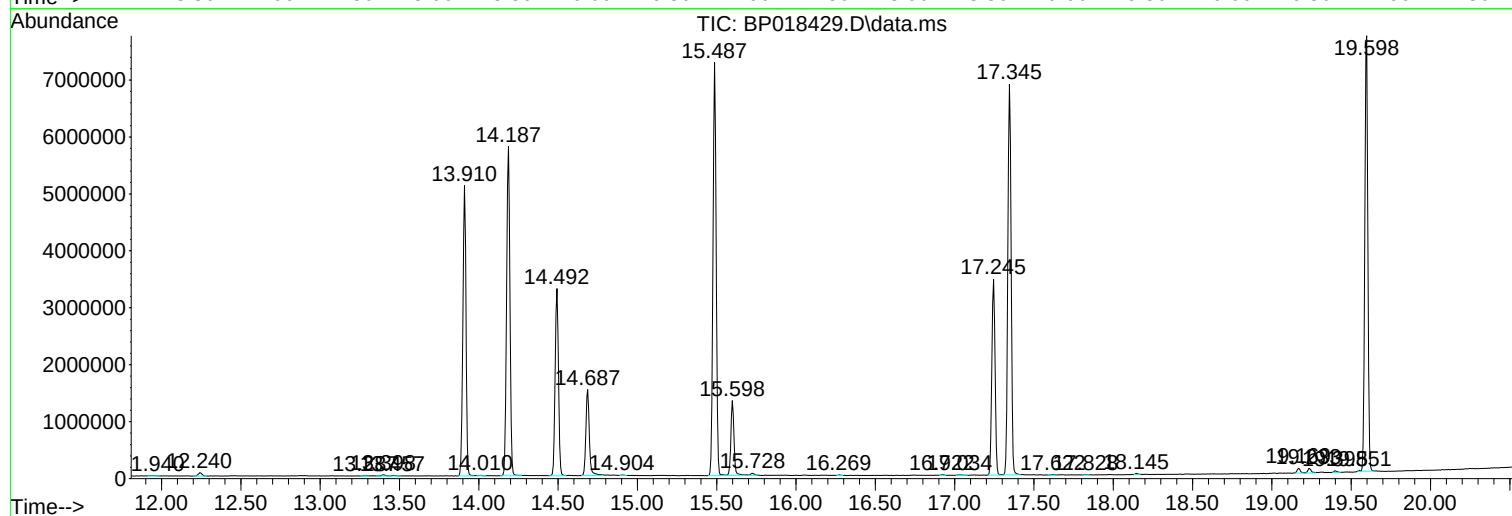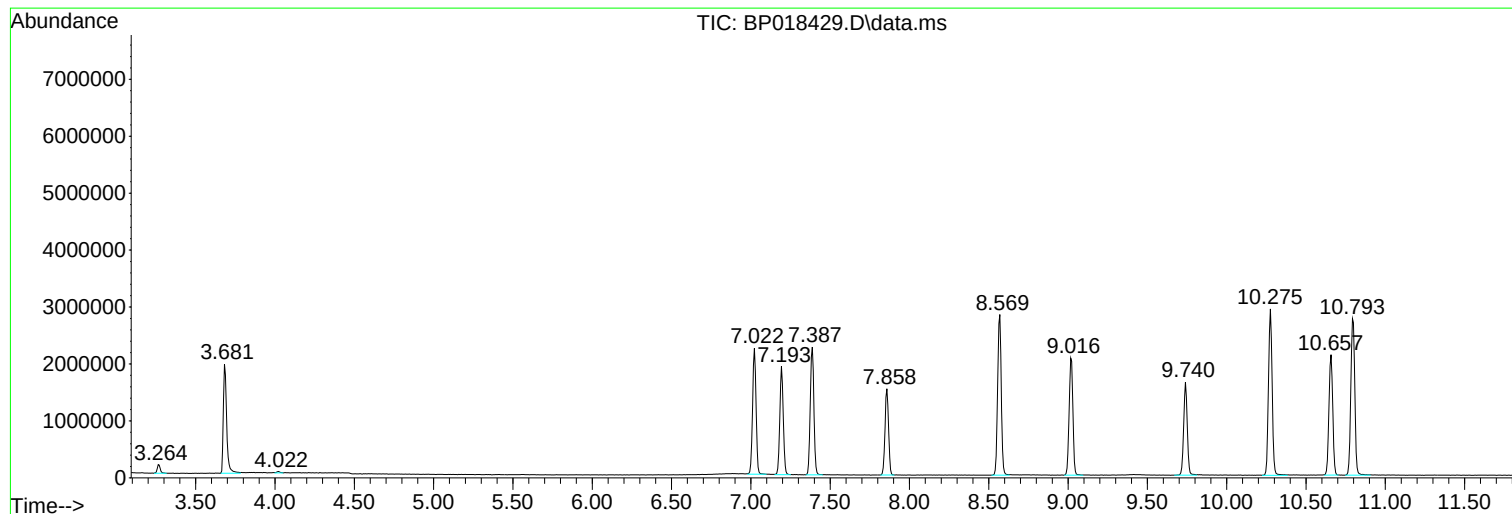

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018429.D
Acq On : 28 Nov 2023 07:54
Operator : MA/JU
Sample : PB157282BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK282

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018429.D
Acq On : 28 Nov 2023 07:54
Operator : MA/JU
Sample : PB157282BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK282

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------