

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018431.D
 Acq On : 28 Nov 2023 09:38
 Operator : MA/JU
 Sample : PB157287BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK287

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	39	rVB	106729	144399	1.90%	0.163%
2	3.681	96	101	114	rBV	1195039	1757185	23.14%	1.987%
3	4.017	155	158	163	rVB	19665	24581	0.32%	0.028%
4	7.017	662	668	676	rVB	1548094	2351597	30.97%	2.659%
5	7.187	691	697	705	rVB	1288631	2016126	26.55%	2.279%
6	7.381	723	730	739	rBV	1575783	2475265	32.60%	2.798%
7	7.852	804	810	822	rVB	1336747	2096765	27.61%	2.371%
8	8.564	922	931	947	rBV	1999025	3176933	41.84%	3.592%
9	9.016	1000	1008	1021	rBV	1430234	2319121	30.54%	2.622%
10	9.740	1121	1131	1147	rBV	1047297	1748155	23.02%	1.976%
11	10.275	1214	1222	1236	rBV	1985933	3325179	43.79%	3.759%
12	10.658	1279	1287	1298	rVB	1880107	3200459	42.15%	3.618%
13	10.793	1302	1310	1328	rBV	1784063	2987447	39.34%	3.377%
14	11.934	1497	1504	1509	rBV8	11064	26025	0.34%	0.029%
15	12.246	1550	1557	1566	rVB	39920	72434	0.95%	0.082%
16	12.681	1624	1631	1633	rBV7	4996	10691	0.14%	0.012%
17	13.069	1692	1697	1703	rBV10	3947	8456	0.11%	0.010%
18	13.399	1747	1753	1759	rBV4	28344	47193	0.62%	0.053%
19	13.799	1814	1821	1823	rBV6	4701	7945	0.10%	0.009%
20	13.910	1832	1840	1851	rBV	3443721	4986153	65.66%	5.637%
21	14.187	1879	1887	1897	rBV	4215097	6174556	81.31%	6.981%
22	14.493	1932	1939	1951	rBV	3021565	4462300	58.76%	5.045%
23	14.681	1964	1971	1989	rBV	930040	1528005	20.12%	1.728%
24	14.904	2005	2009	2014	rVB8	6160	12233	0.16%	0.014%
25	15.487	2101	2108	2117	rBV	5219183	7592625	99.98%	8.584%
26	15.598	2121	2127	2136	rVV	826221	1114047	14.67%	1.259%
27	15.722	2143	2148	2155	rVB3	26931	47151	0.62%	0.053%
28	16.275	2238	2242	2246	rVB7	7771	9912	0.13%	0.011%
29	16.740	2319	2321	2327	rBV6	7397	10879	0.14%	0.012%
30	16.922	2349	2352	2357	rVB7	7415	12513	0.16%	0.014%
31	17.028	2367	2370	2376	rVB4	6296	8428	0.11%	0.010%
32	17.245	2400	2407	2417	rBV	3467030	4768907	62.80%	5.392%
33	17.345	2417	2424	2441	rVV	5217016	7497271	98.73%	8.476%
34	17.628	2468	2472	2475	rBV5	6548	8457	0.11%	0.010%
35	19.169	2730	2734	2740	rVB2	62431	82732	1.09%	0.094%
36	19.239	2742	2746	2751	rBV	53663	75694	1.00%	0.086%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018431.D
Acq On : 28 Nov 2023 09:38
Operator : MA/JU
Sample : PB157287BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK287

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	19.598	2801	2807	2815	rBV	5936348	7593863	100.00%	8.585%
38	21.398	3108	3113	3120	rBV	2873337	3792841	49.95%	4.288%
39	23.798	3512	3521	3537	rVB	2523332	6765608	89.09%	7.649%
40	23.969	3542	3550	3571	rVB2	1444147	4111420	54.14%	4.648%




Sum of corrected areas: 88451551

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018431.D
Acq On : 28 Nov 2023 09:38
Operator : MA/JU
Sample : PB157287BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

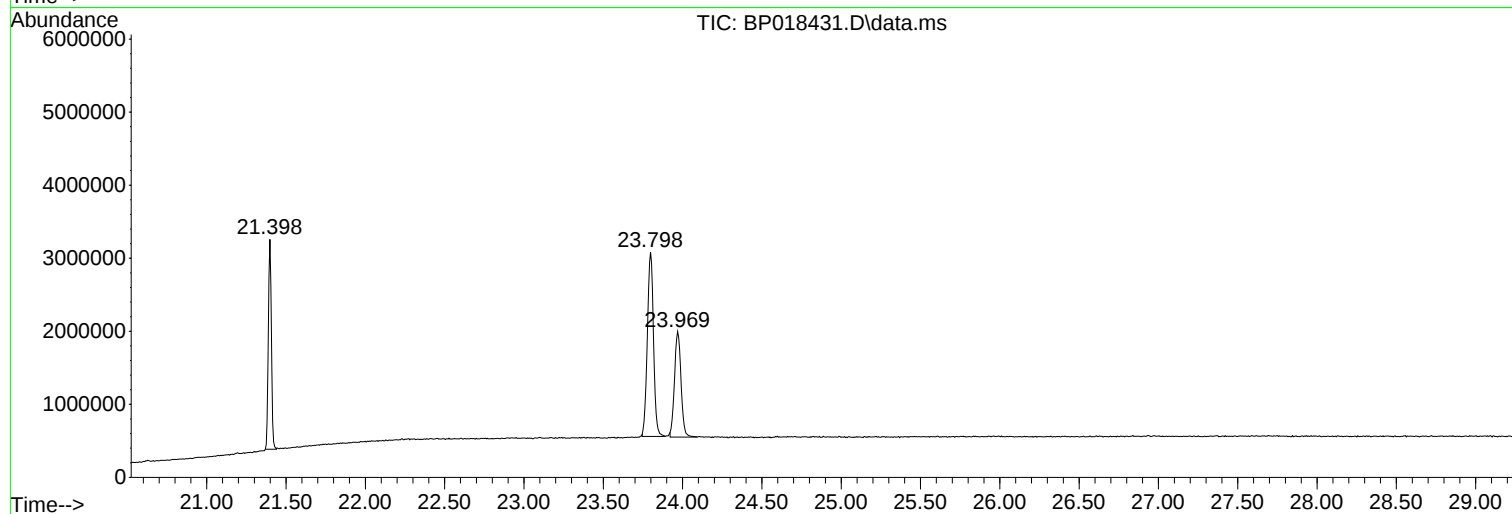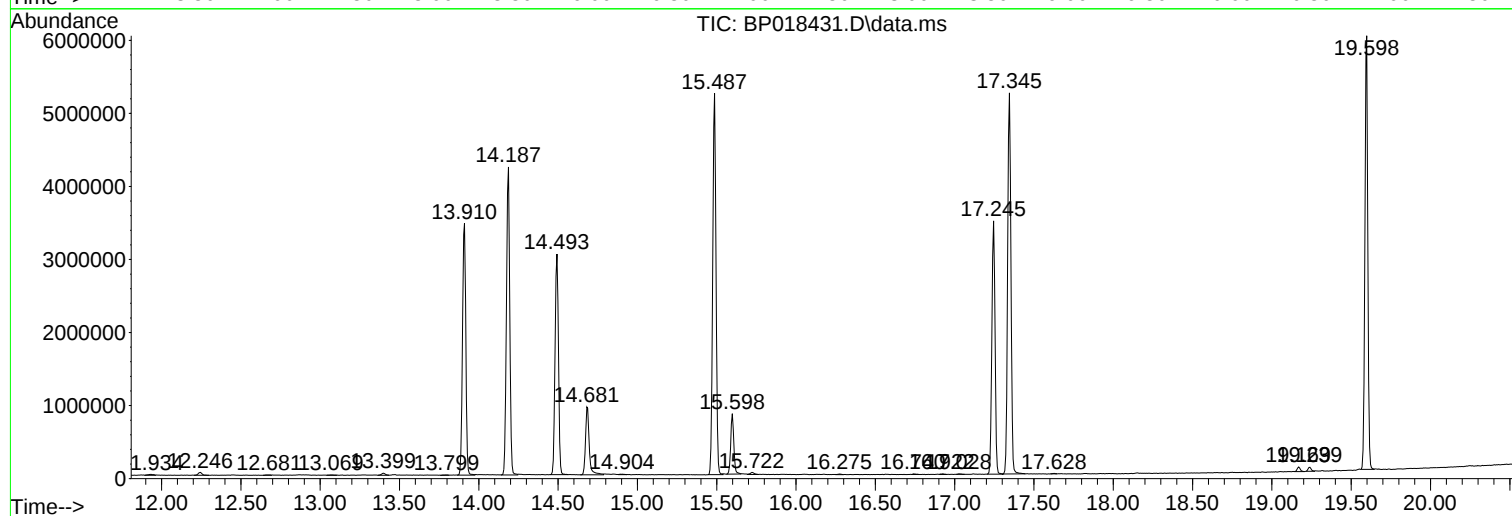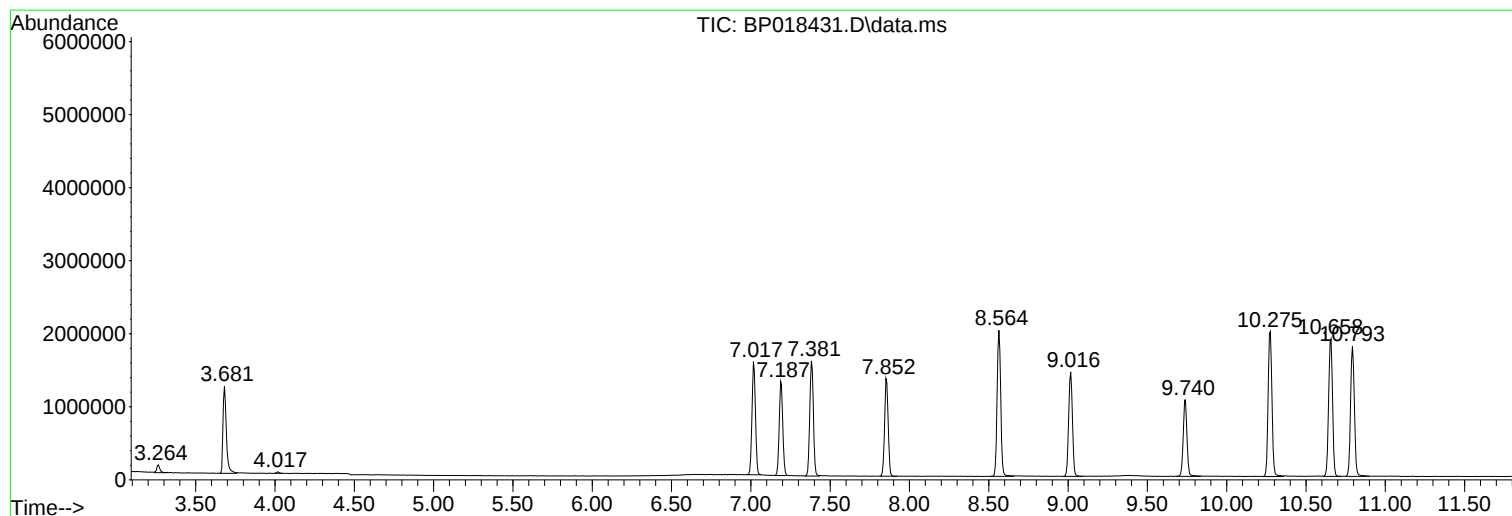

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018431.D
Acq On : 28 Nov 2023 09:38
Operator : MA/JU
Sample : PB157287BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018431.D
Acq On : 28 Nov 2023 09:38
Operator : MA/JU
Sample : PB157287BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------