

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018432.D
 Acq On : 28 Nov 2023 10:12
 Operator : MA/JU
 Sample : PB157193BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK193

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	26	31	40	rVB	129055	183677	1.76%	0.163%
2	3.681	97	101	116	rBV	1671490	2542012	24.42%	2.249%
3	4.022	155	159	165	rVB2	24445	35147	0.34%	0.031%
4	7.022	662	669	679	rVB	1978852	3058758	29.39%	2.706%
5	7.193	691	698	706	rVB	1713114	2576553	24.75%	2.280%
6	7.387	724	731	744	rBV	2022821	3170598	30.46%	2.805%
7	7.858	803	811	822	rVB	1496902	2342728	22.51%	2.073%
8	8.563	924	931	943	rBV	2517856	4093108	39.32%	3.622%
9	9.016	999	1008	1017	rBV	1885541	3025735	29.07%	2.677%
10	9.410	1069	1075	1077	rBV7	6816	12353	0.12%	0.011%
11	9.740	1118	1131	1144	rBV	1381490	2286089	21.96%	2.023%
12	10.275	1214	1222	1239	rBV	2581972	4308140	41.39%	3.812%
13	10.657	1279	1287	1296	rVB	2179187	3592448	34.51%	3.179%
14	10.793	1302	1310	1326	rBV	2624930	4467277	42.92%	3.953%
15	12.240	1551	1556	1562	rVB	52057	85297	0.82%	0.075%
16	12.669	1623	1629	1637	rBV	4071	13536	0.13%	0.012%
17	13.275	1730	1732	1739	rVB7	6427	11203	0.11%	0.010%
18	13.398	1748	1753	1761	rVV3	31349	52014	0.50%	0.046%
19	13.463	1761	1764	1772	rVB9	9057	15427	0.15%	0.014%
20	13.910	1832	1840	1850	rBV	4785215	6588634	63.30%	5.830%
21	14.187	1879	1887	1899	rBV	5522155	8118500	78.00%	7.183%
22	14.493	1932	1939	1948	rBV	3532588	5042768	48.45%	4.462%
23	14.687	1965	1972	1988	rBV	1462244	2181723	20.96%	1.930%
24	14.904	2006	2009	2013	rVB6	7478	10449	0.10%	0.009%
25	15.487	2100	2108	2121	rBV	7081694	9994148	96.02%	8.843%
26	15.598	2121	2127	2143	rVV	1220155	1675365	16.10%	1.482%
27	15.728	2143	2149	2154	rVB	33466	61452	0.59%	0.054%
28	16.051	2198	2204	2206	rBV7	9073	12685	0.12%	0.011%
29	16.922	2348	2352	2359	rVB9	9076	17142	0.16%	0.015%
30	17.028	2367	2370	2375	rBV4	10423	15118	0.15%	0.013%
31	17.245	2400	2407	2416	rBV	4009811	5545346	53.28%	4.906%
32	17.345	2417	2424	2438	rVB	7193738	10029829	96.36%	8.874%
33	17.622	2467	2471	2476	rBV4	10523	14458	0.14%	0.013%
34	19.169	2729	2734	2739	rBV2	86153	116361	1.12%	0.103%
35	19.233	2741	2745	2750	rBV	75477	101929	0.98%	0.090%
36	19.598	2801	2807	2818	rBV	7823424	10408456	100.00%	9.209%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018432.D
Acq On : 28 Nov 2023 10:12
Operator : MA/JU
Sample : PB157193BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK193

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	21.398	3108	3113	3120	rBV	3263328	4334693	41.65%	3.835%
38	23.804	3513	3522	3540	rVB	3126299	8477525	81.45%	7.501%
39	23.974	3543	3551	3569	rVB2	1505397	4401740	42.29%	3.895%




Sum of corrected areas: 113020421

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018432.D
Acq On : 28 Nov 2023 10:12
Operator : MA/JU
Sample : PB157193BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

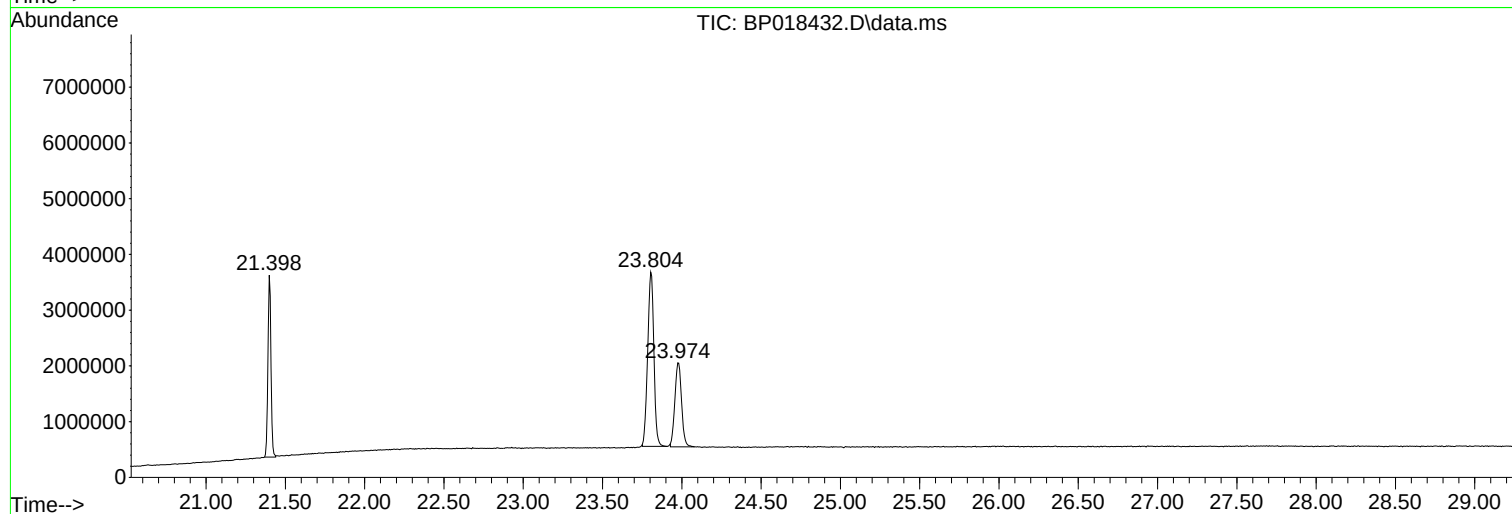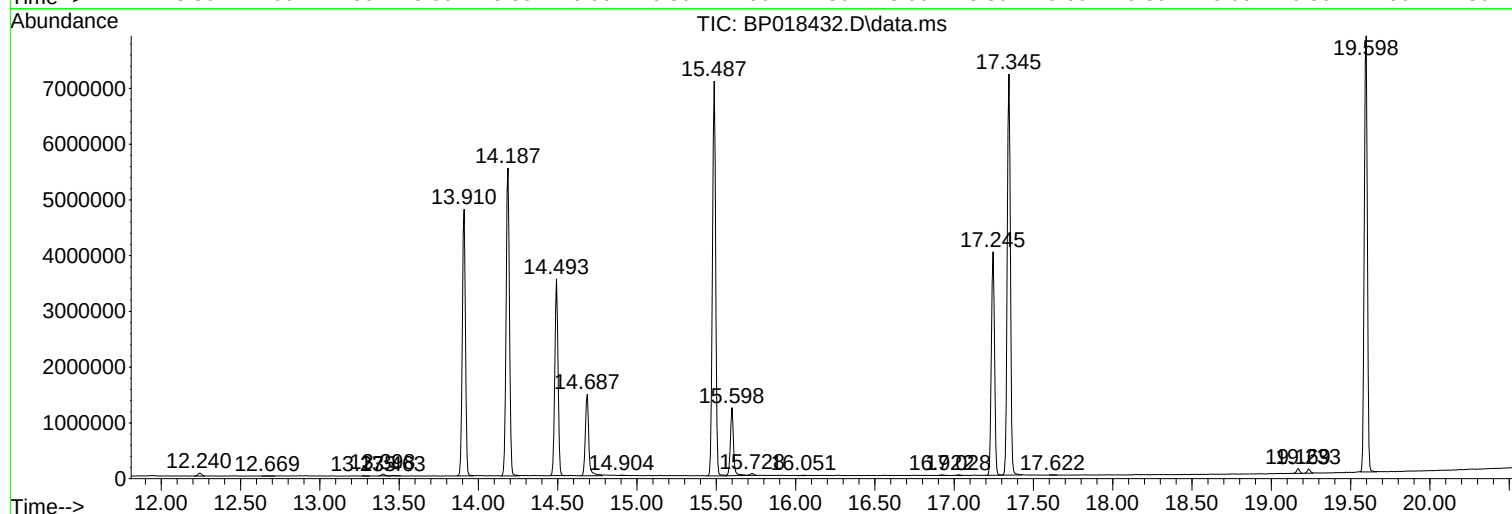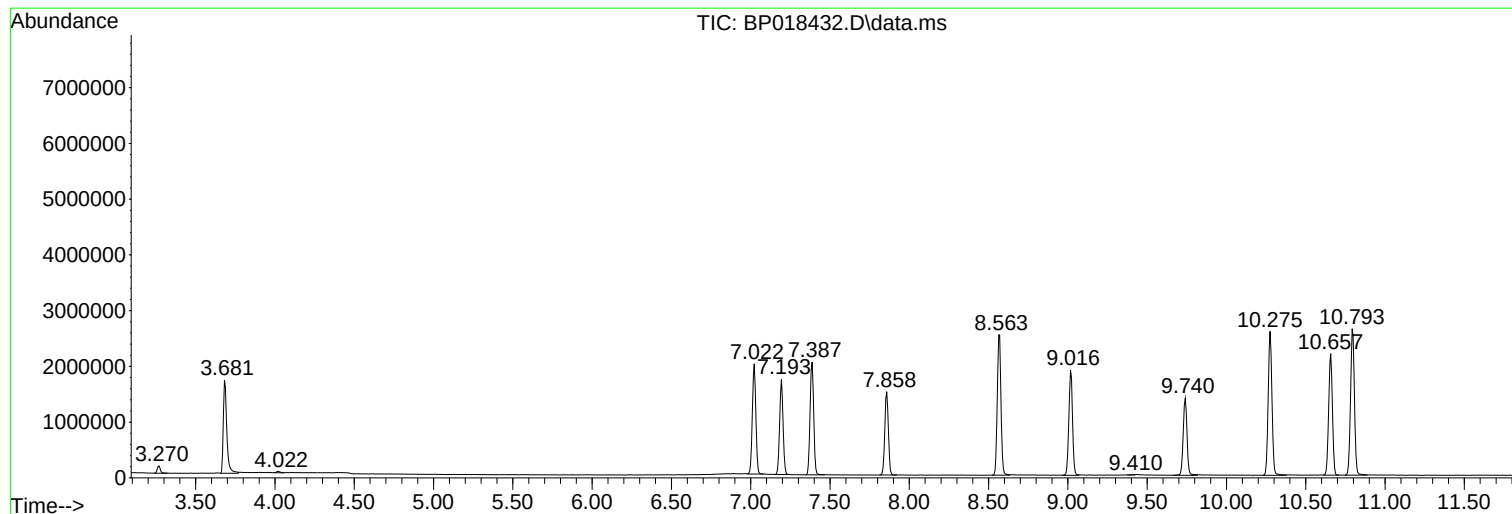

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018432.D
Acq On : 28 Nov 2023 10:12
Operator : MA/JU
Sample : PB157193BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018432.D
Acq On : 28 Nov 2023 10:12
Operator : MA/JU
Sample : PB157193BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------