

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018441.D
 Acq On : 28 Nov 2023 15:17
 Operator : MA/JU
 Sample : 05416-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	37	rVB	44865	61536	1.42%	0.138%
2	3.687	99	102	111	rBV	129245	203435	4.69%	0.457%
3	3.799	118	121	125	rVB2	27122	31556	0.73%	0.071%
4	3.928	138	143	150	rVB2	38980	64924	1.50%	0.146%
5	4.017	155	158	163	rVB	35803	45465	1.05%	0.102%
6	4.587	250	255	258	rBV6	7285	12708	0.29%	0.029%
7	4.952	312	317	326	rVB2	49774	91193	2.10%	0.205%
8	5.834	463	467	470	rVV6	8505	14618	0.34%	0.033%
9	5.869	470	473	476	rVB5	9443	12149	0.28%	0.027%
10	6.534	582	586	593	rVB10	8046	17828	0.41%	0.040%
11	6.840	633	638	643	rBV6	14447	31085	0.72%	0.070%
12	7.016	660	668	682	rVB	567610	1013319	23.36%	2.276%
13	7.187	691	697	705	rBV	513783	795512	18.34%	1.787%
14	7.381	724	730	739	rBV	584903	918967	21.18%	2.064%
15	7.464	740	744	755	rVB3	30638	77729	1.79%	0.175%
16	7.675	773	780	783	rBV7	6536	11181	0.26%	0.025%
17	7.858	804	811	818	rBV	1365575	2176084	50.16%	4.887%
18	7.922	818	822	825	rVV6	8168	10878	0.25%	0.024%
19	8.563	924	931	942	rBV	509046	794039	18.30%	1.783%
20	8.681	945	951	959	rVV	228598	372923	8.60%	0.838%
21	8.805	966	972	979	rVV2	18770	46471	1.07%	0.104%
22	9.016	1000	1008	1015	rVV	510219	840645	19.38%	1.888%
23	9.099	1019	1022	1025	rVV5	10161	17968	0.41%	0.040%
24	9.122	1025	1026	1033	rVB6	10583	13151	0.30%	0.030%
25	9.187	1033	1037	1041	rBV6	10982	17486	0.40%	0.039%
26	9.446	1079	1081	1087	rVV6	9749	15639	0.36%	0.035%
27	9.734	1116	1130	1139	rBV	320989	585330	13.49%	1.315%
28	9.875	1148	1154	1160	rBV	37989	66541	1.53%	0.149%
29	10.099	1186	1192	1198	rVV2	36491	63777	1.47%	0.143%
30	10.275	1214	1222	1233	rBV	635066	1071636	24.70%	2.407%
31	10.652	1278	1286	1293	rBV	1784132	3091413	71.27%	6.943%
32	10.793	1300	1310	1323	rBV	341311	616080	14.20%	1.384%
33	11.193	1372	1378	1387	rVV8	20268	40287	0.93%	0.090%
34	11.440	1415	1420	1428	rVV	19170	36447	0.84%	0.082%
35	11.693	1459	1463	1466	rBV5	11941	16648	0.38%	0.037%
36	11.940	1500	1505	1509	rBV6	6187	11693	0.27%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018441.D
 Acq On : 28 Nov 2023 15:17
 Operator : MA/JU
 Sample : 05416-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	12.022	1513	1519	1523	rVB4	11377	19955	0.46%	0.045%
38	12.087	1525	1530	1535	rBV5	12171	16986	0.39%	0.038%
39	12.240	1549	1556	1562	rVB3	15466	29746	0.69%	0.067%
40	12.316	1565	1569	1573	rBV2	18233	26874	0.62%	0.060%
41	12.528	1601	1605	1610	rVB2	13205	22018	0.51%	0.049%
42	12.863	1658	1662	1666	rBV7	6627	11033	0.25%	0.025%
43	13.328	1736	1741	1745	rVV3	18181	22932	0.53%	0.052%
44	13.398	1745	1753	1761	rVV	184429	299689	6.91%	0.673%
45	13.651	1789	1796	1797	rBV7	7406	11795	0.27%	0.026%
46	13.816	1819	1824	1829	rBV6	21131	37176	0.86%	0.083%
47	13.904	1834	1839	1849	rVV	1147500	1522107	35.09%	3.418%
48	13.993	1849	1854	1856	rVB5	10243	15017	0.35%	0.034%
49	14.181	1874	1886	1897	rBV	1260096	1963302	45.26%	4.409%
50	14.398	1918	1923	1929	rVB3	15923	24104	0.56%	0.054%
51	14.493	1929	1939	1947	rBV	2554973	3772073	86.96%	8.471%
52	14.681	1963	1971	1979	rBV	177730	315961	7.28%	0.710%
53	14.840	1992	1998	2002	rBV5	17638	29497	0.68%	0.066%
54	14.910	2003	2010	2015	rVV5	20512	46251	1.07%	0.104%
55	14.957	2015	2018	2024	rVB8	6438	12142	0.28%	0.027%
56	15.287	2067	2074	2075	rBV7	8127	13687	0.32%	0.031%
57	15.351	2081	2085	2090	rVB2	11182	13871	0.32%	0.031%
58	15.410	2091	2095	2098	rBV6	7880	11777	0.27%	0.026%
59	15.481	2101	2107	2114	rBV	1540116	2298567	52.99%	5.162%
60	15.534	2114	2116	2121	rVV5	18457	29361	0.68%	0.066%
61	15.592	2121	2126	2135	rVB	152111	230692	5.32%	0.518%
62	15.834	2164	2167	2172	rVB4	8143	11423	0.26%	0.026%
63	15.981	2190	2192	2198	rVB6	10517	15805	0.36%	0.035%
64	16.216	2228	2232	2234	rBV3	19366	23446	0.54%	0.053%
65	16.692	2307	2313	2319	rVV10	10244	23175	0.53%	0.052%
66	16.751	2319	2323	2325	rVV5	7973	11387	0.26%	0.026%
67	16.787	2325	2329	2339	rVB4	18459	35402	0.82%	0.080%
68	17.022	2365	2369	2373	rBV4	14879	20135	0.46%	0.045%
69	17.245	2400	2407	2412	rBV	2464692	3520854	81.17%	7.907%
70	17.287	2412	2414	2418	rVV	86374	93832	2.16%	0.211%
71	17.345	2418	2424	2435	rVB	1374249	1960456	45.19%	4.403%
72	17.492	2445	2449	2452	rBV6	7328	10995	0.25%	0.025%
73	17.557	2458	2460	2465	rVB6	11062	10823	0.25%	0.024%
74	17.651	2472	2476	2477	rBV4	9710	11153	0.26%	0.025%
75	17.763	2490	2495	2499	rBV6	18402	28666	0.66%	0.064%
76	17.828	2503	2506	2509	rVB5	10419	12654	0.29%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018441.D
 Acq On : 28 Nov 2023 15:17
 Operator : MA/JU
 Sample : 05416-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	17.904	2516	2519	2522	rBV5	12294	17163	0.40%	0.039%
78	17.934	2522	2524	2529	rVB5	15582	18993	0.44%	0.043%
79	18.016	2535	2538	2544	rVB5	14673	20636	0.48%	0.046%
80	18.122	2552	2556	2557	rBV2	13080	16556	0.38%	0.037%
81	18.145	2557	2560	2568	rVB3	129034	193101	4.45%	0.434%
82	18.304	2583	2587	2591	rBV3	23778	32066	0.74%	0.072%
83	18.445	2608	2611	2617	rVV7	13332	24600	0.57%	0.055%
84	18.575	2629	2633	2635	rBV4	17769	21473	0.50%	0.048%
85	18.610	2636	2639	2641	rVB3	15799	18083	0.42%	0.041%
86	18.704	2651	2655	2660	rVB2	24186	29844	0.69%	0.067%
87	18.922	2689	2692	2696	rVB	33290	39349	0.91%	0.088%
88	18.969	2697	2700	2703	rVV4	12367	16187	0.37%	0.036%
89	19.057	2711	2715	2718	rBV5	56077	82976	1.91%	0.186%
90	19.169	2732	2734	2740	rVB5	29231	36233	0.84%	0.081%
91	19.269	2747	2751	2757	rVB	185394	258785	5.97%	0.581%
92	19.410	2771	2775	2781	rBV4	46386	74223	1.71%	0.167%
93	19.598	2801	2807	2818	rBV	1716027	2479039	57.15%	5.567%
94	20.728	2995	2999	3004	rVB5	143082	187605	4.32%	0.421%
95	20.780	3005	3008	3012	rBV	69413	93928	2.17%	0.211%
96	20.863	3018	3022	3026	rBV5	114538	151574	3.49%	0.340%
97	21.163	3070	3073	3077	rBV4	144431	174917	4.03%	0.393%
98	21.416	3109	3116	3129	rVB	2484419	4337862	100.00%	9.742%
99	23.851	3523	3530	3546	rVB2	679064	1991182	45.90%	4.472%
100	24.039	3553	3562	3578	rVB	1273155	4316307	99.50%	9.694%




Sum of corrected areas: 44527842

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018441.D
Acq On : 28 Nov 2023 15:17
Operator : MA/JU
Sample : 05416-13
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

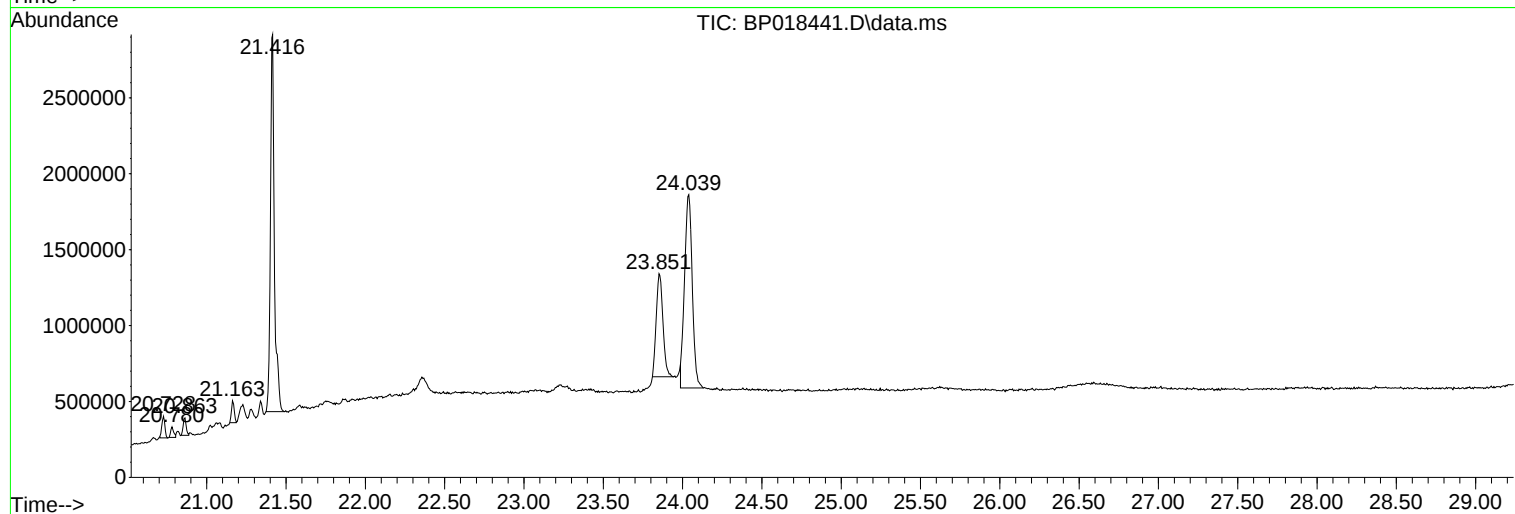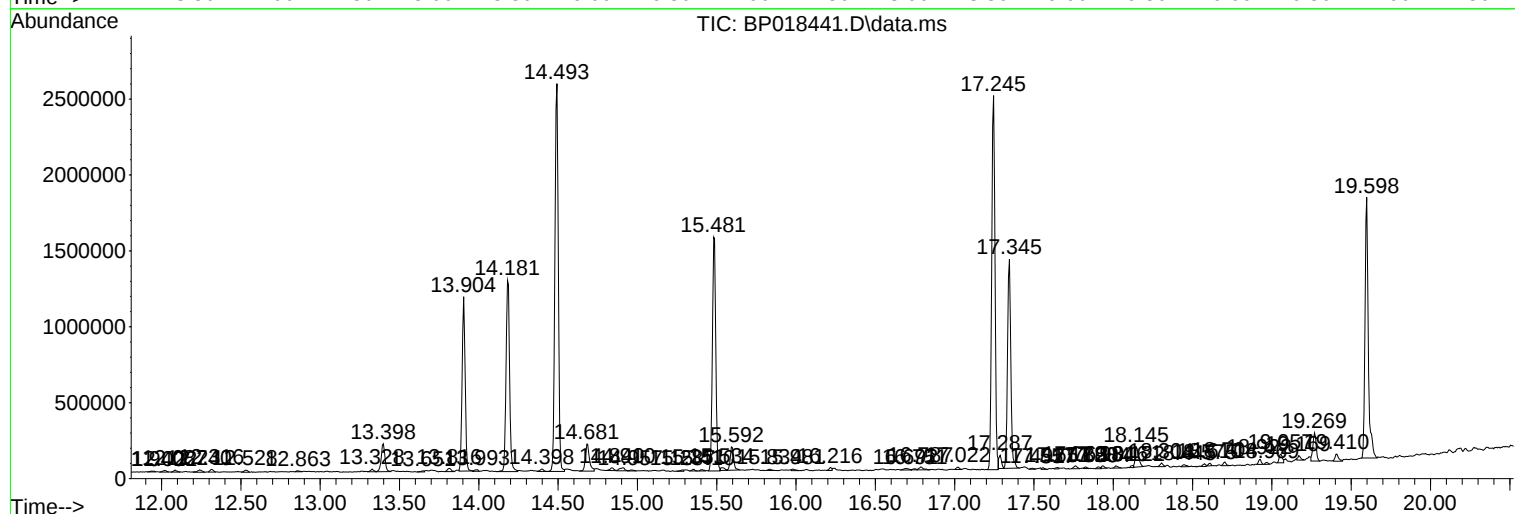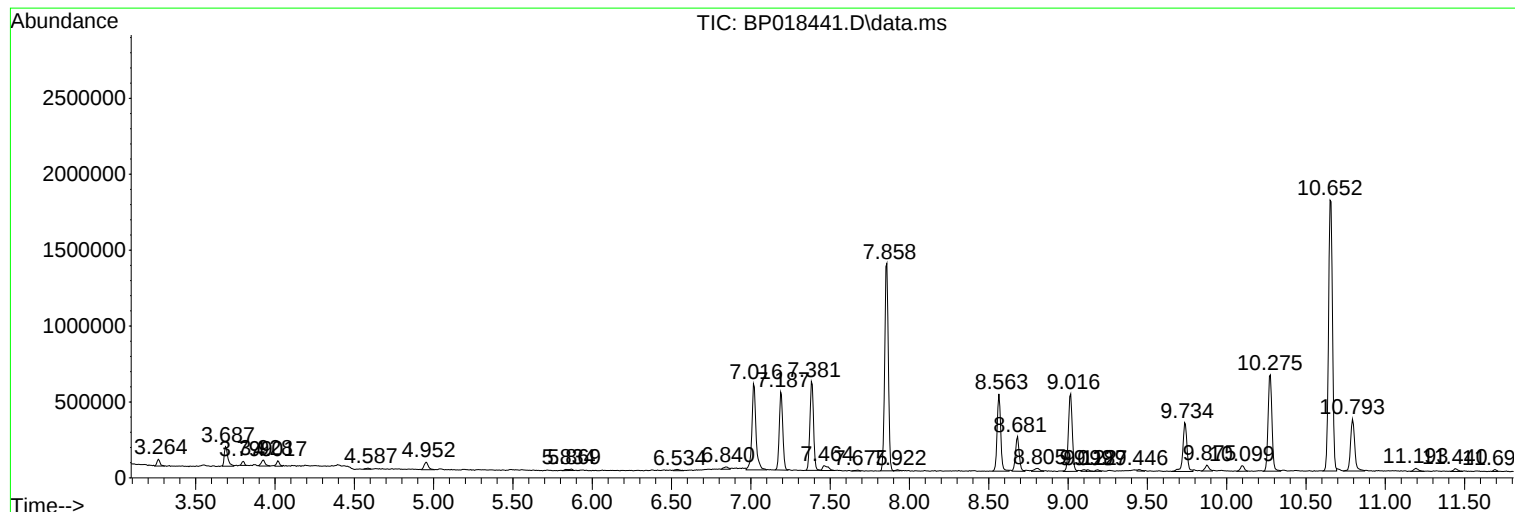

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018441.D
Acq On : 28 Nov 2023 15:17
Operator : MA/JU
Sample : 05416-13
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018441.D
Acq On : 28 Nov 2023 15:17
Operator : MA/JU
Sample : 05416-13
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc