

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018442.D
 Acq On : 28 Nov 2023 15:51
 Operator : MA/JU
 Sample : 05391-01RX
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4A06RX

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	38	rVB	110052	137625	1.34%	0.159%
2	3.681	97	101	116	rBV	835572	1211295	11.82%	1.402%
3	4.017	155	158	162	rVB	29877	39635	0.39%	0.046%
4	7.016	662	668	677	rVB	278653	441996	4.31%	0.512%
5	7.187	687	697	705	rBV	1697451	2694727	26.31%	3.119%
6	7.381	722	730	738	rBV	274634	433457	4.23%	0.502%
7	7.481	741	747	754	rVB	8191	17175	0.17%	0.020%
8	7.858	802	811	818	rBV	1643762	2636069	25.73%	3.051%
9	8.563	923	931	941	rBV	458026	731723	7.14%	0.847%
10	9.016	1000	1008	1019	rBV	1839388	2967548	28.97%	3.435%
11	9.734	1120	1130	1137	rBV	132882	240595	2.35%	0.279%
12	9.893	1152	1157	1167	rBV5	11021	20859	0.20%	0.024%
13	10.275	1214	1222	1232	rBV	277000	484275	4.73%	0.561%
14	10.651	1275	1286	1294	rBV	2112889	3664442	35.77%	4.242%
15	10.793	1301	1310	1323	rBV	2283355	3785611	36.95%	4.382%
16	11.934	1499	1504	1510	rBV9	10541	21776	0.21%	0.025%
17	12.240	1550	1556	1562	rVV3	43587	72237	0.71%	0.084%
18	13.393	1747	1752	1757	rBV3	25208	39400	0.38%	0.046%
19	13.457	1761	1763	1772	rVB7	10523	20911	0.20%	0.024%
20	13.904	1831	1839	1852	rBV	2771389	3808582	37.18%	4.409%
21	14.016	1856	1858	1864	rVB7	5823	11005	0.11%	0.013%
22	14.187	1878	1887	1900	rBV	4522459	6821276	66.59%	7.896%
23	14.492	1932	1939	1950	rBV	3008062	4426388	43.21%	5.124%
24	14.687	1966	1972	1984	rBV	86594	171633	1.68%	0.199%
25	14.904	2005	2009	2015	rVB7	7783	12916	0.13%	0.015%
26	15.487	2101	2108	2121	rBV	5421914	8011143	78.20%	9.274%
27	15.592	2121	2126	2136	rVB2	65991	111620	1.09%	0.129%
28	15.722	2144	2148	2152	rVB3	22820	29491	0.29%	0.034%
29	16.051	2197	2204	2210	rBV10	7495	17846	0.17%	0.021%
30	16.269	2237	2241	2247	rVB9	9512	16093	0.16%	0.019%
31	16.745	2318	2322	2327	rBV6	8001	14046	0.14%	0.016%
32	16.916	2347	2351	2355	rVB7	8355	12982	0.13%	0.015%
33	17.028	2366	2370	2378	rVB5	11142	22663	0.22%	0.026%
34	17.116	2383	2385	2390	rVB6	7366	10688	0.10%	0.012%
35	17.245	2400	2407	2417	rBV	3163939	4602005	44.92%	5.327%
36	17.345	2417	2424	2439	rVB	5304677	7754025	75.69%	8.976%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018442.D
Acq On : 28 Nov 2023 15:51
Operator : MA/JU
Sample : 05391-01RX
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4A06RX

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	18.151	2556	2561	2563	rBV6	11312	17832	0.17%	0.021%
38	18.457	2609	2613	2622	rVB6	17906	36825	0.36%	0.043%
39	18.604	2636	2638	2641	rVB4	9885	11327	0.11%	0.013%
40	19.169	2730	2734	2741	rBV	71870	99148	0.97%	0.115%
41	19.239	2741	2746	2754	rBV	64244	109942	1.07%	0.127%
42	19.598	2801	2807	2817	rVB	7262180	9161872	89.44%	10.606%
43	21.416	3110	3116	3125	rBV	3567669	5255341	51.30%	6.083%
44	23.874	3523	3534	3550	rVB2	3238872	10243955	100.00%	11.858%
45	24.051	3554	3564	3583	rVB	1772640	5935286	57.94%	6.871%




Sum of corrected areas: 86387286

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018442.D
Acq On : 28 Nov 2023 15:51
Operator : MA/JU
Sample : 05391-01RX
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4A06RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

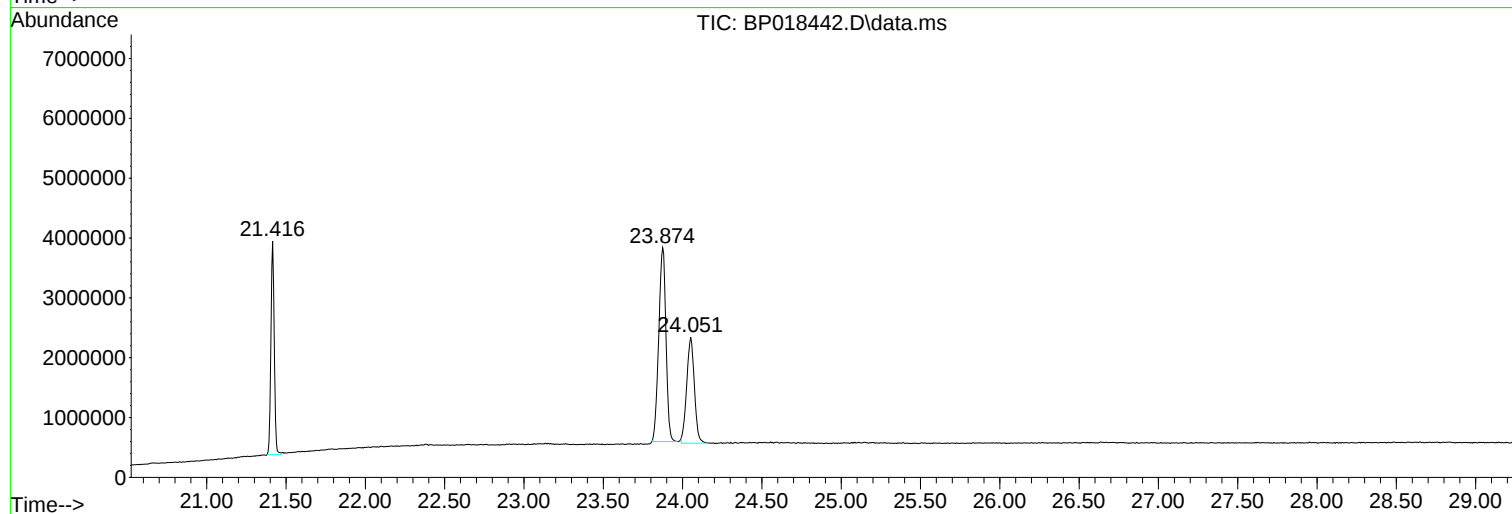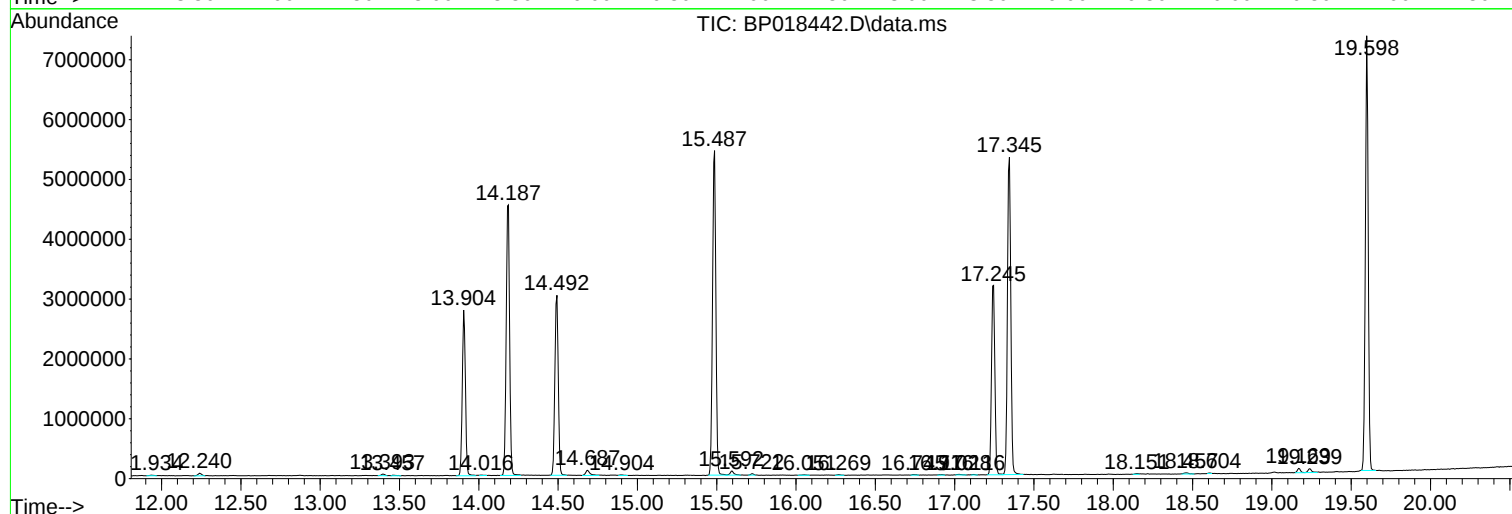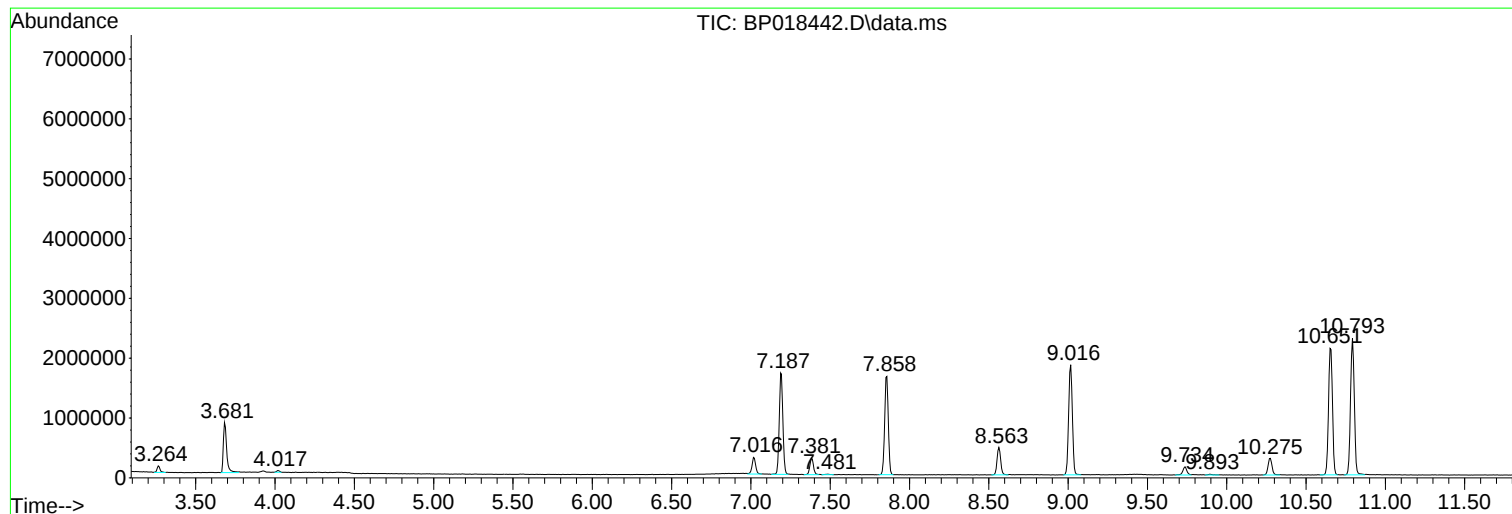

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018442.D
Acq On : 28 Nov 2023 15:51
Operator : MA/JU
Sample : 05391-01RX
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4A06RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018442.D
Acq On : 28 Nov 2023 15:51
Operator : MA/JU
Sample : 05391-01RX
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4A06RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc