

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018443.D
 Acq On : 28 Nov 2023 16:25
 Operator : MA/JU
 Sample : 05416-24
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	42	rVB	44285	74413	1.18%	0.148%
2	3.687	99	102	110	rBV	131754	202019	3.20%	0.403%
3	3.928	139	143	149	rVB	36874	56406	0.89%	0.112%
4	4.016	155	158	163	rVB	26198	34699	0.55%	0.069%
5	4.946	310	316	322	rBV	33045	52693	0.83%	0.105%
6	5.834	464	467	468	rBV3	5795	6415	0.10%	0.013%
7	5.863	470	472	477	rVB6	10108	13222	0.21%	0.026%
8	6.081	504	509	513	rBV8	4133	8103	0.13%	0.016%
9	6.475	569	576	577	rBV6	3135	7075	0.11%	0.014%
10	6.716	613	617	619	rBV5	5429	8018	0.13%	0.016%
11	7.016	661	668	685	rVB	520136	920956	14.58%	1.835%
12	7.187	691	697	706	rBV	459495	719020	11.39%	1.433%
13	7.381	724	730	740	rBV	548864	870112	13.78%	1.734%
14	7.481	740	747	757	rVB6	20636	50826	0.80%	0.101%
15	7.852	800	810	818	rBV	1430550	2314363	36.65%	4.612%
16	7.928	820	823	826	rVB5	6840	7776	0.12%	0.015%
17	8.304	884	887	893	rVB7	5246	7878	0.12%	0.016%
18	8.563	923	931	942	rBV	481207	769497	12.19%	1.533%
19	8.681	944	951	959	rVB	186993	293785	4.65%	0.585%
20	8.799	968	971	973	rBV4	8658	10996	0.17%	0.022%
21	9.016	1000	1008	1015	rBV	453405	745463	11.81%	1.486%
22	9.087	1018	1020	1026	rVB6	6023	9279	0.15%	0.018%
23	9.193	1031	1038	1042	rBV7	13405	22105	0.35%	0.044%
24	9.257	1046	1049	1055	rVB7	5369	7468	0.12%	0.015%
25	9.381	1063	1070	1071	rBV6	4352	8480	0.13%	0.017%
26	9.693	1114	1123	1125	rBV4	21638	48005	0.76%	0.096%
27	9.734	1125	1130	1138	rVB	283475	467676	7.41%	0.932%
28	9.869	1148	1153	1161	rBV	22797	39485	0.63%	0.079%
29	10.099	1187	1192	1201	rVB2	20889	39130	0.62%	0.078%
30	10.275	1214	1222	1231	rBV	564112	952090	15.08%	1.897%
31	10.434	1244	1249	1252	rBV7	6828	11814	0.19%	0.024%
32	10.651	1277	1286	1293	rBV	1870394	3159253	50.03%	6.296%
33	10.793	1300	1310	1325	rBV	426672	772578	12.23%	1.540%
34	11.198	1373	1379	1383	rBV7	14043	23019	0.36%	0.046%
35	11.440	1412	1420	1429	rBV8	14531	33784	0.54%	0.067%
36	11.693	1460	1463	1469	rVB7	8785	12554	0.20%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018443.D
 Acq On : 28 Nov 2023 16:25
 Operator : MA/JU
 Sample : 05416-24
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	11.945	1499	1506	1513	rVB10	8051	20676	0.33%	0.041%
38	12.022	1516	1519	1523	rVB6	6944	8823	0.14%	0.018%
39	12.093	1527	1531	1534	rVB4	9022	12062	0.19%	0.024%
40	12.245	1551	1557	1561	rVB3	14132	23874	0.38%	0.048%

41	12.316	1563	1569	1579	rVB2	23895	43514	0.69%	0.087%
42	12.534	1601	1606	1611	rBV	19478	27867	0.44%	0.056%
43	12.875	1658	1664	1668	rBV9	6221	14590	0.23%	0.029%
44	13.328	1736	1741	1746	rVB4	15392	23906	0.38%	0.048%
45	13.398	1746	1753	1757	rVV	45837	75519	1.20%	0.150%

46	13.457	1760	1763	1767	rVV6	7564	12854	0.20%	0.026%
47	13.651	1790	1796	1798	rBV6	8437	12455	0.20%	0.025%
48	13.675	1798	1800	1804	rVB5	8489	9691	0.15%	0.019%
49	13.816	1817	1824	1828	rVB7	19157	37224	0.59%	0.074%
50	13.863	1828	1832	1833	rBV4	14091	17074	0.27%	0.034%

51	13.904	1833	1839	1850	rVV	1012223	1362758	21.58%	2.716%
52	13.987	1850	1853	1855	rVB4	5985	6423	0.10%	0.013%
53	14.045	1861	1863	1869	rVB7	7737	11234	0.18%	0.022%
54	14.181	1878	1886	1899	rBV	1191575	1758504	27.85%	3.504%
55	14.398	1920	1923	1927	rVB4	12605	13891	0.22%	0.028%

56	14.492	1930	1939	1950	rBV	2537060	3902708	61.80%	7.777%
57	14.581	1950	1954	1958	rVB7	7236	11124	0.18%	0.022%
58	14.681	1966	1971	1984	rBV	123516	237816	3.77%	0.474%
59	14.839	1993	1998	2003	rBV6	15096	29792	0.47%	0.059%
60	14.910	2003	2010	2013	rVV6	22206	54151	0.86%	0.108%

61	14.963	2016	2019	2023	rVB6	7088	11234	0.18%	0.022%
62	15.163	2048	2053	2055	rVB5	6930	10358	0.16%	0.021%
63	15.351	2082	2085	2091	rVB6	12152	15238	0.24%	0.030%
64	15.481	2101	2107	2114	rBV	1603327	2304216	36.49%	4.592%
65	15.592	2122	2126	2138	rVB	83720	135976	2.15%	0.271%

66	15.833	2162	2167	2177	rVB8	9694	20022	0.32%	0.040%
67	15.981	2188	2192	2195	rBV5	7954	10151	0.16%	0.020%
68	16.051	2201	2204	2213	rVB5	6800	15341	0.24%	0.031%
69	16.216	2229	2232	2235	rBV4	13786	17218	0.27%	0.034%
70	16.598	2295	2297	2301	rVB5	4482	6421	0.10%	0.013%

71	16.645	2301	2305	2308	rBV5	8423	10217	0.16%	0.020%
72	16.786	2325	2329	2333	rBV3	20212	27790	0.44%	0.055%
73	17.022	2365	2369	2375	rVB6	15112	23564	0.37%	0.047%
74	17.245	2400	2407	2413	rBV	3391612	4731819	74.93%	9.429%
75	17.286	2413	2414	2417	rVV	52110	44255	0.70%	0.088%

76	17.345	2418	2424	2436	rVV	1732847	2527195	40.02%	5.036%
----	--------	------	------	------	-----	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018443.D
 Acq On : 28 Nov 2023 16:25
 Operator : MA/JU
 Sample : 05416-24
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	17.439	2436	2440	2445	rVB7	23777	40955	0.65%	0.082%
78	17.557	2456	2460	2465	rVB6	5585	8691	0.14%	0.017%
79	17.763	2491	2495	2499	rVB5	17666	25465	0.40%	0.051%
80	17.928	2520	2523	2528	rBV7	9814	16322	0.26%	0.033%
81	18.027	2535	2540	2543	rBV6	15606	31257	0.49%	0.062%
82	18.086	2547	2550	2552	rBV3	7481	7203	0.11%	0.014%
83	18.122	2554	2556	2557	rVV2	8030	7386	0.12%	0.015%
84	18.145	2557	2560	2570	rVB2	150439	220006	3.48%	0.438%
85	18.445	2608	2611	2616	rVB6	23664	27672	0.44%	0.055%
86	18.610	2635	2639	2644	rBV6	19359	30325	0.48%	0.060%
87	18.704	2652	2655	2661	rVB6	19747	27345	0.43%	0.054%
88	18.922	2689	2692	2696	rVB2	32588	39033	0.62%	0.078%
89	18.969	2697	2700	2703	rVB3	15048	16452	0.26%	0.033%
90	19.063	2713	2716	2720	rBV2	31830	41723	0.66%	0.083%
91	19.169	2732	2734	2739	rVB4	32448	42324	0.67%	0.084%
92	19.410	2771	2775	2782	rBV4	86309	124212	1.97%	0.248%
93	19.598	2801	2807	2813	rBV	2775652	3555417	56.30%	7.085%
94	20.192	2905	2908	2911	rVB5	33973	38381	0.61%	0.076%
95	21.416	3110	3116	3127	rBV	3957123	5827005	92.28%	11.612%
96	23.874	3525	3534	3547	rVB2	1067986	3319642	52.57%	6.615%
97	24.062	3555	3566	3586	rVB	1760867	6314754	100.00%	12.584%




Sum of corrected areas: 50181570

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018443.D
Acq On : 28 Nov 2023 16:25
Operator : MA/JU
Sample : 05416-24
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

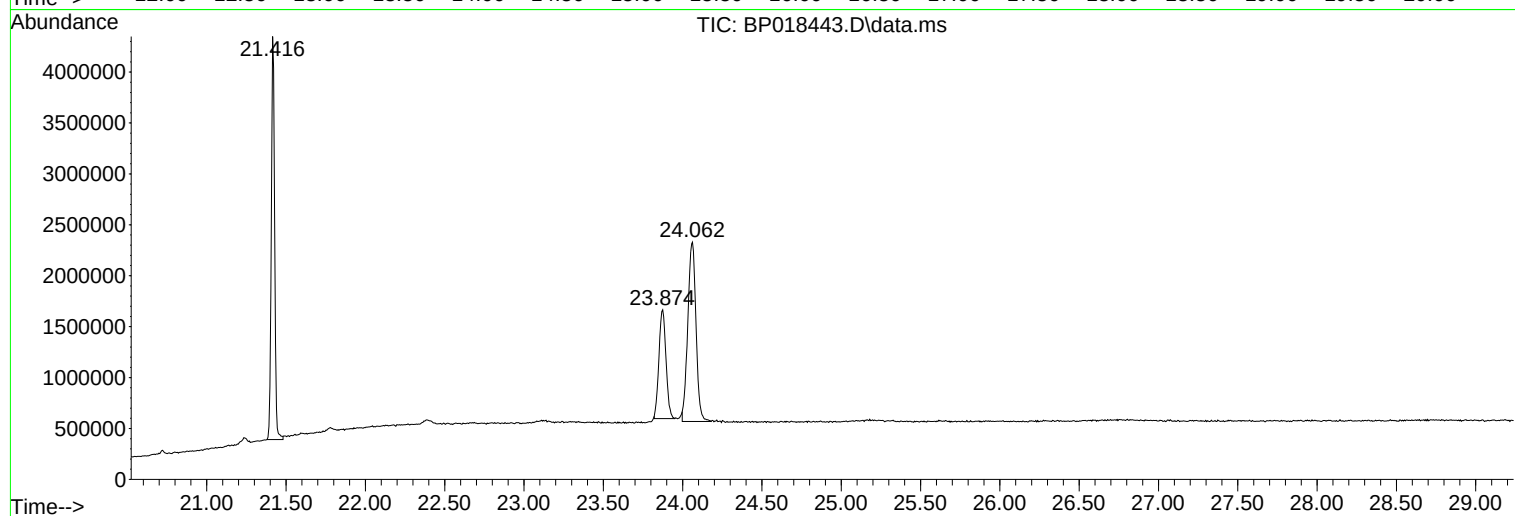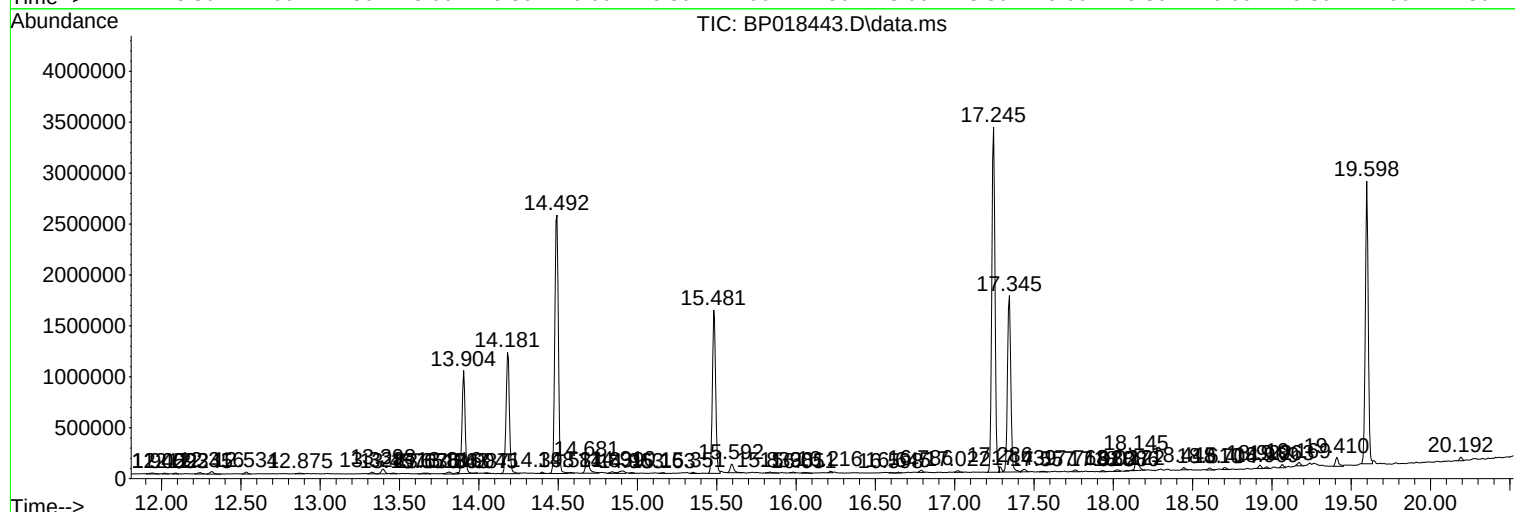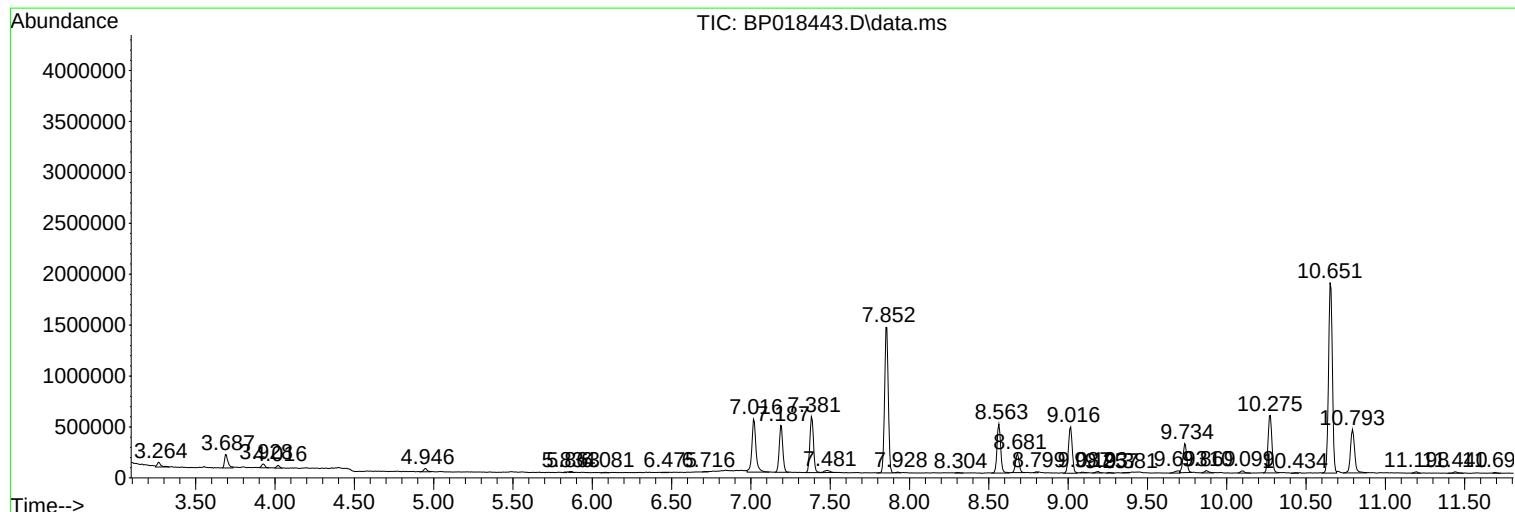

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018443.D
Acq On : 28 Nov 2023 16:25
Operator : MA/JU
Sample : 05416-24
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018443.D
Acq On : 28 Nov 2023 16:25
Operator : MA/JU
Sample : 05416-24
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc