

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018449.D
 Acq On : 28 Nov 2023 20:23
 Operator : MA/JU
 Sample : PB157320BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK320

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	42	rVB	146881	209343	1.95%	0.174%
2	3.681	97	101	122	rBV	1644624	2513408	23.42%	2.088%
3	4.017	155	158	163	rVB2	25188	34519	0.32%	0.029%
4	7.022	662	669	680	rVB	2114523	3348387	31.20%	2.782%
5	7.193	691	698	708	rVB	1766653	2796462	26.06%	2.323%
6	7.381	724	730	741	rBV	2183953	3453149	32.18%	2.869%
7	7.852	800	810	818	rBV	1769888	2810852	26.19%	2.335%
8	8.564	922	931	943	rBV	2826719	4441089	41.38%	3.690%
9	9.016	1000	1008	1019	rBV	2043383	3254481	30.33%	2.704%
10	9.428	1076	1078	1085	rVB8	7701	13031	0.12%	0.011%
11	9.734	1120	1130	1143	rBV	1493077	2458133	22.90%	2.042%
12	10.269	1212	1221	1232	rBV	2762087	4621209	43.06%	3.839%
13	10.652	1278	1286	1299	rVB	2582791	4326617	40.32%	3.594%
14	10.793	1302	1310	1322	rBV	2162281	3714457	34.61%	3.086%
15	12.240	1550	1556	1562	rVB2	55683	89319	0.83%	0.074%
16	13.393	1747	1752	1758	rBV2	30387	52460	0.49%	0.044%
17	13.457	1758	1763	1770	rBV6	9152	17428	0.16%	0.014%
18	13.904	1832	1839	1852	rBV	4703605	6850561	63.83%	5.691%
19	14.181	1879	1886	1898	rBV	5695904	8562132	79.78%	7.113%
20	14.487	1932	1938	1949	rBV	4001184	5997734	55.89%	4.983%
21	14.681	1964	1971	1995	rBV	1417760	2296842	21.40%	1.908%
22	14.846	1997	1999	2004	rVV6	10619	18960	0.18%	0.016%
23	14.898	2004	2008	2015	rVB9	9903	19209	0.18%	0.016%
24	15.487	2100	2108	2119	rBV	7198325	10487509	97.72%	8.713%
25	15.598	2121	2127	2143	rVV	1235470	1697688	15.82%	1.410%
26	15.722	2144	2148	2155	rVB2	35981	58849	0.55%	0.049%
27	16.051	2200	2204	2210	rVB9	7358	12084	0.11%	0.010%
28	16.269	2236	2241	2247	rBV9	8782	16573	0.15%	0.014%
29	16.745	2317	2322	2326	rBV5	7211	12637	0.12%	0.010%
30	16.922	2348	2352	2357	rVB6	11412	18382	0.17%	0.015%
31	17.034	2367	2371	2376	rVB5	9234	13591	0.13%	0.011%
32	17.245	2400	2407	2417	rBV	4589697	6467807	60.27%	5.373%
33	17.345	2417	2424	2441	rVV	7374064	10338307	96.33%	8.589%
34	17.622	2468	2471	2476	rBV4	7693	12049	0.11%	0.010%
35	17.828	2504	2506	2511	rVB6	9085	11175	0.10%	0.009%
36	18.157	2558	2562	2566	rBV7	8093	12747	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018449.D
Acq On : 28 Nov 2023 20:23
Operator : MA/JU
Sample : PB157320BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK320

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	19.175	2731	2735	2742	rVB	80013	108405	1.01%	0.090%
38	19.245	2743	2747	2751	rBV	81793	102555	0.96%	0.085%
39	19.610	2802	2809	2822	rVB	7755557	10731904	100.00%	8.916%
40	21.451	3115	3122	3132	rBV	3123278	5130437	47.81%	4.262%
41	24.010	3545	3557	3573	rVB2	2038765	8271321	77.07%	6.872%
42	24.198	3579	3589	3607	rVB	1168014	4965409	46.27%	4.125%




Sum of corrected areas: 120369211

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018449.D
Acq On : 28 Nov 2023 20:23
Operator : MA/JU
Sample : PB157320BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK320

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

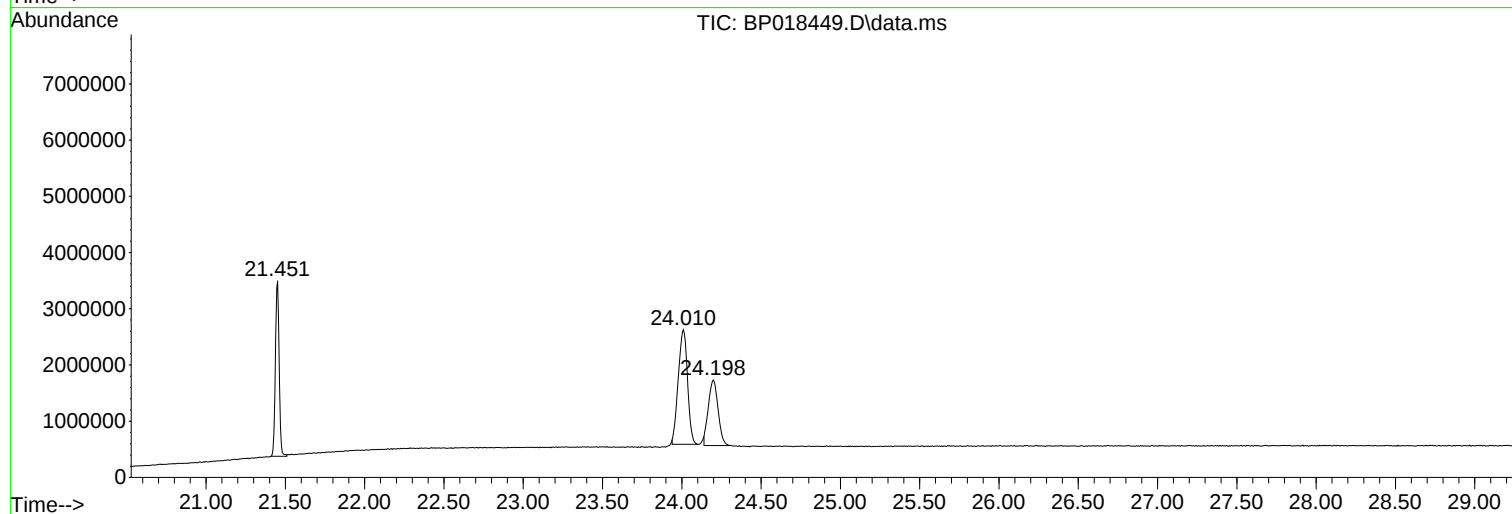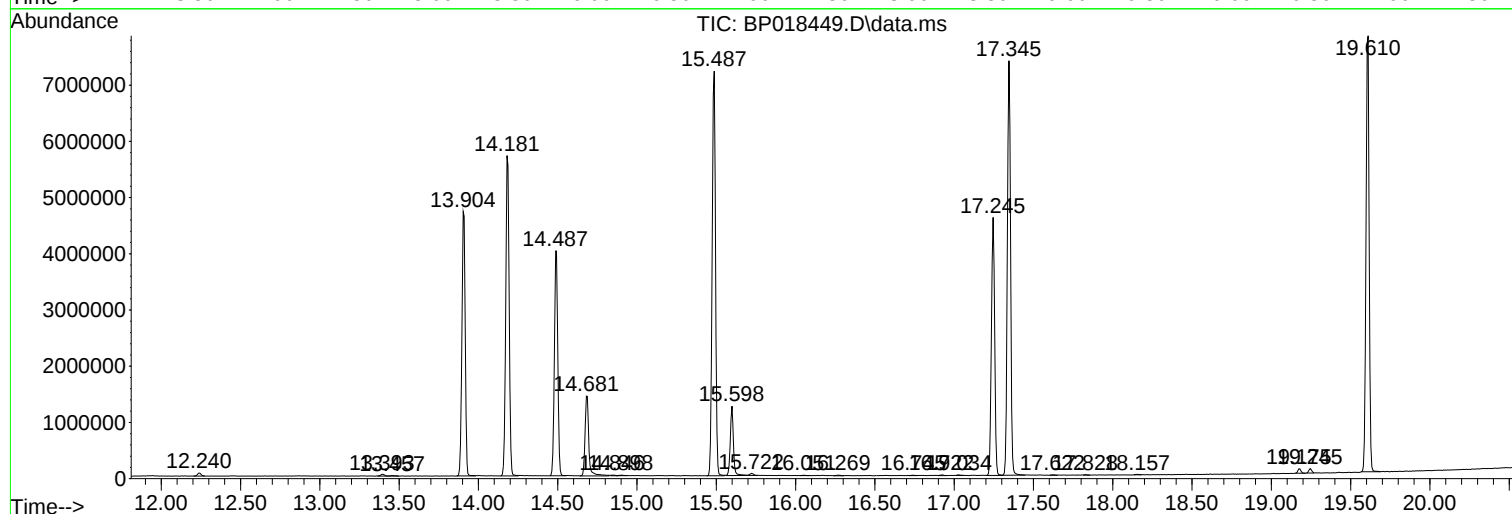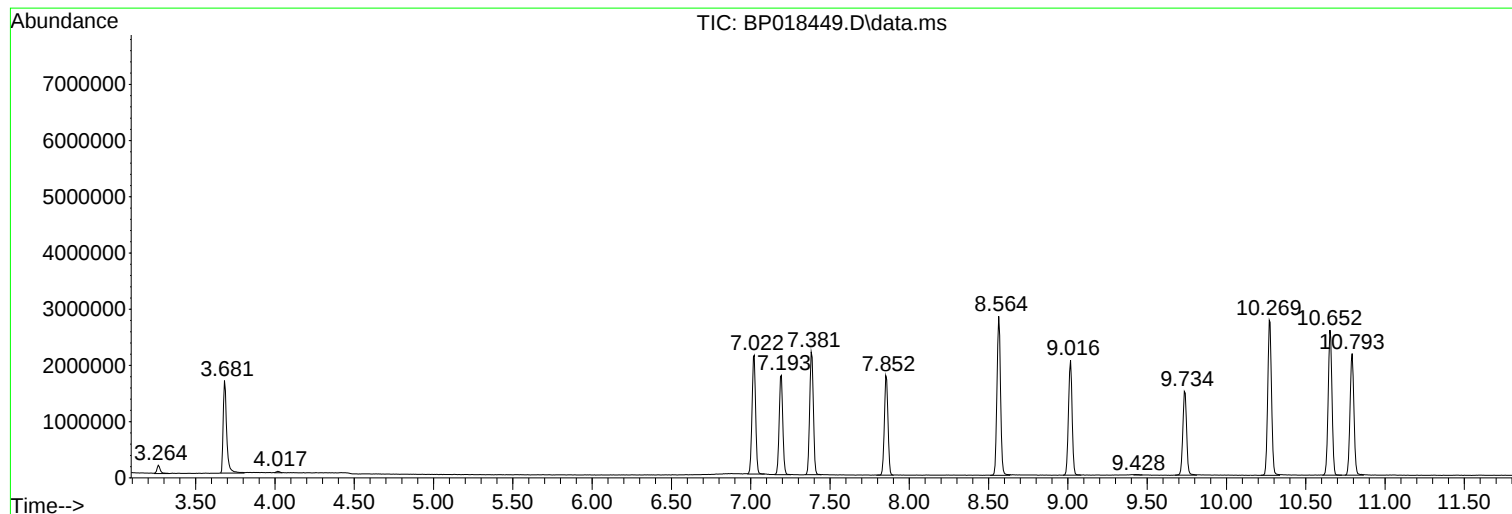

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018449.D
Acq On : 28 Nov 2023 20:23
Operator : MA/JU
Sample : PB157320BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK320

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018449.D
Acq On : 28 Nov 2023 20:23
Operator : MA/JU
Sample : PB157320BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK320

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc