

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018451.D
 Acq On : 28 Nov 2023 21:30
 Operator : MA/JU
 Sample : 05543-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.017	155	158	163	rVB3	23603	32381	0.74%	0.142%
2	7.193	695	698	703	rVB6	5347	9139	0.21%	0.040%
3	7.317	717	719	721	rBV2	4710	5443	0.12%	0.024%
4	7.852	802	810	820	rBV	1627705	2528783	57.64%	11.069%
5	8.640	939	944	945	rBV5	3317	5580	0.13%	0.024%
6	9.169	1031	1034	1036	rBV4	3623	4576	0.10%	0.020%
7	9.240	1043	1046	1049	rBV5	4298	4853	0.11%	0.021%
8	9.363	1061	1067	1068	rBV6	4017	5663	0.13%	0.025%
9	9.399	1068	1073	1074	rBV5	4147	5762	0.13%	0.025%
10	9.722	1121	1128	1129	rBV7	3726	4587	0.10%	0.020%
11	9.811	1141	1143	1146	rBV4	3530	4452	0.10%	0.019%
12	9.846	1146	1149	1153	rVB5	3895	4975	0.11%	0.022%
13	9.916	1157	1161	1166	rBV7	2983	4673	0.11%	0.020%
14	10.252	1215	1218	1223	rBV7	3617	5007	0.11%	0.022%
15	10.605	1269	1278	1279	rBV8	5035	11123	0.25%	0.049%
16	10.652	1279	1286	1294	rVV	2069292	3463742	78.95%	15.162%
17	11.722	1464	1468	1470	rBV5	3541	5535	0.13%	0.024%
18	11.934	1498	1504	1506	rBV7	6387	11459	0.26%	0.050%
19	12.010	1515	1517	1521	rVB5	3738	5221	0.12%	0.023%
20	12.863	1659	1662	1663	rBV2	6471	5128	0.12%	0.022%
21	13.287	1729	1734	1735	rBV5	3853	4752	0.11%	0.021%
22	13.916	1836	1841	1847	rBV8	7313	16107	0.37%	0.071%
23	14.487	1928	1938	1948	rBV	2710846	4057861	92.49%	17.762%
24	15.393	2090	2092	2096	rVB5	3743	5455	0.12%	0.024%
25	15.481	2103	2107	2111	rBV6	7842	13430	0.31%	0.059%
26	16.222	2230	2233	2236	rBV5	3886	6105	0.14%	0.027%
27	16.645	2302	2305	2308	rBV4	4101	4655	0.11%	0.020%
28	16.822	2332	2335	2339	rBV5	3411	4462	0.10%	0.020%
29	16.963	2355	2359	2363	rBV5	3290	4825	0.11%	0.021%
30	17.245	2401	2407	2422	rBV	2983229	4090224	93.22%	17.904%
31	17.839	2503	2508	2511	rBV7	8062	11281	0.26%	0.049%
32	21.457	3117	3123	3133	rBV	2696948	4387508	100.00%	19.205%
33	24.227	3585	3594	3610	rVB2	950495	4110816	93.69%	17.994%




Sum of corrected areas: 22845563

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018451.D
Acq On : 28 Nov 2023 21:30
Operator : MA/JU
Sample : 05543-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

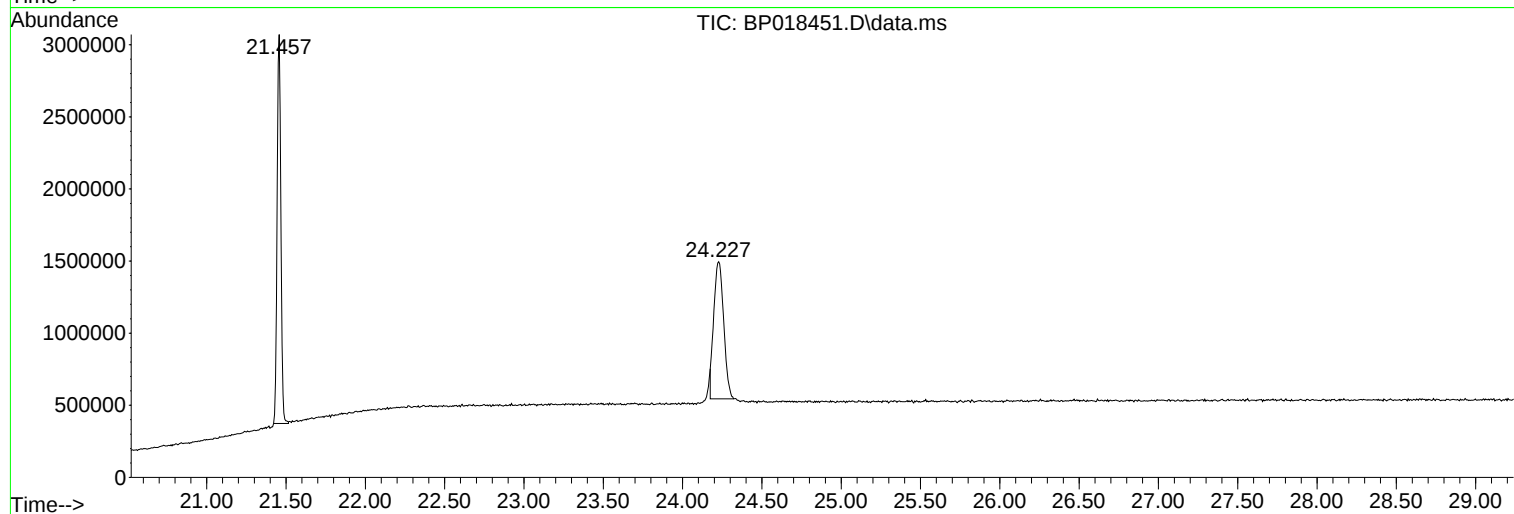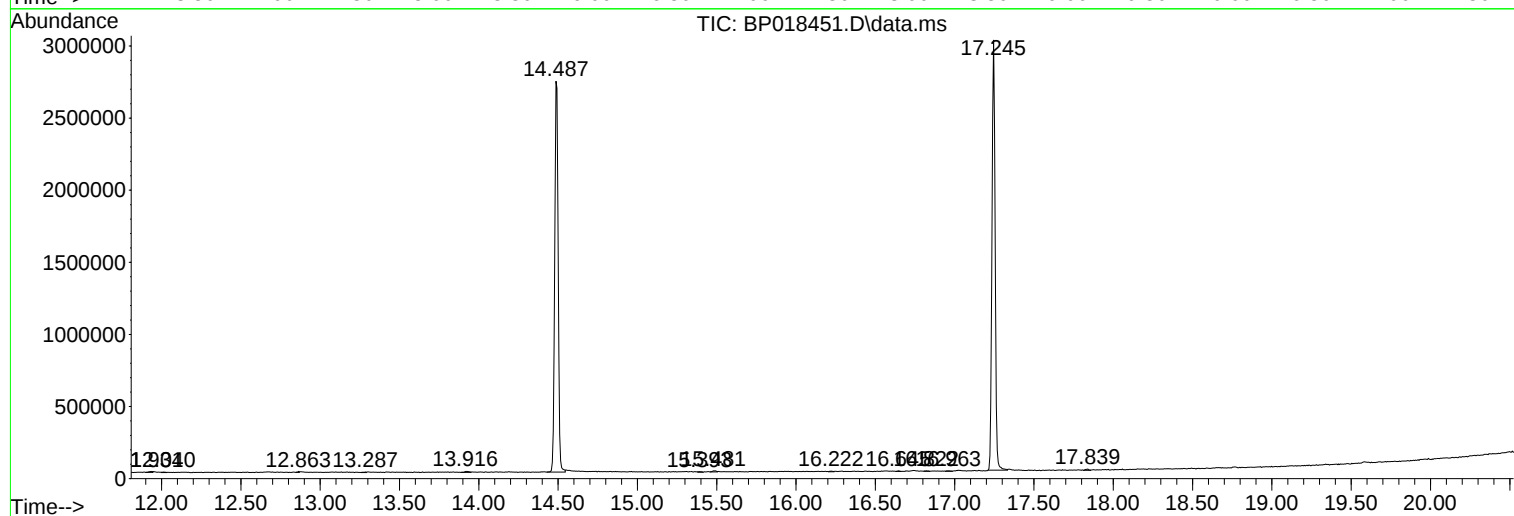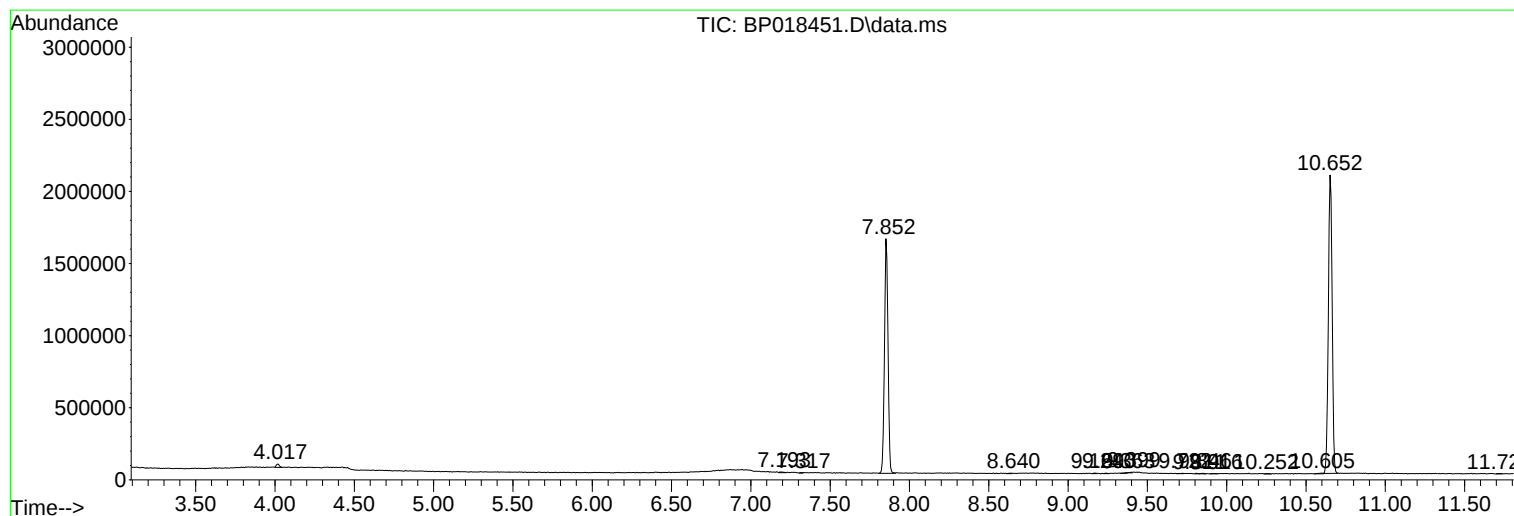

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018451.D
Acq On : 28 Nov 2023 21:30
Operator : MA/JU
Sample : 05543-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018451.D
Acq On : 28 Nov 2023 21:30
Operator : MA/JU
Sample : 05543-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc