

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018453.D
 Acq On : 28 Nov 2023 22:38
 Operator : MA/JU
 Sample : 05416-14
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rVB	37401	47696	0.95%	0.092%
2	3.540	74	77	85	rBV	122813	170247	3.40%	0.328%
3	3.687	98	102	113	rBV	166828	252672	5.04%	0.487%
4	3.799	118	121	129	rVB4	22978	32998	0.66%	0.064%
5	3.928	138	143	149	rVB	46369	75727	1.51%	0.146%
6	4.017	154	158	163	rVB	44713	59883	1.19%	0.115%
7	4.575	249	253	257	rVB7	8985	13113	0.26%	0.025%
8	4.952	311	317	327	rBV3	49966	99506	1.98%	0.192%
9	5.040	330	332	337	rVB6	5532	7935	0.16%	0.015%
10	5.481	403	407	411	rVV5	9459	14918	0.30%	0.029%
11	5.552	417	419	426	rVV7	6592	11417	0.23%	0.022%
12	5.834	464	467	470	rBV3	7495	10842	0.22%	0.021%
13	5.864	470	472	478	rVB7	10634	14690	0.29%	0.028%
14	6.840	634	638	643	rBV7	9514	17018	0.34%	0.033%
15	7.016	660	668	684	rVB	754531	1297326	25.87%	2.500%
16	7.187	691	697	706	rVB	672489	1031581	20.57%	1.988%
17	7.381	724	730	737	rBV	778483	1194116	23.81%	2.301%
18	7.475	740	746	754	rVV6	25269	62034	1.24%	0.120%
19	7.852	802	810	818	rBV	1699784	2617995	52.21%	5.045%
20	7.922	819	822	827	rVB6	8876	13904	0.28%	0.027%
21	8.563	924	931	939	rBV	766641	1189699	23.73%	2.293%
22	8.681	945	951	958	rBV	252010	413476	8.25%	0.797%
23	8.810	968	973	974	rBV4	10200	12682	0.25%	0.024%
24	9.010	998	1007	1014	rBV	650669	1066225	21.26%	2.055%
25	9.087	1017	1020	1023	rVV4	7829	11444	0.23%	0.022%
26	9.122	1023	1026	1032	rVB6	8208	13600	0.27%	0.026%
27	9.187	1032	1037	1041	rBV7	6976	11362	0.23%	0.022%
28	9.393	1066	1072	1073	rVV6	6685	9819	0.20%	0.019%
29	9.446	1073	1081	1085	rVB6	11240	32141	0.64%	0.062%
30	9.734	1118	1130	1140	rBV	419304	733323	14.62%	1.413%
31	9.875	1148	1154	1160	rBV3	35778	66019	1.32%	0.127%
32	10.099	1187	1192	1198	rVB2	37802	62202	1.24%	0.120%
33	10.269	1214	1221	1234	rBV	849037	1384691	27.62%	2.668%
34	10.652	1278	1286	1293	rBV	2237481	3715922	74.11%	7.161%
35	10.793	1303	1310	1323	rBV	564603	1004083	20.02%	1.935%
36	11.193	1373	1378	1385	rBV6	20025	38241	0.76%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018453.D
 Acq On : 28 Nov 2023 22:38
 Operator : MA/JU
 Sample : 05416-14
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	11.440	1414	1420	1425	rBV2	20490	38766	0.77%	0.075%
38	11.693	1459	1463	1469	rVB7	7999	13347	0.27%	0.026%
39	11.934	1502	1504	1511	rVB8	7072	11498	0.23%	0.022%
40	12.016	1513	1518	1524	rBV4	9773	19352	0.39%	0.037%
41	12.087	1524	1530	1533	rBV5	7378	10793	0.22%	0.021%
42	12.240	1552	1556	1561	rVV4	13837	20563	0.41%	0.040%
43	12.316	1564	1569	1578	rVB2	15236	25987	0.52%	0.050%
44	12.534	1601	1606	1613	rVB5	12311	20823	0.42%	0.040%
45	13.040	1688	1692	1697	rVV8	5448	8825	0.18%	0.017%
46	13.328	1735	1741	1746	rVB5	16262	25269	0.50%	0.049%
47	13.398	1746	1753	1760	rBV	36654	63866	1.27%	0.123%
48	13.463	1760	1764	1767	rBV6	8322	11948	0.24%	0.023%
49	13.816	1814	1824	1829	rBV6	15072	31180	0.62%	0.060%
50	13.904	1833	1839	1849	rVV	1424232	1950287	38.90%	3.758%
51	13.981	1849	1852	1856	rVB5	10509	13989	0.28%	0.027%
52	14.045	1862	1863	1867	rVB4	8983	7897	0.16%	0.015%
53	14.181	1875	1886	1899	rBV	1685585	2483514	49.53%	4.786%
54	14.398	1920	1923	1927	rVB3	13935	16430	0.33%	0.032%
55	14.487	1931	1938	1947	rBV	3014666	4535824	90.46%	8.741%
56	14.681	1965	1971	1980	rBV	266260	437561	8.73%	0.843%
57	14.840	1994	1998	2003	rVV6	14559	25419	0.51%	0.049%
58	14.904	2003	2009	2015	rVV7	21756	47996	0.96%	0.092%
59	14.963	2015	2019	2023	rVB6	6386	10922	0.22%	0.021%
60	15.098	2038	2042	2045	rBV6	4263	7730	0.15%	0.015%
61	15.287	2069	2074	2075	rBV5	8664	11836	0.24%	0.023%
62	15.351	2083	2085	2091	rVB4	10836	12620	0.25%	0.024%
63	15.481	2101	2107	2114	rBV	2045606	2987575	59.58%	5.757%
64	15.598	2121	2127	2132	rBV	198944	284971	5.68%	0.549%
65	15.839	2163	2168	2176	rVB10	8425	15741	0.31%	0.030%
66	15.981	2188	2192	2200	rVB9	9134	18763	0.37%	0.036%
67	16.216	2229	2232	2240	rBV9	14526	23782	0.47%	0.046%
68	16.539	2285	2287	2295	rVB9	9059	16055	0.32%	0.031%
69	16.651	2302	2306	2309	rBV5	7676	10521	0.21%	0.020%
70	16.710	2309	2316	2318	rBV8	7592	12946	0.26%	0.025%
71	16.787	2325	2329	2334	rBV8	8551	13400	0.27%	0.026%
72	16.898	2345	2348	2351	rBV5	5744	8470	0.17%	0.016%
73	17.022	2366	2369	2373	rVB4	11010	15791	0.31%	0.030%
74	17.063	2373	2376	2379	rBV4	8657	9423	0.19%	0.018%
75	17.245	2401	2407	2412	rBV	3205662	4434570	88.44%	8.545%
76	17.286	2412	2414	2418	rVV	81390	105716	2.11%	0.204%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018453.D
 Acq On : 28 Nov 2023 22:38
 Operator : MA/JU
 Sample : 05416-14
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	17.345	2418	2424	2436	rVV2	1891358	2702258	53.89%	5.207%
78	17.439	2438	2440	2445	rVB6	18157	25120	0.50%	0.048%
79	17.486	2445	2448	2452	rBV3	8474	10550	0.21%	0.020%
80	17.651	2474	2476	2481	rBV5	7364	10996	0.22%	0.021%
81	17.769	2491	2496	2501	rBV7	15299	25811	0.51%	0.050%
82	18.028	2534	2540	2544	rBV3	16568	29638	0.59%	0.057%
83	18.122	2553	2556	2558	rBV2	10805	15295	0.31%	0.029%
84	18.157	2558	2562	2569	rVV3	154117	227072	4.53%	0.438%
85	18.222	2571	2573	2580	rVV3	15051	30146	0.60%	0.058%
86	18.310	2584	2588	2592	rVV3	23306	40645	0.81%	0.078%
87	18.345	2592	2594	2599	rVB4	13478	15942	0.32%	0.031%
88	18.457	2610	2613	2618	rVB6	14093	18013	0.36%	0.035%
89	18.616	2637	2640	2643	rVB3	20403	22242	0.44%	0.043%
90	18.710	2653	2656	2661	rVB2	28048	34026	0.68%	0.066%
91	18.933	2690	2694	2698	rBV2	41692	57066	1.14%	0.110%
92	18.975	2698	2701	2706	rBV	21519	27387	0.55%	0.053%
93	19.028	2706	2710	2712	rBV4	15768	24060	0.48%	0.046%
94	19.180	2733	2736	2741	rVB6	29196	40751	0.81%	0.079%
95	19.280	2748	2753	2758	rVB	217232	298151	5.95%	0.575%
96	19.433	2775	2779	2783	rBV2	61885	86235	1.72%	0.166%
97	19.610	2803	2809	2820	rBV	2400527	3494805	69.70%	6.735%
98	20.816	3011	3014	3020	rVB2	81151	114196	2.28%	0.220%
99	21.463	3118	3124	3136	rVB	2831272	5014217	100.00%	9.662%
100	24.268	3592	3601	3623	rVB2	1053771	4896750	97.66%	9.436%




Sum of corrected areas: 51893885

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018453.D
Acq On : 28 Nov 2023 22:38
Operator : MA/JU
Sample : 05416-14
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

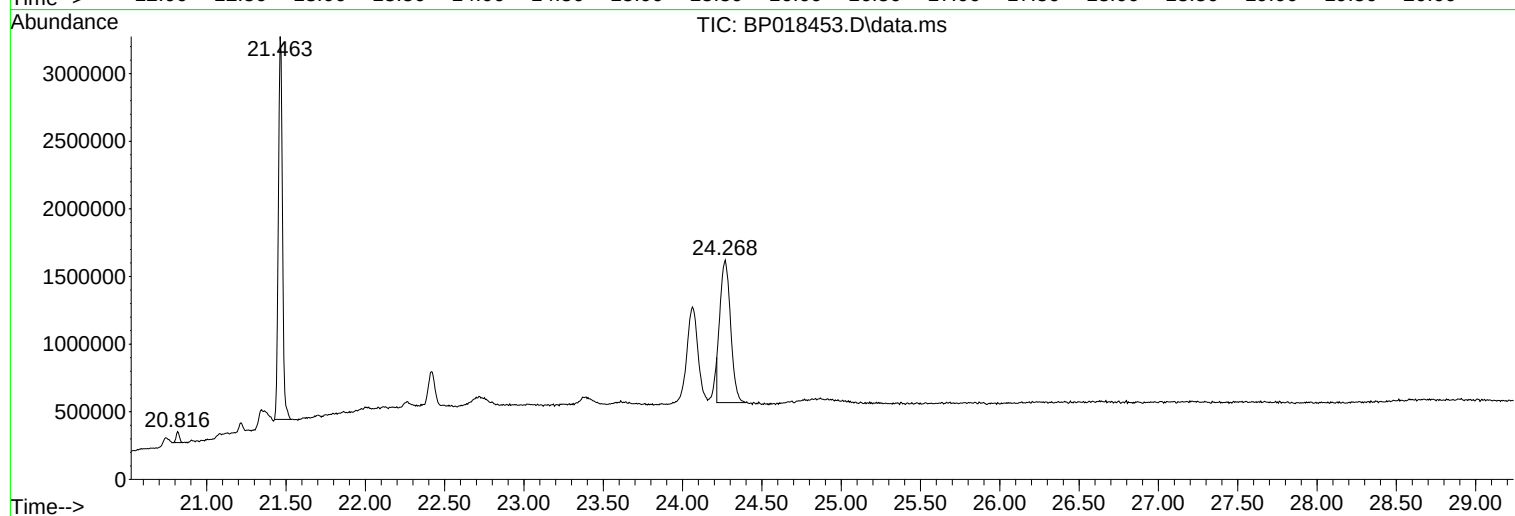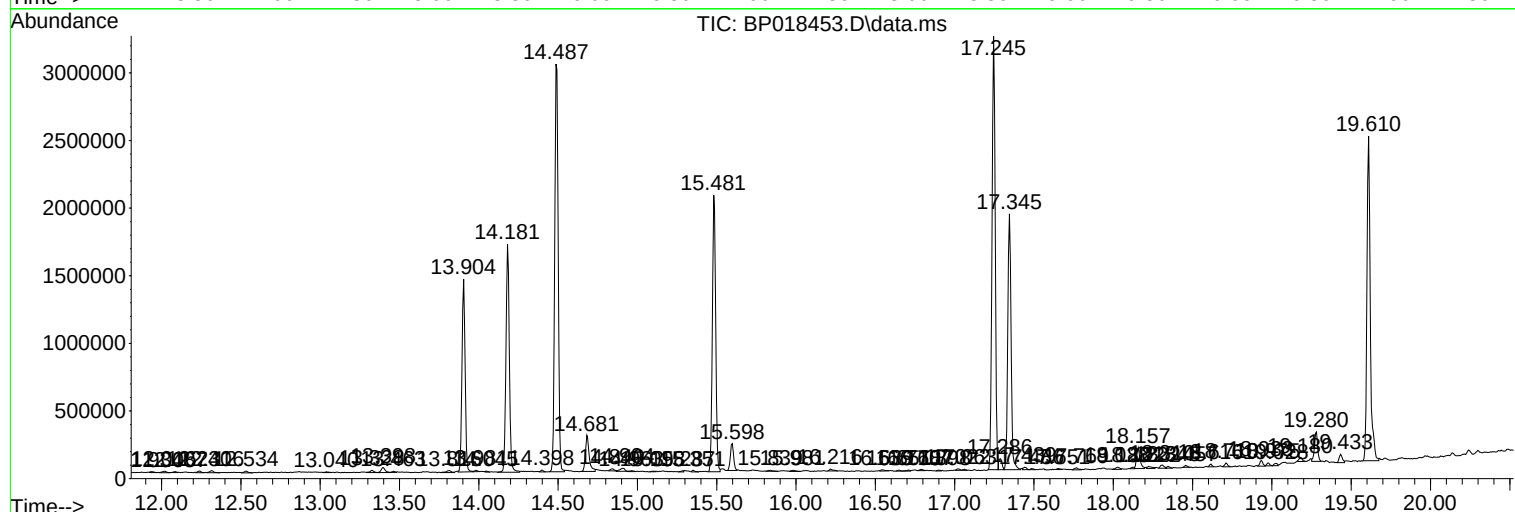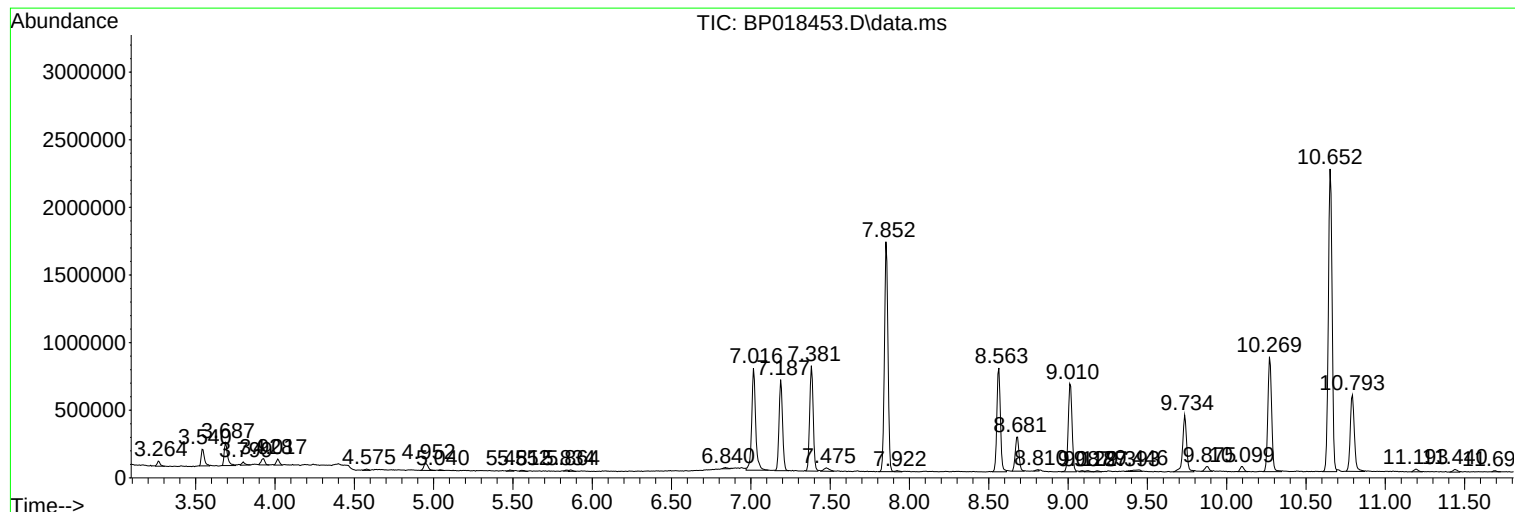

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018453.D
Acq On : 28 Nov 2023 22:38
Operator : MA/JU
Sample : 05416-14
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018453.D
Acq On : 28 Nov 2023 22:38
Operator : MA/JU
Sample : 05416-14
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc