

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018454.D
 Acq On : 28 Nov 2023 23:12
 Operator : MA/JU
 Sample : 05416-15
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COAH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	27	30	35	rVB	43506	49578	0.78%	0.078%
2	3.687	99	102	113	rBV	165583	258572	4.08%	0.406%
3	3.799	117	121	125	rVV	34389	47783	0.75%	0.075%
4	3.922	138	142	147	rVB	38024	53073	0.84%	0.083%
5	4.016	154	158	164	rVB2	35676	50778	0.80%	0.080%
6	4.952	310	317	327	rVV2	55374	109724	1.73%	0.172%
7	5.863	469	472	477	rVB7	9797	14379	0.23%	0.023%
8	6.840	632	638	644	rBV8	14587	35727	0.56%	0.056%
9	7.016	659	668	681	rVB	858189	1474070	23.29%	2.312%
10	7.187	691	697	711	rVB	759338	1152166	18.20%	1.807%
11	7.381	724	730	739	rVV	889621	1346698	21.28%	2.112%
12	7.481	739	747	756	rVV6	24895	67111	1.06%	0.105%
13	7.675	773	780	783	rBV7	7682	16447	0.26%	0.026%
14	7.851	803	810	819	rBV	1725663	2690864	42.51%	4.220%
15	8.563	923	931	943	rBV	852798	1372000	21.67%	2.152%
16	8.675	943	950	958	rVV	363587	601154	9.50%	0.943%
17	8.810	966	973	984	rVB5	17916	52473	0.83%	0.082%
18	9.010	1001	1007	1017	rVV	777915	1268180	20.03%	1.989%
19	9.087	1017	1020	1024	rVV4	12663	22087	0.35%	0.035%
20	9.181	1032	1036	1043	rVB10	11840	22282	0.35%	0.035%
21	9.257	1045	1049	1055	rVV8	8470	14158	0.22%	0.022%
22	9.445	1076	1081	1086	rVB8	11144	25586	0.40%	0.040%
23	9.734	1116	1130	1147	rBV	526243	955869	15.10%	1.499%
24	9.875	1147	1154	1161	rBV	47850	92186	1.46%	0.145%
25	10.092	1185	1191	1198	rBV	44300	76981	1.22%	0.121%
26	10.269	1213	1221	1230	rBV	1070068	1745127	27.57%	2.737%
27	10.651	1278	1286	1293	rBV	2469203	4134924	65.32%	6.485%
28	10.704	1293	1295	1299	rVB2	17134	18866	0.30%	0.030%
29	10.792	1302	1310	1323	rVV	750615	1322684	20.90%	2.074%
30	11.192	1372	1378	1386	rBV5	25696	46272	0.73%	0.073%
31	11.439	1414	1420	1429	rBV2	30933	59458	0.94%	0.093%
32	11.692	1457	1463	1471	rBV10	16010	29526	0.47%	0.046%
33	12.016	1512	1518	1524	rBV2	18112	34744	0.55%	0.054%
34	12.086	1526	1530	1536	rVB5	17119	27423	0.43%	0.043%
35	12.239	1548	1556	1562	rVV2	18910	36218	0.57%	0.057%
36	12.310	1562	1568	1578	rVB	24909	45496	0.72%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018454.D
 Acq On : 28 Nov 2023 23:12
 Operator : MA/JU
 Sample : 05416-15
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COAH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	12.533	1600	1606	1612	rVB2	16613	28054	0.44%	0.044%
38	13.328	1737	1741	1744	rVB2	26500	34132	0.54%	0.054%
39	13.392	1746	1752	1758	rBV	48053	81849	1.29%	0.128%
40	13.657	1788	1797	1798	rBV8	10565	21198	0.33%	0.033%
41	13.816	1819	1824	1828	rBV4	31662	49581	0.78%	0.078%
42	13.904	1833	1839	1849	rVV	2062198	2805473	44.32%	4.400%
43	13.980	1849	1852	1857	rVV4	12983	19687	0.31%	0.031%
44	14.039	1857	1862	1868	rVB8	8454	16665	0.26%	0.026%
45	14.180	1876	1886	1897	rBV	2360189	3475259	54.90%	5.450%
46	14.398	1919	1923	1928	rVB4	23797	32069	0.51%	0.050%
47	14.492	1928	1939	1947	rBV	3826781	5822372	91.98%	9.131%
48	14.551	1947	1949	1958	rVB10	14136	31592	0.50%	0.050%
49	14.680	1965	1971	1979	rBV	416404	674384	10.65%	1.058%
50	14.839	1994	1998	2003	rBV3	22865	35166	0.56%	0.055%
51	14.910	2003	2010	2015	rVV5	34518	72514	1.15%	0.114%
52	14.969	2015	2020	2023	rVB6	11334	17381	0.27%	0.027%
53	15.157	2048	2052	2056	rVB6	11618	15786	0.25%	0.025%
54	15.280	2067	2073	2076	rBV6	11653	22186	0.35%	0.035%
55	15.310	2076	2078	2082	rVV5	12046	16584	0.26%	0.026%
56	15.351	2082	2085	2091	rVB3	22763	28627	0.45%	0.045%
57	15.480	2100	2107	2114	rBV	2970416	4336711	68.51%	6.801%
58	15.598	2121	2127	2136	rBV	368335	521353	8.24%	0.818%
59	15.722	2145	2148	2152	rBV4	10543	15718	0.25%	0.025%
60	15.833	2162	2167	2173	rBV3	14450	28111	0.44%	0.044%
61	15.980	2186	2192	2199	rVV9	13753	30708	0.49%	0.048%
62	16.069	2201	2207	2214	rVB9	9328	18970	0.30%	0.030%
63	16.216	2228	2232	2235	rBV4	28984	42628	0.67%	0.067%
64	16.539	2282	2287	2293	rBV	71247	99400	1.57%	0.156%
65	16.792	2325	2330	2333	rBV4	28552	44374	0.70%	0.070%
66	16.904	2344	2349	2350	rBV4	10595	14520	0.23%	0.023%
67	16.969	2358	2360	2363	rBV3	10322	13975	0.22%	0.022%
68	17.021	2366	2369	2373	rVV4	30231	47573	0.75%	0.075%
69	17.063	2373	2376	2383	rVB3	16915	29432	0.46%	0.046%
70	17.245	2400	2407	2412	rVV	4523083	6329891	100.00%	9.927%
71	17.286	2412	2414	2418	rVV	209273	257366	4.07%	0.404%
72	17.345	2418	2424	2436	rVV2	2911674	4208283	66.48%	6.600%
73	17.439	2436	2440	2447	rVB10	29851	54636	0.86%	0.086%
74	17.551	2457	2459	2465	rVB4	13544	22128	0.35%	0.035%
75	17.769	2491	2496	2501	rVB5	35158	54296	0.86%	0.085%
76	17.827	2503	2506	2512	rVB5	12196	16947	0.27%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018454.D
 Acq On : 28 Nov 2023 23:12
 Operator : MA/JU
 Sample : 05416-15
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COAH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	17.910	2516	2520	2528	rBV6	56512	107767	1.70%	0.169%
78	18.027	2536	2540	2546	rVB3	22117	36864	0.58%	0.058%
79	18.121	2552	2556	2558	rBV2	33444	42926	0.68%	0.067%
80	18.157	2558	2562	2570	rVB2	283493	420943	6.65%	0.660%
81	18.310	2583	2588	2592	rBV4	45414	78064	1.23%	0.122%
82	18.345	2592	2594	2599	rVB2	30116	35227	0.56%	0.055%
83	18.457	2609	2613	2618	rVB4	33866	48932	0.77%	0.077%
84	18.586	2632	2635	2637	rBV3	19022	23601	0.37%	0.037%
85	18.616	2637	2640	2644	rVB	35069	45232	0.71%	0.071%
86	18.710	2653	2656	2661	rVB3	43085	56578	0.89%	0.089%
87	18.857	2678	2681	2685	rVB4	25208	28721	0.45%	0.045%
88	18.933	2691	2694	2698	rVB	59790	71890	1.14%	0.113%
89	18.974	2698	2701	2705	rBV4	25528	31711	0.50%	0.050%
90	19.021	2705	2709	2712	rBV2	35184	56880	0.90%	0.089%
91	19.068	2713	2717	2728	rVV8	119079	257810	4.07%	0.404%
92	19.180	2733	2736	2742	rVB3	48736	79384	1.25%	0.124%
93	19.280	2749	2753	2759	rVB	325610	419827	6.63%	0.658%
94	19.433	2775	2779	2783	rBV3	115078	161428	2.55%	0.253%
95	19.610	2803	2809	2818	rBV	3461564	5058743	79.92%	7.934%
96	20.245	2914	2917	2921	rVB5	43570	58965	0.93%	0.092%
97	20.745	2996	3002	3011	rBV	907644	1918753	30.31%	3.009%
98	20.815	3012	3014	3019	rVB3	103424	153411	2.42%	0.241%
99	21.221	3079	3083	3091	rVB4	178383	308856	4.88%	0.484%
100	21.468	3118	3125	3138	rVB	3047626	5402684	85.35%	8.473%




Sum of corrected areas: 63763440

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018454.D
Acq On : 28 Nov 2023 23:12
Operator : MA/JU
Sample : 05416-15
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COAH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

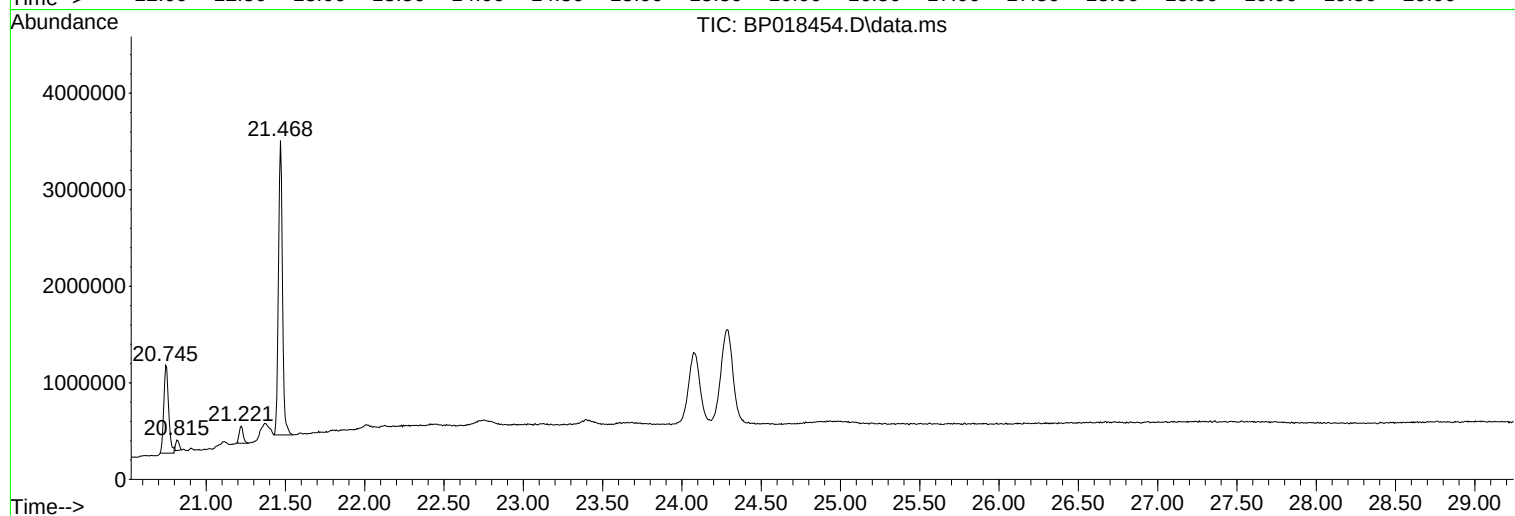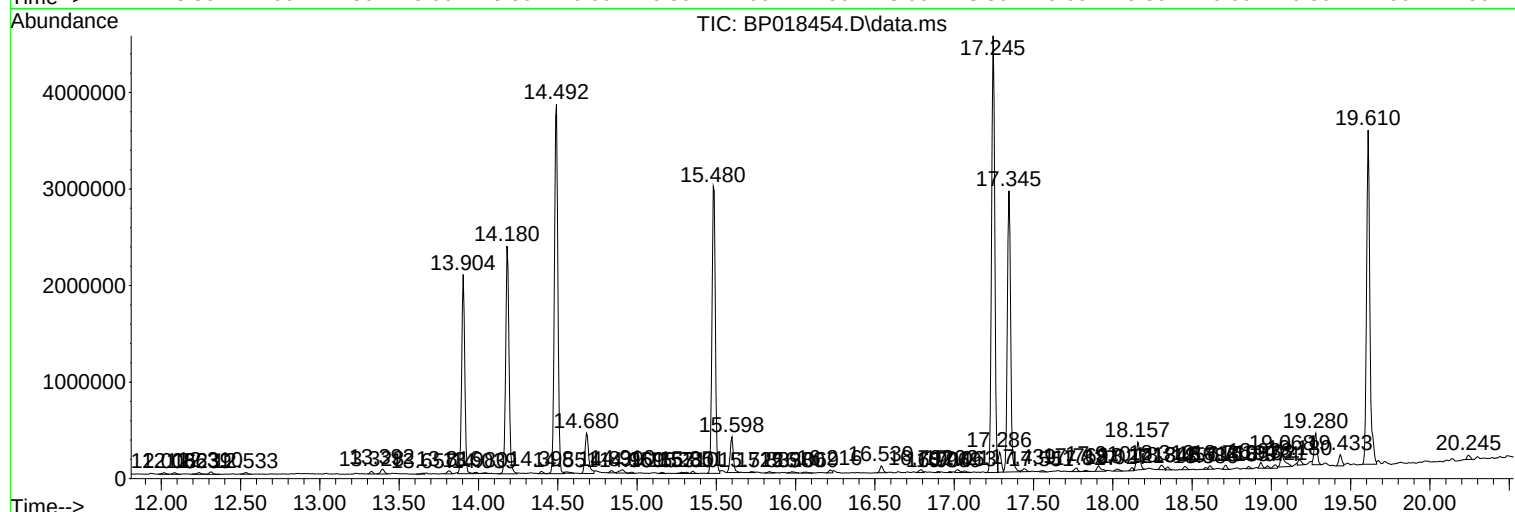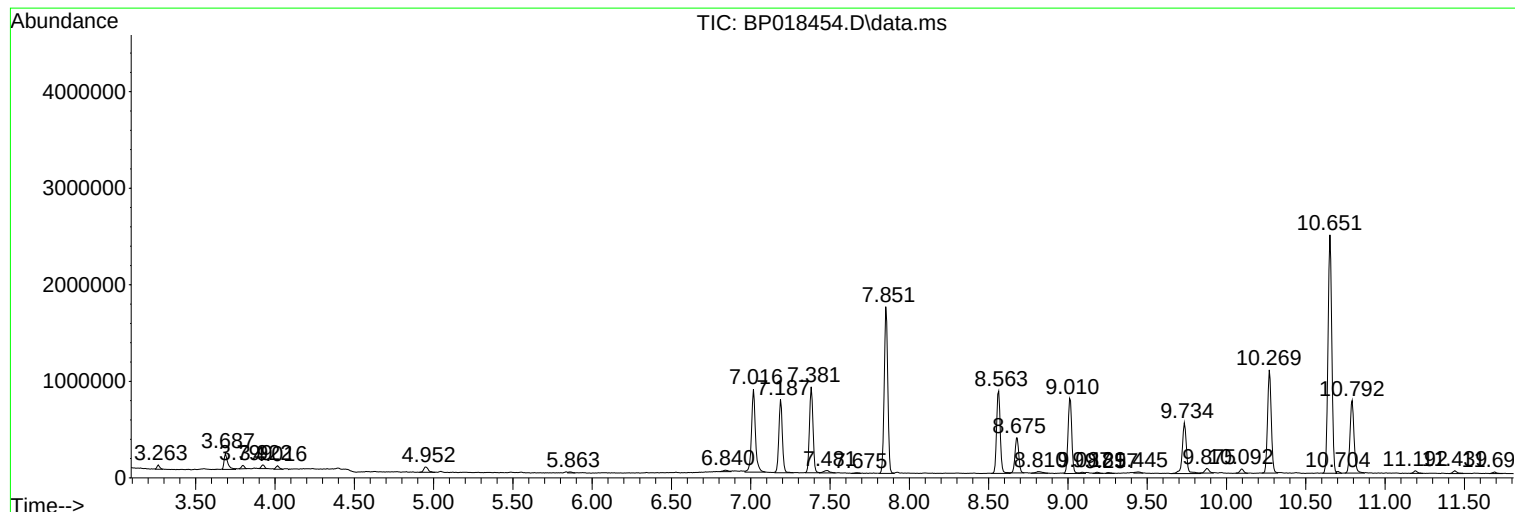

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018454.D
Acq On : 28 Nov 2023 23:12
Operator : MA/JU
Sample : 05416-15
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COAH0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, bis(2-eth... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.745	7.10 ng/ul	1918750	Chrysene-d12	21.468

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	91
3			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
4			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	90
5			Adipic acid, 2-ethylhexyl octyl ...	370	C22H42O4	1000324-48-6	90

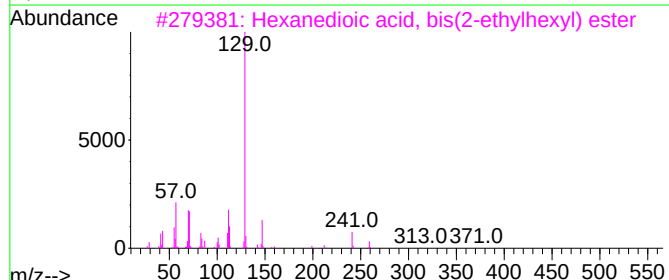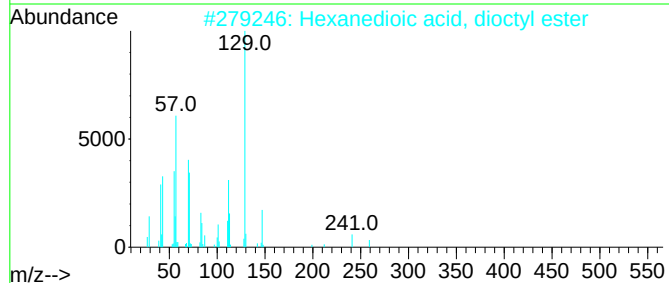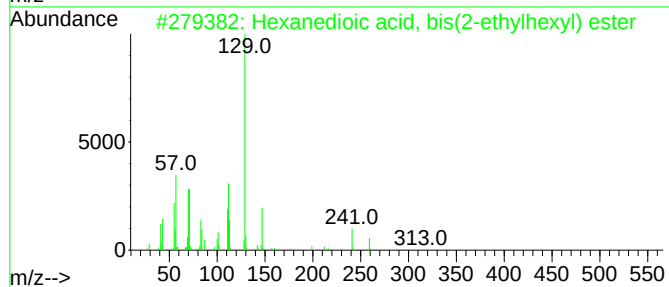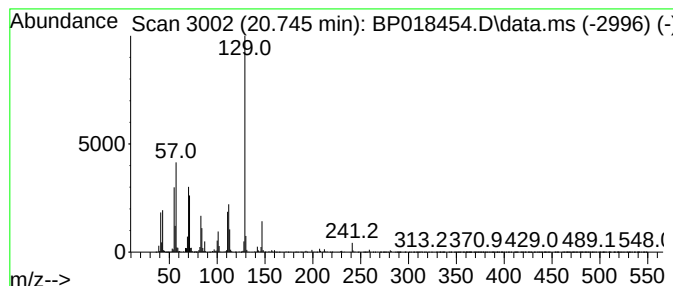

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018454.D
Acq On : 28 Nov 2023 23:12
Operator : MA/JU
Sample : 05416-15
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.745	7.1	ng/ul	1918750	5	21.468	5402680	20.0