

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018457.D
 Acq On : 29 Nov 2023 00:54
 Operator : MA/JU
 Sample : 05328-02
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49P9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	39	rVB	94200	118955	1.48%	0.157%
2	3.687	98	102	112	rBV	251187	372377	4.64%	0.490%
3	3.922	139	142	148	rVB3	20578	31405	0.39%	0.041%
4	4.016	154	158	162	rVB2	23452	33544	0.42%	0.044%
5	4.546	244	248	251	rBV6	5801	8589	0.11%	0.011%
6	4.581	251	254	261	rVB7	9162	14854	0.19%	0.020%
7	4.958	314	318	322	rVB6	7176	11221	0.14%	0.015%
8	5.940	477	485	490	rVB10	5795	12555	0.16%	0.017%
9	7.016	662	668	678	rVB	276831	441484	5.50%	0.581%
10	7.187	691	697	707	rVB	1272958	1933204	24.09%	2.546%
11	7.381	723	730	741	rBV	1131346	1743960	21.73%	2.296%
12	7.852	803	810	818	rBV	1724658	2670355	33.28%	3.516%
13	7.922	818	822	827	rVB4	10023	13643	0.17%	0.018%
14	8.563	921	931	943	rBV	792312	1283659	16.00%	1.690%
15	9.010	999	1007	1016	rBV	1325395	2146008	26.74%	2.826%
16	9.446	1076	1081	1087	rVB2	22522	38527	0.48%	0.051%
17	9.581	1101	1104	1113	rBV2	4037	10737	0.13%	0.014%
18	9.734	1119	1130	1145	rBV	955540	1554986	19.38%	2.048%
19	10.269	1213	1221	1232	rBV	1592932	2636830	32.86%	3.472%
20	10.651	1272	1286	1294	rBV	2283010	3777925	47.08%	4.975%
21	10.787	1301	1309	1327	rBV	1070432	1894098	23.60%	2.494%
22	11.940	1499	1505	1510	rVB8	7326	11469	0.14%	0.015%
23	12.240	1550	1556	1562	rBV	34512	58393	0.73%	0.077%
24	13.328	1735	1741	1746	rBV4	13793	20839	0.26%	0.027%
25	13.398	1746	1753	1758	rVV2	26121	45816	0.57%	0.060%
26	13.463	1760	1764	1769	rVB6	6464	8788	0.11%	0.012%
27	13.904	1832	1839	1850	rBV	3142816	4229405	52.70%	5.569%
28	14.181	1875	1886	1896	rBV	3605679	5238286	65.28%	6.898%
29	14.398	1920	1923	1926	rVB5	7721	8459	0.11%	0.011%
30	14.487	1929	1938	1949	rBV	3008242	4625176	57.64%	6.090%
31	14.681	1966	1971	1982	rBV	131028	228366	2.85%	0.301%
32	14.845	1993	1999	2003	rBV5	15983	29873	0.37%	0.039%
33	14.910	2006	2010	2014	rVB7	12293	20411	0.25%	0.027%
34	15.145	2048	2050	2056	rVB7	5681	8992	0.11%	0.012%
35	15.481	2101	2107	2121	rBV	4326286	6428872	80.11%	8.466%
36	15.598	2121	2127	2143	rVV	779486	1119178	13.95%	1.474%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018457.D
 Acq On : 29 Nov 2023 00:54
 Operator : MA/JU
 Sample : 05328-02
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49P9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	15.722	2145	2148	2153	rVB3	21301	29468	0.37%	0.039%
38	16.645	2302	2305	2309	rBV6	6890	9383	0.12%	0.012%
39	16.928	2348	2353	2356	rBV7	7181	11983	0.15%	0.016%
40	17.122	2383	2386	2393	rBV9	9881	14188	0.18%	0.019%
41	17.245	2400	2407	2415	rBV	3274466	4700474	58.57%	6.190%
42	17.345	2418	2424	2436	rVB	4578789	6368729	79.36%	8.386%
43	18.163	2558	2563	2570	rBV	171926	252866	3.15%	0.333%
44	18.463	2608	2614	2621	rBV3	41285	80158	1.00%	0.106%
45	18.616	2636	2640	2646	rBV3	40546	58480	0.73%	0.077%
46	19.186	2733	2737	2742	rBV	58902	78275	0.98%	0.103%
47	19.251	2744	2748	2753	rVV	78121	106923	1.33%	0.141%
48	19.451	2778	2782	2789	rBV3	59362	92465	1.15%	0.122%
49	19.616	2804	2810	2819	rBV	5976587	8024894	100.00%	10.567%
50	21.492	3122	3129	3139	rVB	2825777	5389511	67.16%	7.097%
51	24.204	3576	3590	3607	rVB3	1469242	7892538	98.35%	10.393%




Sum of corrected areas: 75941574

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018457.D
Acq On : 29 Nov 2023 00:54
Operator : MA/JU
Sample : 05328-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49P9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

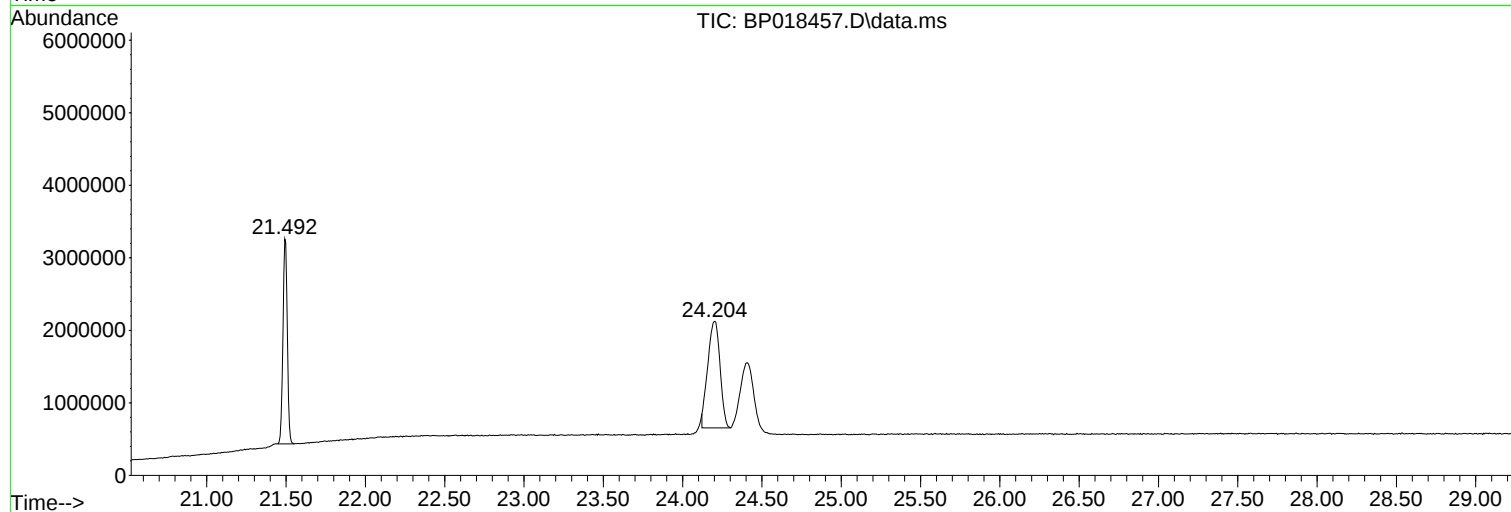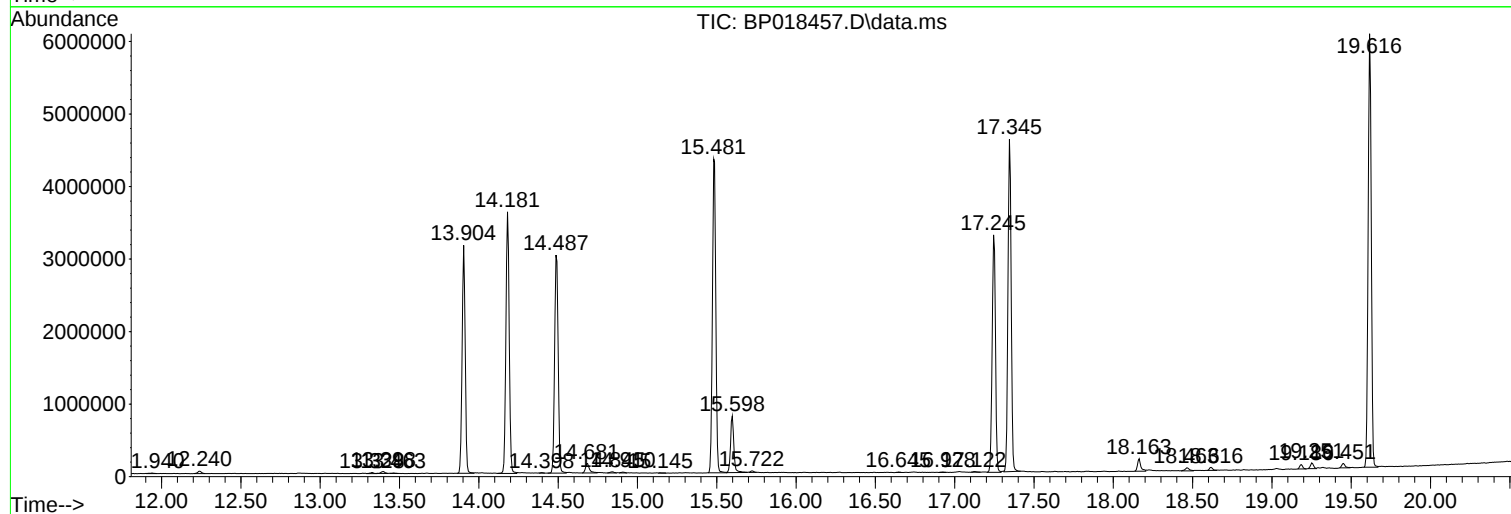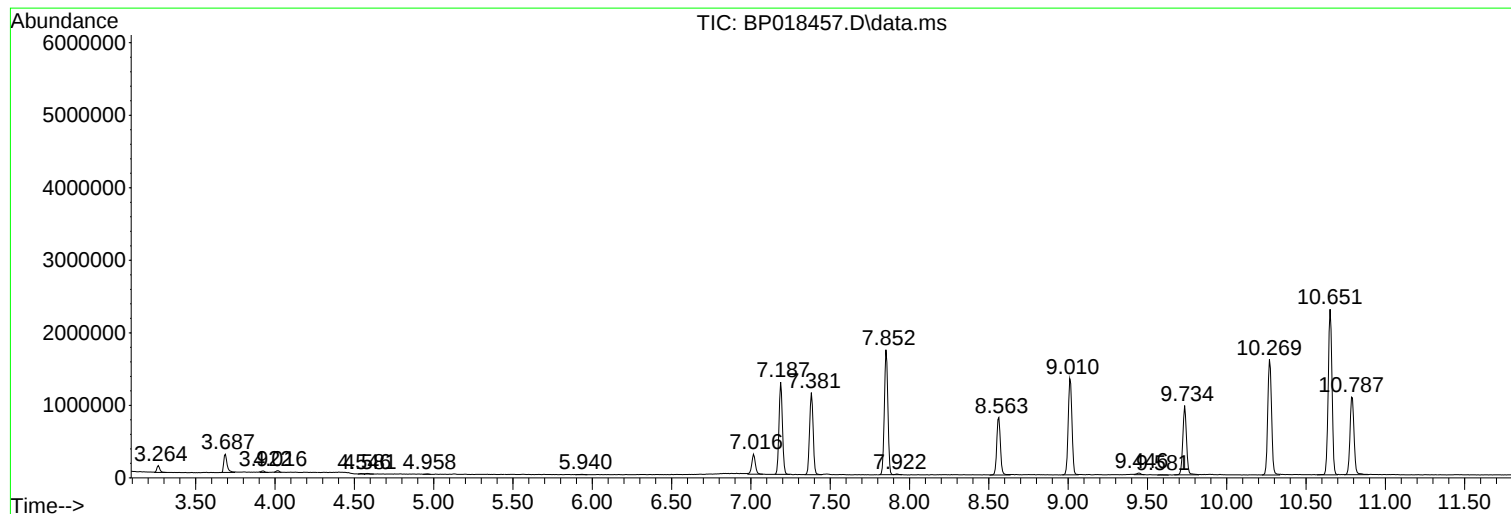

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018457.D
Acq On : 29 Nov 2023 00:54
Operator : MA/JU
Sample : 05328-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49P9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018457.D
Acq On : 29 Nov 2023 00:54
Operator : MA/JU
Sample : 05328-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49P9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc