

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018459.D
 Acq On : 29 Nov 2023 02:01
 Operator : MA/JU
 Sample : 05328-05
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	38	rVB	85735	115663	1.02%	0.124%
2	3.681	98	101	117	rBV	396431	623649	5.52%	0.667%
3	3.922	139	142	148	rVB	20792	30553	0.27%	0.033%
4	4.017	155	158	163	rVB	24431	32804	0.29%	0.035%
5	4.952	313	317	324	rVB4	6875	12845	0.11%	0.014%
6	5.128	344	347	354	rVB5	8751	14261	0.13%	0.015%
7	7.016	662	668	678	rVB	377633	604898	5.36%	0.647%
8	7.187	690	697	709	rVB	1575828	2396672	21.22%	2.562%
9	7.381	722	730	738	rBV	1433112	2210005	19.57%	2.362%
10	7.481	740	747	754	rVB8	13082	34593	0.31%	0.037%
11	7.852	802	810	817	rBV	1696416	2672387	23.66%	2.856%
12	7.922	817	822	830	rVB	18863	33524	0.30%	0.036%
13	8.563	922	931	939	rBV	1129583	1795296	15.89%	1.919%
14	9.010	999	1007	1017	rBV	1711274	2823765	25.00%	3.018%
15	9.181	1030	1036	1043	rBV	5867	11817	0.10%	0.013%
16	9.446	1071	1081	1087	rVB	76154	127235	1.13%	0.136%
17	9.734	1119	1130	1138	rBV	1254246	2038415	18.05%	2.179%
18	10.269	1214	1221	1237	rBV	2231668	3675106	32.54%	3.928%
19	10.651	1279	1286	1296	rVB	2491314	4120136	36.48%	4.404%
20	10.793	1301	1310	1320	rBV	1678180	2928981	25.93%	3.131%
21	11.440	1416	1420	1424	rBV7	8941	16772	0.15%	0.018%
22	11.940	1497	1505	1512	rBV	62473	101979	0.90%	0.109%
23	12.157	1537	1542	1547	rVB9	6032	11536	0.10%	0.012%
24	12.240	1550	1556	1563	rVB	48425	81823	0.72%	0.087%
25	12.681	1626	1631	1633	rBV6	8605	12572	0.11%	0.013%
26	12.863	1658	1662	1666	rBV7	6117	12589	0.11%	0.013%
27	13.104	1698	1703	1709	rVB8	7530	13782	0.12%	0.015%
28	13.328	1735	1741	1747	rVB2	30076	45065	0.40%	0.048%
29	13.398	1747	1753	1758	rBV2	48304	82875	0.73%	0.089%
30	13.463	1761	1764	1767	rVB5	9775	12653	0.11%	0.014%
31	13.904	1832	1839	1847	rBV	4499805	6476586	57.34%	6.922%
32	14.022	1857	1859	1864	rVB6	9262	12701	0.11%	0.014%
33	14.181	1876	1886	1897	rBV	5215975	7688284	68.06%	8.217%
34	14.404	1918	1924	1928	rVB8	11329	20283	0.18%	0.022%
35	14.487	1931	1938	1949	rVV	3822566	5886456	52.11%	6.292%
36	14.569	1950	1952	1958	rVB7	10757	16583	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018459.D
 Acq On : 29 Nov 2023 02:01
 Operator : MA/JU
 Sample : 05328-05
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	14.681	1966	1971	1983	rBV	207689	350214	3.10%	0.374%
38	14.839	1993	1998	2005	rBV5	29001	57794	0.51%	0.062%
39	14.904	2006	2009	2016	rVB9	21891	38202	0.34%	0.041%
40	15.310	2073	2078	2082	rBV4	10705	19723	0.17%	0.021%
41	15.486	2101	2108	2120	rBV	6729385	9854964	87.25%	10.533%
42	15.598	2121	2127	2141	rVV	1386359	1882634	16.67%	2.012%
43	15.722	2145	2148	2154	rVB3	31382	45561	0.40%	0.049%
44	16.275	2239	2242	2246	rVB6	12228	14831	0.13%	0.016%
45	17.028	2366	2370	2374	rBV4	15716	24776	0.22%	0.026%
46	17.128	2383	2387	2390	rBV4	17368	20009	0.18%	0.021%
47	17.245	2401	2407	2418	rVV	4314797	6481180	57.38%	6.927%
48	17.351	2418	2425	2437	rVV2	6830368	10046938	88.94%	10.738%
49	17.433	2437	2439	2444	rVB6	12500	17978	0.16%	0.019%
50	17.633	2468	2473	2479	rBV5	9623	19122	0.17%	0.020%
51	17.945	2522	2526	2531	rVB7	14387	25125	0.22%	0.027%
52	18.169	2558	2564	2572	rBV2	383595	572605	5.07%	0.612%
53	18.469	2610	2615	2621	rBV4	44496	74368	0.66%	0.079%
54	18.622	2637	2641	2649	rVB2	69840	99778	0.88%	0.107%
55	19.033	2709	2711	2718	rVB8	19330	27438	0.24%	0.029%
56	19.186	2733	2737	2744	rBV2	96646	134399	1.19%	0.144%
57	19.257	2745	2749	2754	rBV	112623	163095	1.44%	0.174%
58	19.463	2780	2784	2791	rBV2	95623	154508	1.37%	0.165%
59	19.622	2805	2811	2822	rBV	8066459	11295686	100.00%	12.073%
60	21.516	3126	3133	3144	rVB	2560288	5345121	47.32%	5.713%




Sum of corrected areas: 93561193

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018459.D
Acq On : 29 Nov 2023 02:01
Operator : MA/JU
Sample : 05328-05
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49T6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

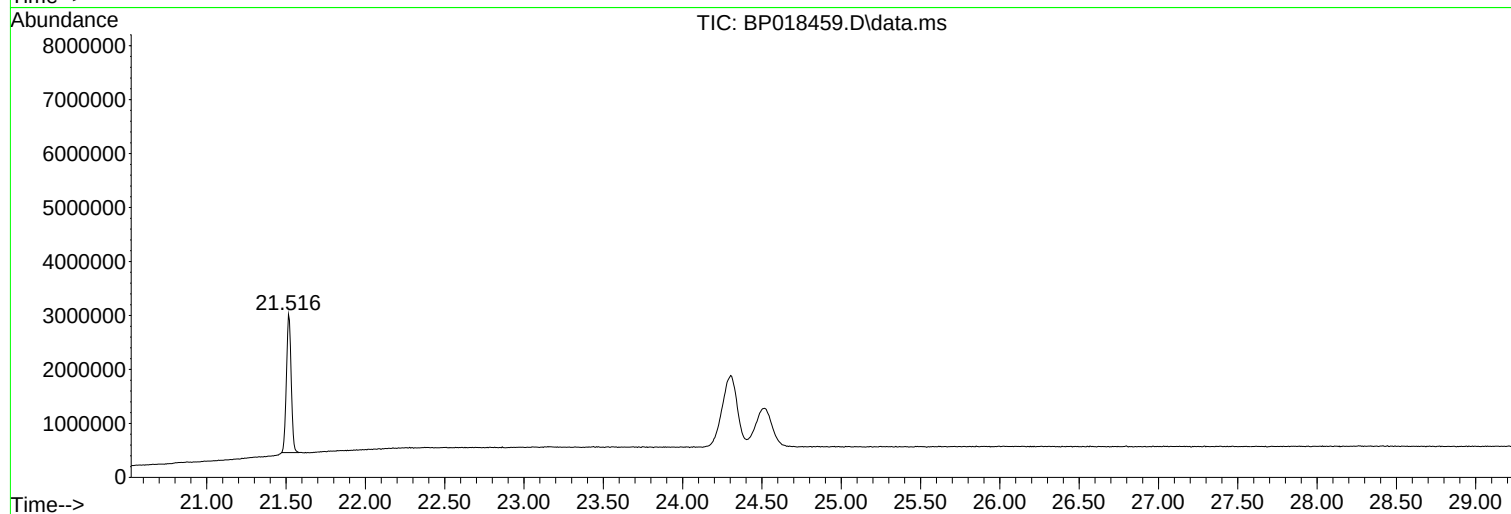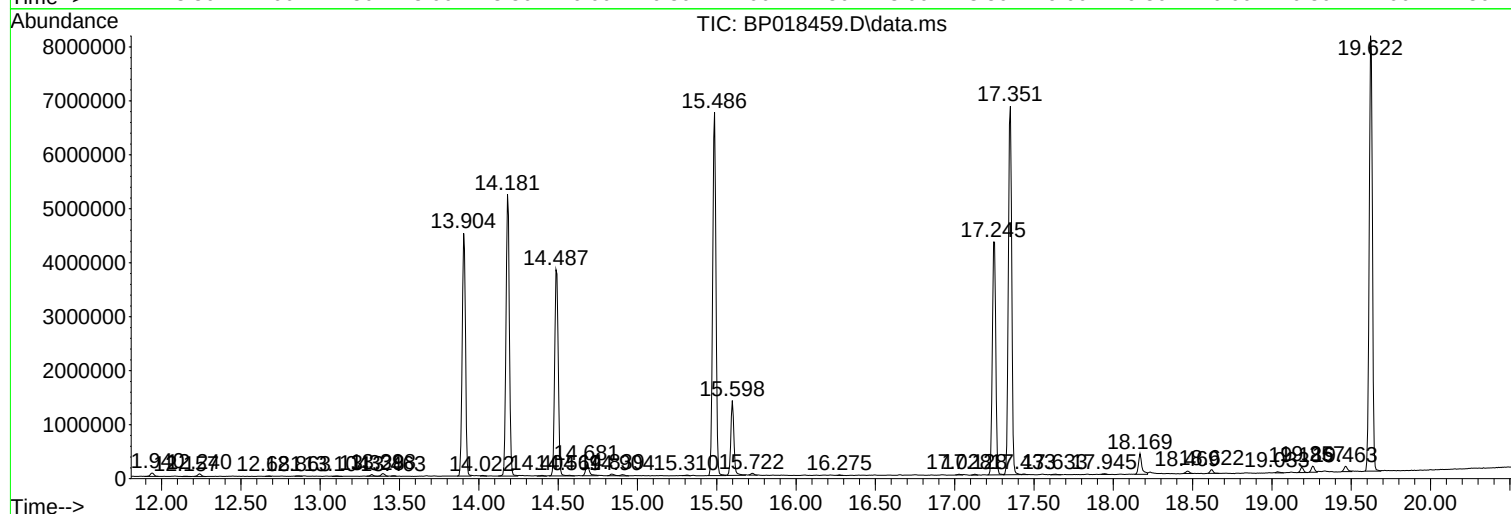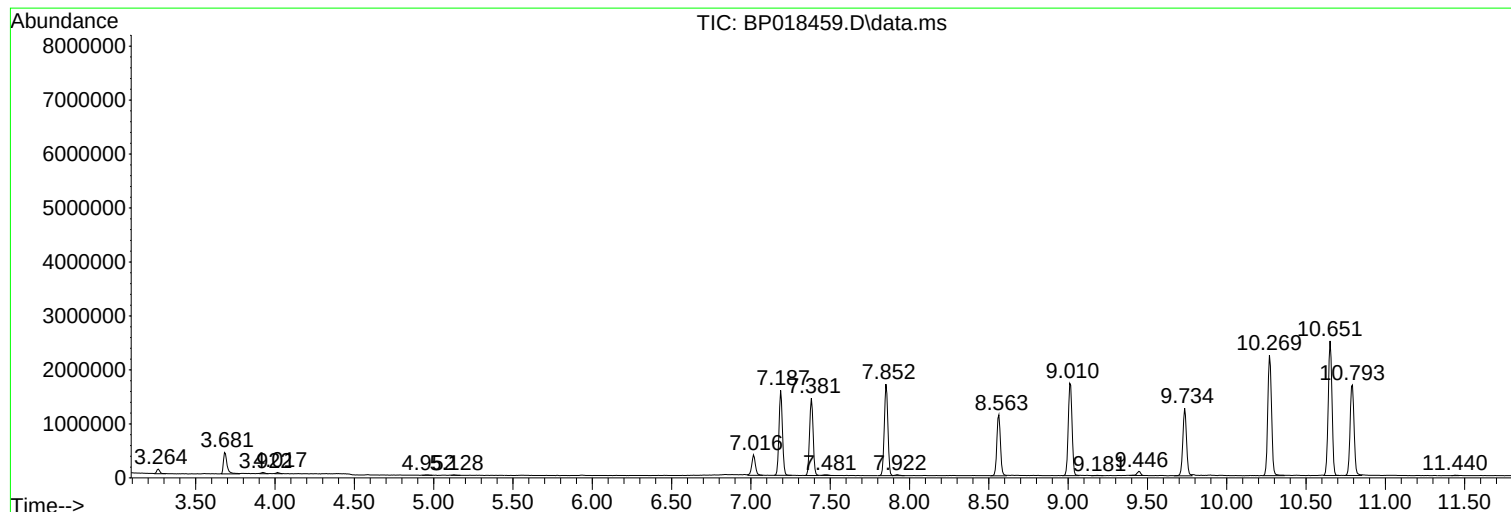

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018459.D
Acq On : 29 Nov 2023 02:01
Operator : MA/JU
Sample : 05328-05
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49T6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018459.D
Acq On : 29 Nov 2023 02:01
Operator : MA/JU
Sample : 05328-05
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49T6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc