

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018460.D
 Acq On : 29 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05328-07
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	42	rVB	89241	133517	1.12%	0.147%
2	3.687	97	102	112	rBV	268236	455307	3.81%	0.502%
3	3.922	139	142	147	rVB4	17742	24273	0.20%	0.027%
4	4.017	154	158	163	rVB	19585	28843	0.24%	0.032%
5	7.016	662	668	678	rVB	355335	559434	4.69%	0.617%
6	7.187	689	697	709	rVB	1448810	2197623	18.41%	2.425%
7	7.381	723	730	738	rBV	1301521	2027943	16.99%	2.238%
8	7.481	740	747	754	rVB10	11439	26309	0.22%	0.029%
9	7.852	803	810	817	rBV	1642108	2571687	21.54%	2.838%
10	7.922	817	822	825	rVB2	10154	14185	0.12%	0.016%
11	8.563	920	931	940	rBV	1014486	1636209	13.70%	1.806%
12	9.010	999	1007	1016	rBV	1581882	2590952	21.70%	2.859%
13	9.187	1032	1037	1042	rVB9	8737	15259	0.13%	0.017%
14	9.446	1075	1081	1090	rVB	74395	128334	1.07%	0.142%
15	9.734	1119	1130	1137	rBV	1141716	1845599	15.46%	2.037%
16	10.269	1213	1221	1239	rBV	2037460	3363800	28.17%	3.712%
17	10.652	1278	1286	1294	rVB	2393673	4019131	33.66%	4.435%
18	10.787	1301	1309	1324	rBV	1461395	2483315	20.80%	2.741%
19	11.446	1415	1421	1427	rBV10	7573	18158	0.15%	0.020%
20	11.940	1498	1505	1512	rVB2	46566	75762	0.63%	0.084%
21	12.240	1548	1556	1561	rBV2	41062	69863	0.59%	0.077%
22	13.322	1735	1740	1747	rBV2	19072	30296	0.25%	0.033%
23	13.398	1747	1753	1758	rVV	34318	55218	0.46%	0.061%
24	13.457	1760	1763	1769	rVV6	6973	12784	0.11%	0.014%
25	13.675	1796	1800	1805	rVB6	7975	12900	0.11%	0.014%
26	13.904	1832	1839	1850	rBV	4425587	6080658	50.93%	6.710%
27	14.022	1855	1859	1864	rVB8	7293	14838	0.12%	0.016%
28	14.181	1877	1886	1897	rBV	4851747	7075555	59.26%	7.808%
29	14.392	1918	1922	1928	rVB8	8094	13797	0.12%	0.015%
30	14.487	1931	1938	1948	rVV	3796693	5774856	48.37%	6.373%
31	14.569	1950	1952	1957	rVB6	11925	15919	0.13%	0.018%
32	14.687	1965	1972	1982	rBV	220732	376444	3.15%	0.415%
33	14.840	1993	1998	2003	rVV3	27347	42283	0.35%	0.047%
34	14.904	2005	2009	2014	rVB7	19388	29194	0.24%	0.032%
35	15.304	2072	2077	2078	rBV4	11193	13007	0.11%	0.014%
36	15.487	2101	2108	2121	rBV	6294616	9362103	78.41%	10.332%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018460.D
 Acq On : 29 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05328-07
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	15.598	2121	2127	2144	rVV	1369899	1871502	15.67%	2.065%
38	15.722	2144	2148	2158	rVB	31941	57645	0.48%	0.064%
39	16.275	2238	2242	2246	rVB6	11319	15879	0.13%	0.018%
40	16.651	2303	2306	2311	rBV7	11748	16263	0.14%	0.018%
41	17.028	2365	2370	2374	rBV4	19324	35566	0.30%	0.039%
42	17.128	2383	2387	2392	rBV5	21713	27994	0.23%	0.031%
43	17.251	2401	2408	2418	rBV	4602214	6572455	55.05%	7.253%
44	17.351	2418	2425	2437	rVB	6791061	9761516	81.76%	10.773%
45	17.951	2523	2527	2532	rVB8	10300	14620	0.12%	0.016%
46	18.039	2539	2542	2548	rBV7	11968	20884	0.17%	0.023%
47	18.175	2559	2565	2573	rBV	322385	513824	4.30%	0.567%
48	18.469	2610	2615	2623	rBV3	72623	123113	1.03%	0.136%
49	18.622	2636	2641	2647	rBV2	77384	115242	0.97%	0.127%
50	19.039	2709	2712	2720	rVB3	38715	58989	0.49%	0.065%
51	19.192	2734	2738	2745	rBV2	92770	125025	1.05%	0.138%
52	19.263	2745	2750	2755	rBV	123108	181120	1.52%	0.200%
53	19.480	2782	2787	2793	rBV3	102919	189647	1.59%	0.209%
54	19.628	2806	2812	2824	rBV	8436057	11939596	100.00%	13.176%
55	21.545	3130	3138	3149	rBV2	2478610	5778060	48.39%	6.377%




Sum of corrected areas: 90614295

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018460.D
Acq On : 29 Nov 2023 02:35
Operator : MA/JU
Sample : 05328-07
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

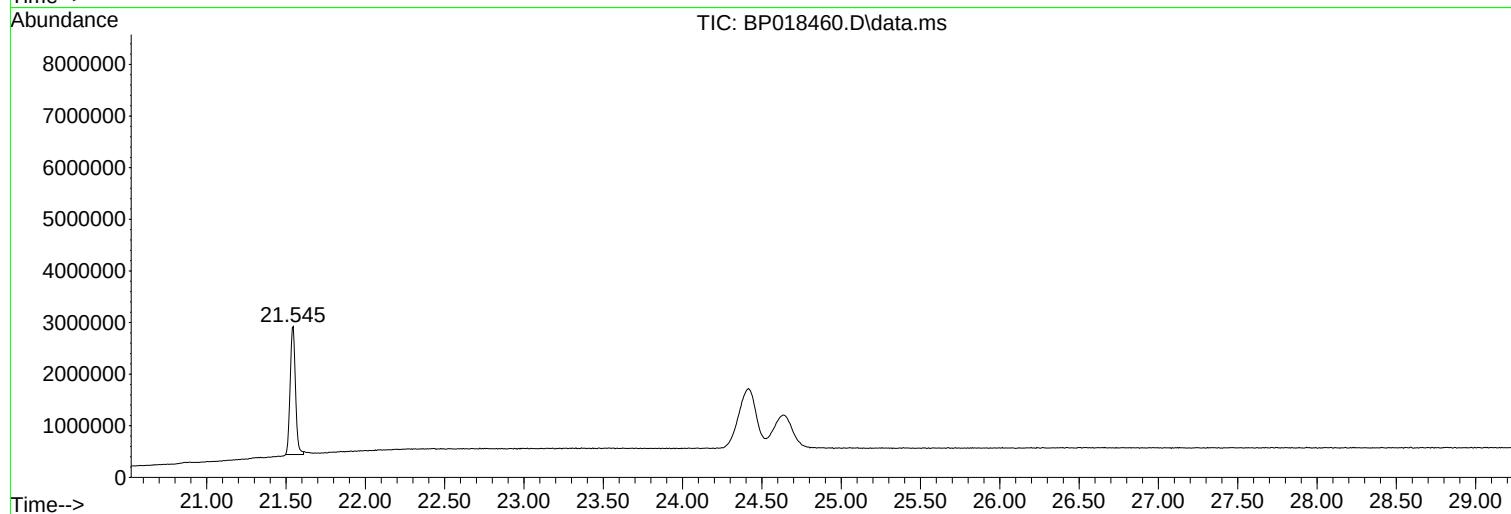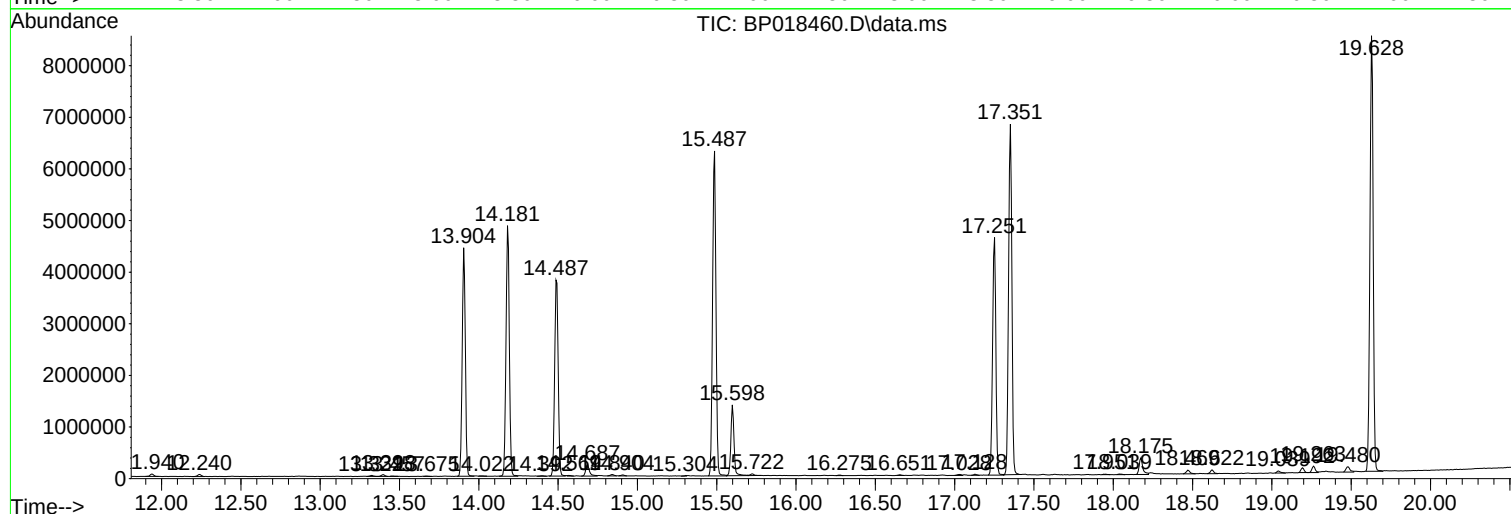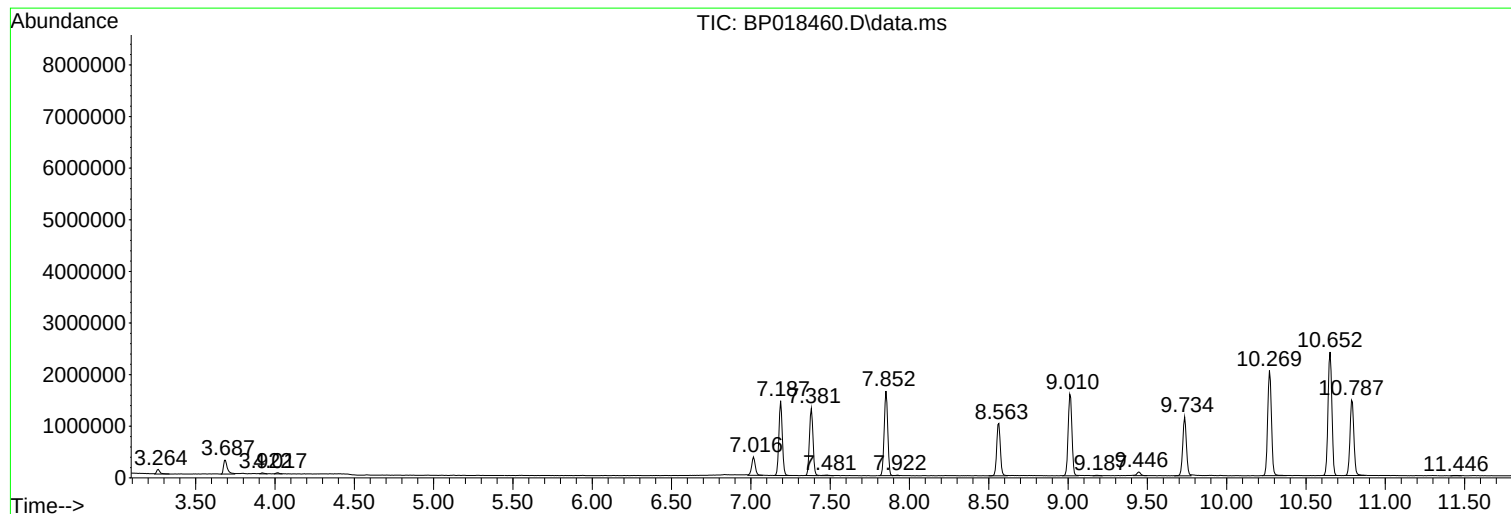

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018460.D
Acq On : 29 Nov 2023 02:35
Operator : MA/JU
Sample : 05328-07
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018460.D
Acq On : 29 Nov 2023 02:35
Operator : MA/JU
Sample : 05328-07
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc