

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018461.D
 Acq On : 29 Nov 2023 03:09
 Operator : MA/JU
 Sample : 05416-16
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	36	rVB	41817	56705	0.94%	0.096%
2	3.552	76	79	82	rBV2	9960	9774	0.16%	0.017%
3	3.687	98	102	115	rBV	168268	268120	4.43%	0.454%
4	3.799	117	121	128	rVB2	19503	30146	0.50%	0.051%
5	3.922	137	142	148	rVB	37824	62225	1.03%	0.105%
6	4.017	154	158	162	rVB2	36268	48432	0.80%	0.082%
7	4.399	220	223	228	rVB5	10099	11529	0.19%	0.020%
8	4.952	311	317	326	rVB2	53731	103362	1.71%	0.175%
9	5.487	403	408	414	rVB7	5669	13600	0.22%	0.023%
10	5.840	463	468	470	rBV4	8994	15591	0.26%	0.026%
11	6.534	580	586	590	rBV6	12028	20896	0.35%	0.035%
12	6.840	634	638	641	rBV4	15554	21935	0.36%	0.037%
13	7.016	659	668	683	rVB	864427	1448636	23.95%	2.452%
14	7.187	689	697	708	rVB	747870	1145624	18.94%	1.939%
15	7.381	723	730	737	rVV	867944	1342321	22.19%	2.272%
16	7.475	740	746	755	rVB4	20304	54120	0.89%	0.092%
17	7.852	803	810	818	rBV	1715726	2644834	43.73%	4.477%
18	7.922	818	822	825	rVV4	10360	14082	0.23%	0.024%
19	8.563	922	931	938	rBV	839911	1341416	22.18%	2.271%
20	8.675	944	950	957	rBV	283795	447547	7.40%	0.758%
21	8.816	968	974	975	rBV5	10155	14400	0.24%	0.024%
22	9.010	1000	1007	1016	rVV	797699	1280464	21.17%	2.168%
23	9.087	1016	1020	1023	rVV6	7627	13413	0.22%	0.023%
24	9.116	1023	1025	1032	rVV8	6770	13430	0.22%	0.023%
25	9.181	1032	1036	1041	rVV8	7880	12993	0.21%	0.022%
26	9.257	1043	1049	1054	rVB8	8032	12885	0.21%	0.022%
27	9.446	1071	1081	1091	rVB5	17039	50151	0.83%	0.085%
28	9.734	1116	1130	1137	rBV	570380	967163	15.99%	1.637%
29	9.875	1148	1154	1161	rBV	37835	68651	1.13%	0.116%
30	9.963	1164	1169	1175	rVB10	6817	11402	0.19%	0.019%
31	10.093	1183	1191	1198	rBV	36637	69951	1.16%	0.118%
32	10.269	1214	1221	1232	rBV	1116171	1780701	29.44%	3.015%
33	10.575	1266	1273	1275	rBV7	3410	8134	0.13%	0.014%
34	10.651	1278	1286	1293	rBV	2428663	4031562	66.65%	6.825%
35	10.787	1302	1309	1325	rBV	815505	1467671	24.26%	2.485%
36	11.193	1372	1378	1384	rVB3	24723	39557	0.65%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018461.D
 Acq On : 29 Nov 2023 03:09
 Operator : MA/JU
 Sample : 05416-16
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	11.440	1414	1420	1428	rBV2	26097	50374	0.83%	0.085%
38	11.687	1456	1462	1468	rVB8	11192	19192	0.32%	0.032%
39	11.946	1498	1506	1511	rVB8	7561	16926	0.28%	0.029%
40	12.016	1514	1518	1524	rVV5	12495	19731	0.33%	0.033%
41	12.087	1524	1530	1533	rVB5	9891	15490	0.26%	0.026%
42	12.240	1550	1556	1560	rVB3	19595	35041	0.58%	0.059%
43	12.310	1564	1568	1573	rVB2	25282	36935	0.61%	0.063%
44	12.534	1601	1606	1611	rVB4	17555	26607	0.44%	0.045%
45	12.863	1657	1662	1665	rBV7	6085	10213	0.17%	0.017%
46	13.328	1735	1741	1746	rBB4	19885	30149	0.50%	0.051%
47	13.398	1747	1753	1758	rBV	80001	128550	2.13%	0.218%
48	13.651	1787	1796	1797	rBV9	10716	21880	0.36%	0.037%
49	13.816	1817	1824	1828	rVV3	25883	44479	0.74%	0.075%
50	13.863	1828	1832	1833	rVV3	13899	14229	0.24%	0.024%
51	13.904	1833	1839	1849	rVV	2053088	2862652	47.33%	4.846%
52	13.981	1849	1852	1856	rVV5	9851	14774	0.24%	0.025%
53	14.040	1859	1862	1871	rVB10	7419	17353	0.29%	0.029%
54	14.181	1875	1886	1899	rBV	2396470	3531732	58.39%	5.979%
55	14.398	1918	1923	1928	rVB5	18320	27854	0.46%	0.047%
56	14.492	1931	1939	1947	rBV	3703397	5632863	93.12%	9.536%
57	14.681	1965	1971	1986	rBV	445256	741150	12.25%	1.255%
58	14.816	1991	1994	1995	rVV3	10856	13992	0.23%	0.024%
59	14.840	1995	1998	2002	rVV4	18826	33289	0.55%	0.056%
60	14.910	2003	2010	2015	rVV6	40937	88593	1.46%	0.150%
61	14.963	2015	2019	2022	rVB4	7956	13523	0.22%	0.023%
62	15.163	2050	2053	2058	rVB6	8285	12479	0.21%	0.021%
63	15.304	2069	2077	2081	rBV9	8398	22426	0.37%	0.038%
64	15.351	2082	2085	2090	rVB4	16637	21701	0.36%	0.037%
65	15.481	2101	2107	2115	rBV	2969721	4373505	72.30%	7.404%
66	15.598	2121	2127	2138	rBV	389908	557778	9.22%	0.944%
67	15.722	2144	2148	2152	rBV	11149	15897	0.26%	0.027%
68	15.834	2164	2167	2172	rBV5	6923	11013	0.18%	0.019%
69	15.981	2188	2192	2199	rVB6	11603	24364	0.40%	0.041%
70	16.051	2199	2204	2211	rBV10	10514	26970	0.45%	0.046%
71	16.222	2229	2233	2235	rBV4	19934	24184	0.40%	0.041%
72	16.386	2256	2261	2268	rVV4	9438	21402	0.35%	0.036%
73	16.545	2283	2288	2294	rBV9	10353	20959	0.35%	0.035%
74	16.792	2326	2330	2336	rVV2	30214	45361	0.75%	0.077%
75	17.028	2366	2370	2374	rVV5	25267	34028	0.56%	0.058%
76	17.075	2374	2378	2383	rVB8	7929	14541	0.24%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018461.D
 Acq On : 29 Nov 2023 03:09
 Operator : MA/JU
 Sample : 05416-16
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	17.251	2401	2408	2413	rVV	4286071	6048784	100.00%	10.240%
78	17.292	2413	2415	2419	rVV	78017	94853	1.57%	0.161%
79	17.351	2419	2425	2437	rVV	3082522	4272523	70.63%	7.233%
80	17.451	2438	2442	2448	rVB5	38597	57435	0.95%	0.097%
81	17.633	2470	2473	2476	rBV5	6569	9694	0.16%	0.016%
82	17.781	2495	2498	2502	rVB4	20191	27083	0.45%	0.046%
83	17.916	2518	2521	2524	rBV4	13872	17678	0.29%	0.030%
84	17.957	2524	2528	2534	rVB7	14468	20586	0.34%	0.035%
85	18.033	2536	2541	2543	rBV4	20882	29423	0.49%	0.050%
86	18.128	2555	2557	2561	rVB	12395	14361	0.24%	0.024%
87	18.175	2561	2565	2571	rBV	202292	288879	4.78%	0.489%
88	18.316	2585	2589	2593	rBV5	19172	28887	0.48%	0.049%
89	18.475	2611	2616	2622	rBV7	39571	69429	1.15%	0.118%
90	18.622	2636	2641	2645	rBV7	24049	43704	0.72%	0.074%
91	18.728	2656	2659	2663	rBV2	35157	47106	0.78%	0.080%
92	18.957	2694	2698	2702	rBV	45373	58389	0.97%	0.099%
93	18.998	2702	2705	2708	rBV3	21152	25719	0.43%	0.044%
94	19.086	2717	2720	2724	rBV4	57102	78149	1.29%	0.132%
95	19.128	2724	2727	2731	rVB4	30949	43618	0.72%	0.074%
96	19.198	2736	2739	2743	rVB4	46584	69871	1.16%	0.118%
97	19.298	2752	2756	2761	rVB	146128	205483	3.40%	0.348%
98	19.492	2786	2789	2794	rBV6	41313	69119	1.14%	0.117%
99	19.633	2807	2813	2822	rBV	3323397	4881857	80.71%	8.264%
100	21.569	3134	3142	3155	rBV2	1977834	4950711	81.85%	8.381%




Sum of corrected areas: 59070943

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018461.D
Acq On : 29 Nov 2023 03:09
Operator : MA/JU
Sample : 05416-16
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

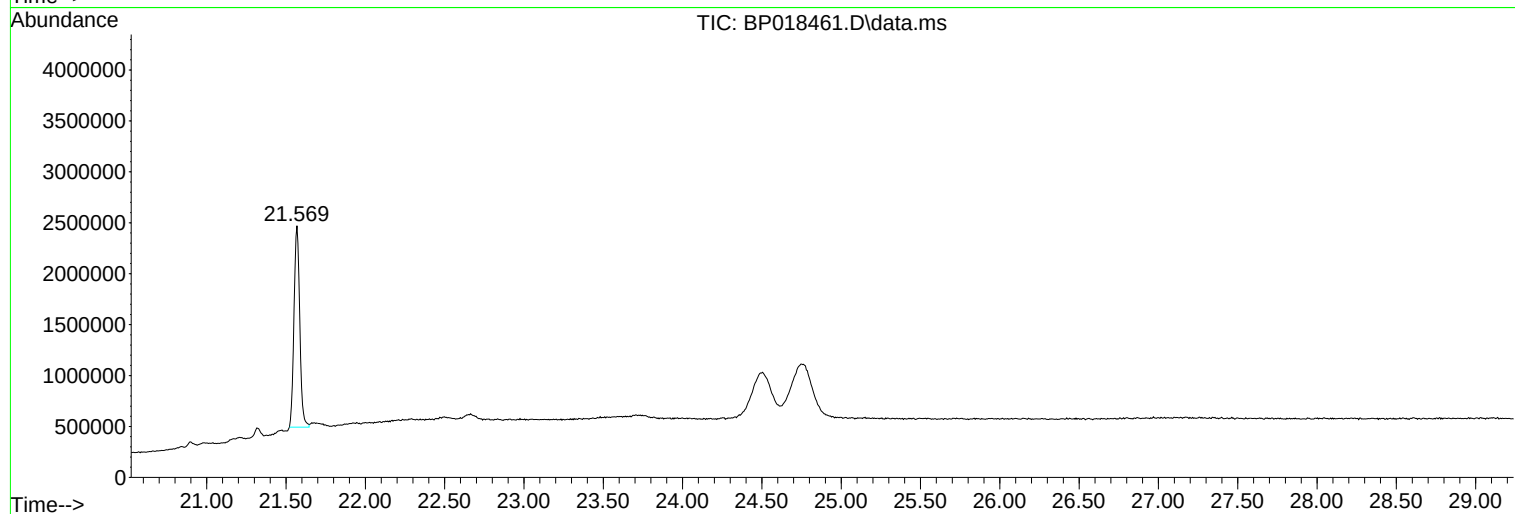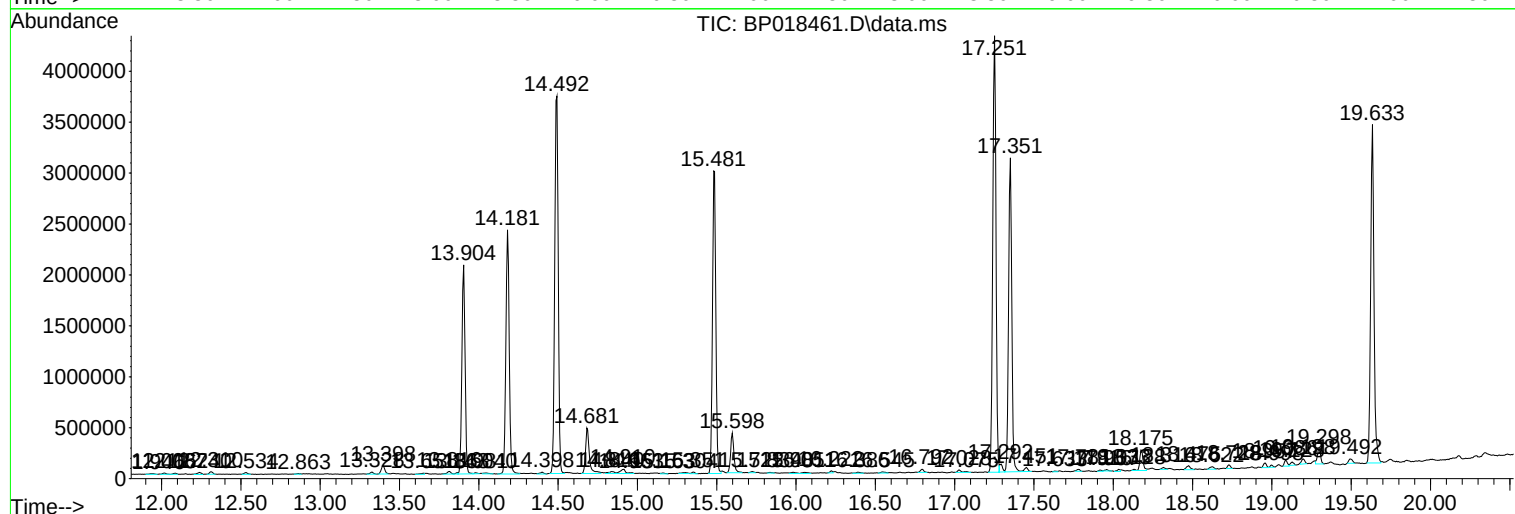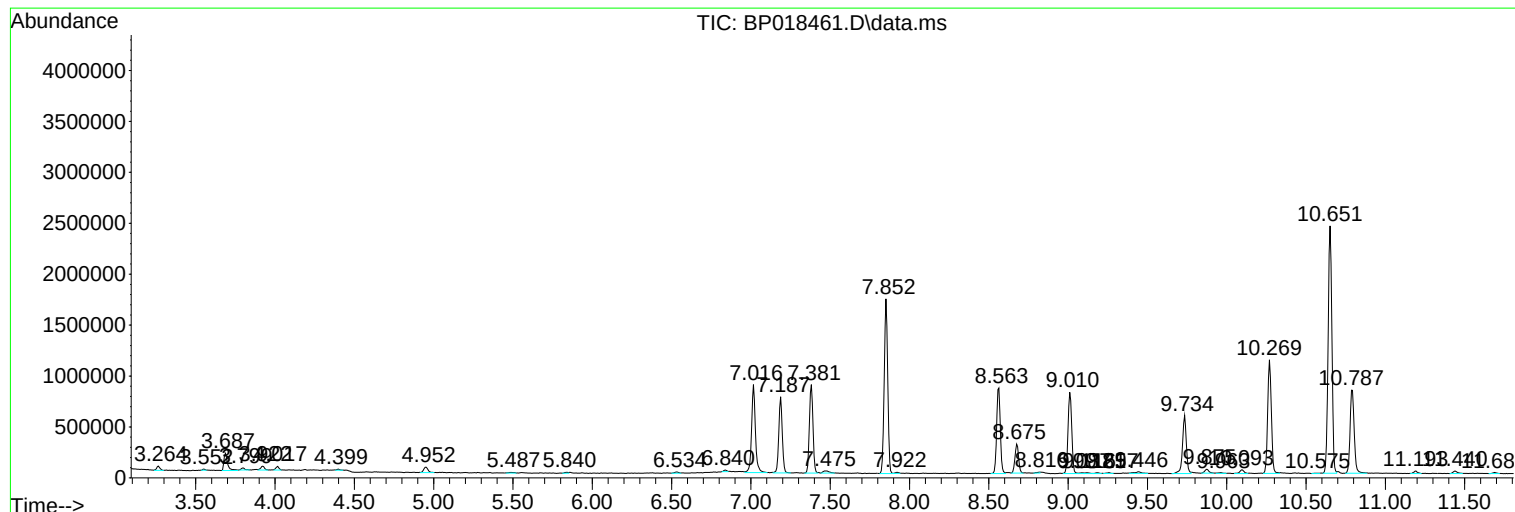

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018461.D
Acq On : 29 Nov 2023 03:09
Operator : MA/JU
Sample : 05416-16
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018461.D
Acq On : 29 Nov 2023 03:09
Operator : MA/JU
Sample : 05416-16
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc