

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018462.D
 Acq On : 29 Nov 2023 03:43
 Operator : MA/JU
 Sample : 05416-19
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	39	rVB	33889	47161	1.04%	0.121%
2	3.687	99	102	110	rBV	123988	186497	4.12%	0.477%
3	3.799	118	121	126	rVB4	16932	21019	0.46%	0.054%
4	3.923	138	142	149	rVB	41466	66795	1.47%	0.171%
5	4.017	154	158	164	rVB	33178	46423	1.02%	0.119%
6	4.952	310	317	322	rBV2	46263	87437	1.93%	0.224%
7	5.834	462	467	469	rBV5	6084	9031	0.20%	0.023%
8	5.858	469	471	476	rVB6	7526	8572	0.19%	0.022%
9	6.528	582	585	591	rVB8	4590	6855	0.15%	0.018%
10	6.834	634	637	638	rBV3	8288	8336	0.18%	0.021%
11	7.017	659	668	682	rVB	605189	1077144	23.77%	2.754%
12	7.187	691	697	705	rVB	543136	826444	18.24%	2.113%
13	7.381	723	730	739	rVB	633776	980509	21.64%	2.507%
14	7.487	743	748	755	rVB5	16113	32536	0.72%	0.083%
15	7.852	803	810	817	rBV	1478813	2296233	50.68%	5.872%
16	7.922	817	822	826	rVB3	5708	9793	0.22%	0.025%
17	8.093	845	851	856	rVB10	3049	7568	0.17%	0.019%
18	8.558	924	930	939	rVV	579954	928969	20.50%	2.376%
19	8.622	939	941	944	rVB4	8218	8875	0.20%	0.023%
20	8.675	944	950	957	rBV	197135	319152	7.04%	0.816%
21	8.811	966	973	979	rVV4	12654	33599	0.74%	0.086%
22	9.011	1000	1007	1016	rBV	538543	865895	19.11%	2.214%
23	9.122	1023	1026	1030	rVB6	6172	9095	0.20%	0.023%
24	9.181	1032	1036	1041	rVB7	9444	14122	0.31%	0.036%
25	9.440	1078	1080	1086	rVB6	12515	18799	0.41%	0.048%
26	9.687	1117	1122	1123	rBV4	7766	8540	0.19%	0.022%
27	9.734	1123	1130	1141	rVB	344328	574564	12.68%	1.469%
28	9.869	1148	1153	1160	rBV2	23484	41815	0.92%	0.107%
29	10.093	1186	1191	1198	rVB	29799	51803	1.14%	0.132%
30	10.269	1212	1221	1231	rVV	670896	1106998	24.43%	2.831%
31	10.352	1233	1235	1242	rVB8	4909	7724	0.17%	0.020%
32	10.428	1242	1248	1251	rBV8	3913	7870	0.17%	0.020%
33	10.652	1277	1286	1293	rBV	1927502	3175099	70.08%	8.119%
34	10.787	1301	1309	1318	rBV	486534	840883	18.56%	2.150%
35	11.193	1371	1378	1386	rBV6	18049	36336	0.80%	0.093%
36	11.440	1415	1420	1428	rBV2	14987	33323	0.74%	0.085%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018462.D
 Acq On : 29 Nov 2023 03:43
 Operator : MA/JU
 Sample : 05416-19
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	11.563	1439	1441	1451	rVB2	4356	7070	0.16%	0.018%
38	11.687	1458	1462	1467	rBV8	9905	15018	0.33%	0.038%
39	11.934	1499	1504	1512	rVB10	11581	23360	0.52%	0.060%
40	12.022	1512	1519	1523	rBV7	11083	21912	0.48%	0.056%
41	12.081	1523	1529	1534	rVV6	9381	17670	0.39%	0.045%
42	12.152	1537	1541	1545	rVB7	3860	6915	0.15%	0.018%
43	12.240	1551	1556	1561	rBV5	9180	15602	0.34%	0.040%
44	12.310	1564	1568	1573	rVB3	14847	21827	0.48%	0.056%
45	12.528	1602	1605	1609	rVB2	10360	12611	0.28%	0.032%
46	13.322	1736	1740	1745	rVV4	14639	18681	0.41%	0.048%
47	13.393	1747	1752	1761	rVV	53711	88918	1.96%	0.227%
48	13.457	1761	1763	1767	rVB5	4530	5677	0.13%	0.015%
49	13.816	1815	1824	1827	rVV8	15366	27455	0.61%	0.070%
50	13.904	1829	1839	1846	rBV	1124663	1523272	33.62%	3.895%
51	13.987	1850	1853	1856	rVB5	6650	7628	0.17%	0.020%
52	14.046	1861	1863	1866	rVB4	5964	5863	0.13%	0.015%
53	14.181	1878	1886	1898	rBV	1362326	1981058	43.73%	5.066%
54	14.328	1908	1911	1919	rVB10	4719	9168	0.20%	0.023%
55	14.399	1919	1923	1928	rBV5	11126	14180	0.31%	0.036%
56	14.487	1931	1938	1946	rBV	2487658	3759105	82.97%	9.613%
57	14.687	1965	1972	1980	rBV	212897	366149	8.08%	0.936%
58	14.846	1995	1999	2003	rVB7	10992	18150	0.40%	0.046%
59	14.916	2003	2011	2017	rVV8	24206	48541	1.07%	0.124%
60	14.969	2017	2020	2025	rVB7	5673	7921	0.17%	0.020%
61	15.298	2075	2076	2081	rVV5	8015	11521	0.25%	0.029%
62	15.357	2082	2086	2091	rVB8	10899	16328	0.36%	0.042%
63	15.487	2101	2108	2115	rBV	1621405	2354767	51.97%	6.021%
64	15.534	2115	2116	2120	rVV4	14454	14754	0.33%	0.038%
65	15.598	2121	2127	2136	rVV	157946	228728	5.05%	0.585%
66	15.834	2162	2167	2169	rBV5	5355	7613	0.17%	0.019%
67	16.063	2203	2206	2211	rVB7	8137	14790	0.33%	0.038%
68	16.222	2228	2233	2235	rBV6	12966	17268	0.38%	0.044%
69	16.545	2283	2288	2294	rVB6	20561	32783	0.72%	0.084%
70	16.657	2304	2307	2312	rBV6	5384	6272	0.14%	0.016%
71	16.716	2312	2317	2319	rBV6	7684	8377	0.18%	0.021%
72	16.751	2321	2323	2326	rVV4	5910	5879	0.13%	0.015%
73	16.793	2326	2330	2334	rVB6	13112	21481	0.47%	0.055%
74	17.034	2367	2371	2374	rVV6	15394	22373	0.49%	0.057%
75	17.069	2376	2377	2381	rVV4	6323	6437	0.14%	0.016%
76	17.140	2385	2389	2394	rBV4	5786	11646	0.26%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018462.D
 Acq On : 29 Nov 2023 03:43
 Operator : MA/JU
 Sample : 05416-19
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	17.251	2401	2408	2414	rBV	2705065	3804503	83.97%	9.729%
78	17.292	2414	2415	2419	rVV	55816	58063	1.28%	0.148%
79	17.351	2419	2425	2437	rVV	1554077	2266297	50.02%	5.795%
80	17.457	2438	2443	2448	rVB9	21904	39121	0.86%	0.100%
81	17.787	2490	2499	2503	rBV8	15002	34619	0.76%	0.089%
82	17.922	2518	2522	2524	rBV5	8513	11958	0.26%	0.031%
83	18.040	2540	2542	2548	rVB5	11119	16516	0.36%	0.042%
84	18.134	2555	2558	2561	rBV	15324	15978	0.35%	0.041%
85	18.181	2561	2566	2573	rBV2	145793	201713	4.45%	0.516%
86	18.316	2586	2589	2593	rBV4	16192	19713	0.44%	0.050%
87	18.357	2593	2596	2600	rVB2	13380	15093	0.33%	0.039%
88	18.481	2614	2617	2623	rVB4	25287	31615	0.70%	0.081%
89	18.628	2638	2642	2646	rBV4	18309	31284	0.69%	0.080%
90	18.734	2656	2660	2667	rVB4	23036	35636	0.79%	0.091%
91	18.963	2695	2699	2702	rBV2	34536	47236	1.04%	0.121%
92	18.998	2703	2705	2710	rVB4	14675	16946	0.37%	0.043%
93	19.051	2710	2714	2717	rBV6	17614	24937	0.55%	0.064%
94	19.092	2717	2721	2724	rBV5	43604	55605	1.23%	0.142%
95	19.139	2726	2729	2734	rVV6	24122	37091	0.82%	0.095%
96	19.204	2737	2740	2747	rVV8	24752	62163	1.37%	0.159%
97	19.304	2753	2757	2761	rVB	95901	133065	2.94%	0.340%
98	19.510	2787	2792	2798	rBV8	49120	94170	2.08%	0.241%
99	19.639	2808	2814	2826	rBV	1924360	2915559	64.35%	7.456%
100	21.592	3137	3146	3160	rBV2	1656642	4530673	100.00%	11.586%




Sum of corrected areas: 39106136

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018462.D
Acq On : 29 Nov 2023 03:43
Operator : MA/JU
Sample : 05416-19
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

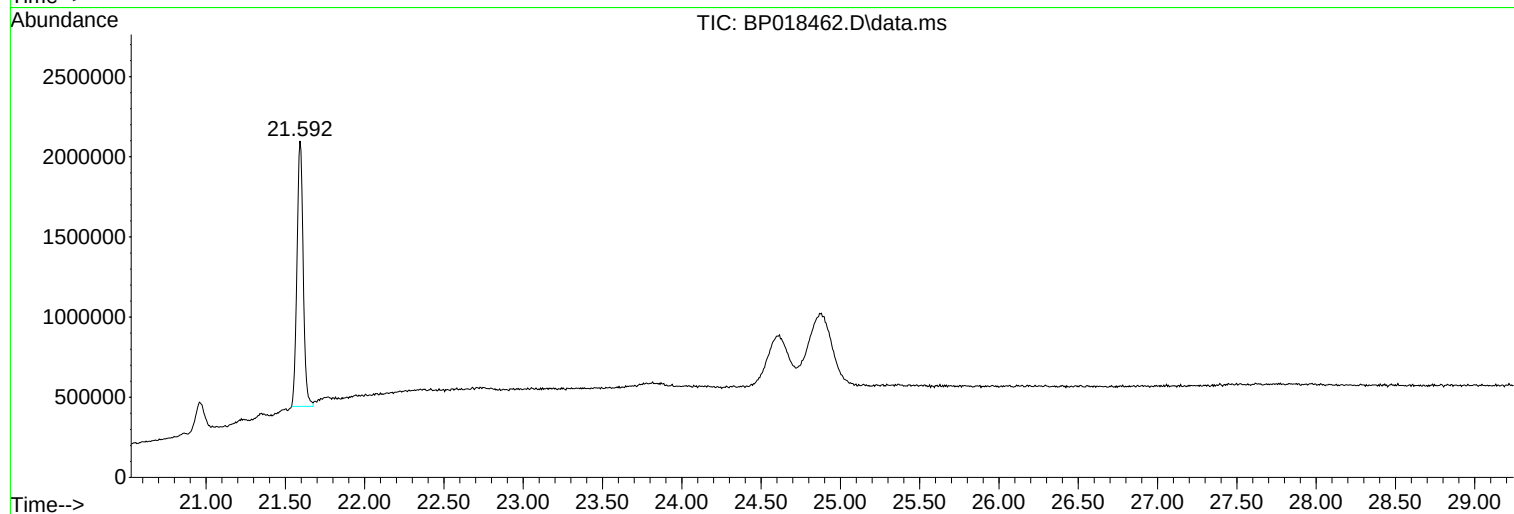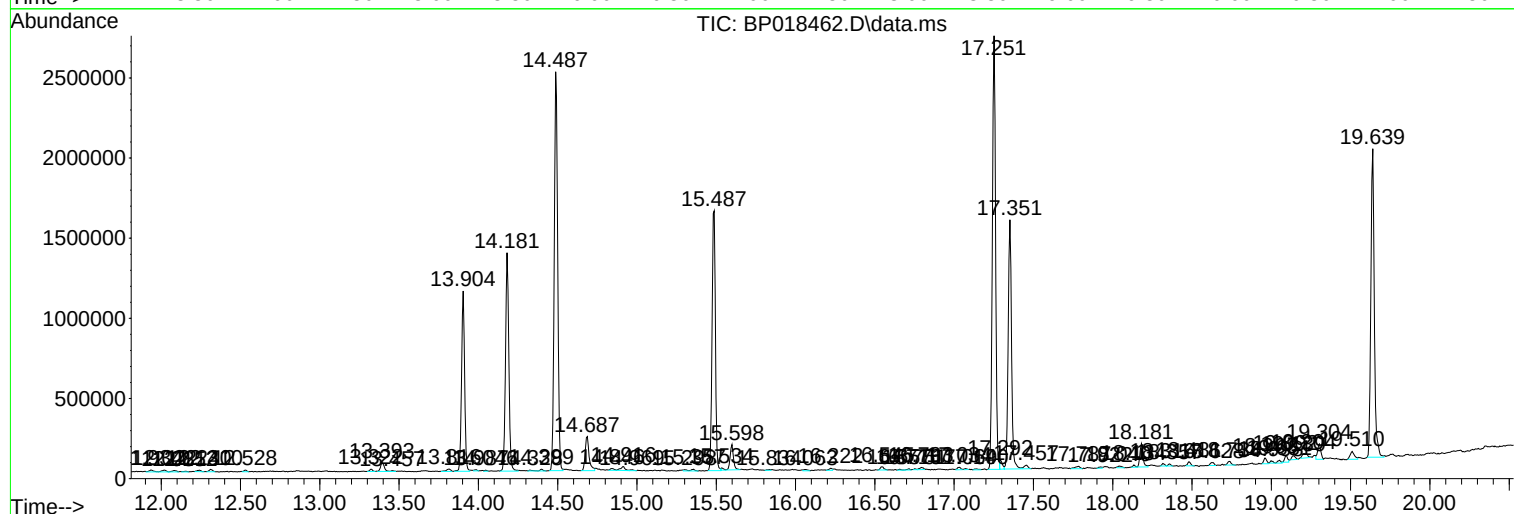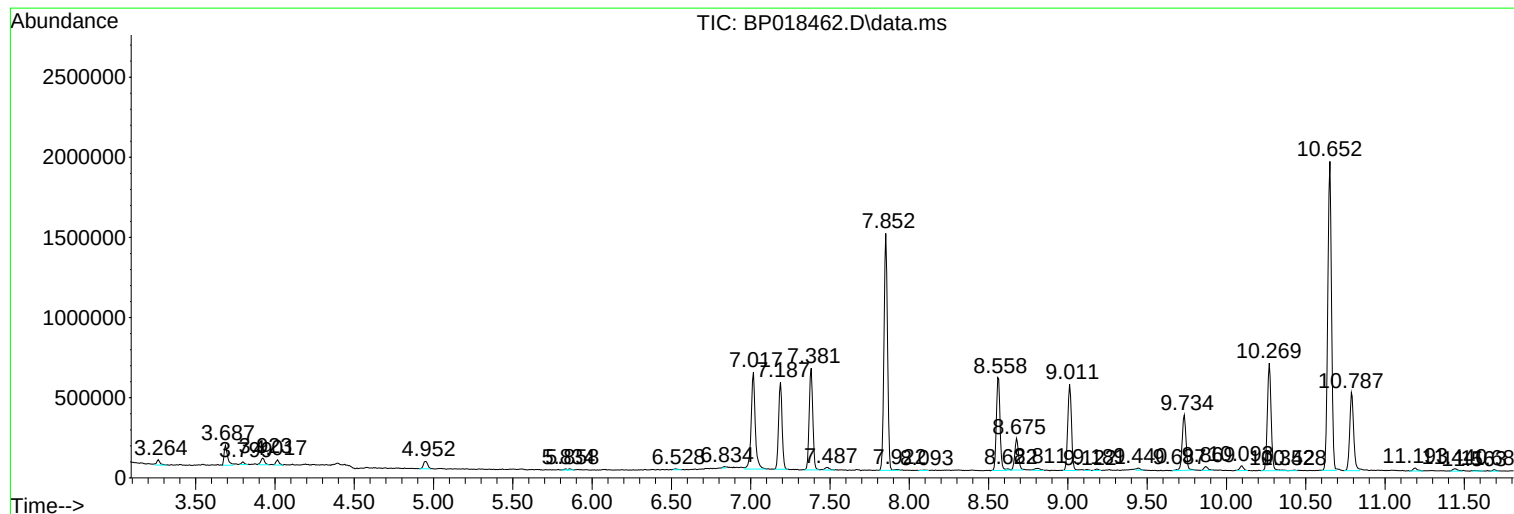

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018462.D
Acq On : 29 Nov 2023 03:43
Operator : MA/JU
Sample : 05416-19
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018462.D
Acq On : 29 Nov 2023 03:43
Operator : MA/JU
Sample : 05416-19
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc