

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018463.D
 Acq On : 29 Nov 2023 04:17
 Operator : MA/JU
 Sample : 05416-21
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018463.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	34	rBV	29213	34770	0.67%	0.075%
2	3.687	98	102	110	rBV	116029	175899	3.40%	0.379%
3	3.922	138	142	148	rVB	44048	67389	1.30%	0.145%
4	4.017	154	158	163	rVB	31337	36584	0.71%	0.079%
5	4.640	261	264	266	rBV4	5061	7260	0.14%	0.016%
6	4.946	311	316	325	rVB2	47600	95532	1.84%	0.206%
7	5.552	415	419	423	rBV7	5156	9434	0.18%	0.020%
8	5.834	463	467	469	rBV5	5794	7150	0.14%	0.015%
9	5.864	470	472	479	rVB8	5674	8184	0.16%	0.018%
10	5.934	482	484	491	rVB8	4665	7001	0.14%	0.015%
11	6.611	594	599	603	rBV8	3401	7300	0.14%	0.016%
12	6.840	635	638	640	rVV4	5949	8394	0.16%	0.018%
13	6.940	653	655	659	rBV5	4396	7369	0.14%	0.016%
14	7.016	660	668	681	rVB	599665	1008792	19.47%	2.173%
15	7.187	690	697	707	rVB	642417	978996	18.90%	2.109%
16	7.381	723	730	740	rVB	703277	1101351	21.26%	2.373%
17	7.481	740	747	751	rBV5	18368	37824	0.73%	0.081%
18	7.752	792	793	798	rVB5	5057	7343	0.14%	0.016%
19	7.852	802	810	817	rVV	1767975	2752965	53.14%	5.931%
20	7.922	819	822	826	rVB6	9107	12147	0.23%	0.026%
21	8.558	924	930	942	rBV	714539	1140945	22.02%	2.458%
22	8.675	944	950	958	rVV	173259	279586	5.40%	0.602%
23	8.816	968	974	985	rVB10	10956	40571	0.78%	0.087%
24	9.010	1000	1007	1018	rBV	643960	1035061	19.98%	2.230%
25	9.087	1018	1020	1023	rVV4	7803	9465	0.18%	0.020%
26	9.122	1023	1026	1033	rVB8	7722	12516	0.24%	0.027%
27	9.187	1033	1037	1043	rBV9	6427	11839	0.23%	0.026%
28	9.258	1043	1049	1052	rBV8	5736	7906	0.15%	0.017%
29	9.387	1063	1071	1072	rBV7	6395	11250	0.22%	0.024%
30	9.410	1072	1075	1076	rVV3	6677	7374	0.14%	0.016%
31	9.440	1076	1080	1085	rVB7	11749	22237	0.43%	0.048%
32	9.734	1119	1130	1138	rBV	410906	710621	13.72%	1.531%
33	9.869	1147	1153	1158	rBV	19877	36571	0.71%	0.079%
34	9.916	1158	1161	1166	rVV7	5047	8826	0.17%	0.019%
35	9.957	1166	1168	1174	rVB7	5737	7475	0.14%	0.016%
36	10.093	1185	1191	1199	rVB3	24967	47885	0.92%	0.103%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018463.D
 Acq On : 29 Nov 2023 04:17
 Operator : MA/JU
 Sample : 05416-21
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	10.269	1214	1221	1229	rBV	804576	1298509	25.07%	2.797%
38	10.652	1277	1286	1293	rBV	2384654	3942167	76.10%	8.493%
39	10.787	1301	1309	1323	rBV	659585	1169768	22.58%	2.520%
40	10.881	1323	1325	1329	rVV5	7236	7149	0.14%	0.015%
41	11.187	1372	1377	1384	rBV10	13983	27854	0.54%	0.060%
42	11.434	1415	1419	1426	rBV3	13900	31714	0.61%	0.068%
43	11.693	1456	1463	1466	rBV8	7936	11686	0.23%	0.025%
44	11.934	1497	1504	1508	rBV7	9135	19085	0.37%	0.041%
45	12.016	1511	1518	1521	rVV8	6407	11096	0.21%	0.024%
46	12.087	1525	1530	1535	rVB8	9631	16505	0.32%	0.036%
47	12.234	1548	1555	1559	rBV2	13467	20200	0.39%	0.044%
48	12.316	1564	1569	1574	rVB2	12553	18734	0.36%	0.040%
49	12.534	1600	1606	1610	rVB2	10271	15899	0.31%	0.034%
50	12.857	1657	1661	1669	rVV10	5956	14322	0.28%	0.031%
51	13.322	1737	1740	1745	rVB3	12397	16758	0.32%	0.036%
52	13.393	1745	1752	1757	rBV	47381	83686	1.62%	0.180%
53	13.457	1759	1763	1766	rVB6	5164	6993	0.13%	0.015%
54	13.710	1804	1806	1812	rVB7	5108	6834	0.13%	0.015%
55	13.810	1818	1823	1828	rVB8	13523	20669	0.40%	0.045%
56	13.904	1833	1839	1846	rVV	1446504	1945527	37.56%	4.191%
57	13.981	1849	1852	1857	rVB7	6920	9388	0.18%	0.020%
58	14.181	1879	1886	1897	rBV	1711107	2471588	47.71%	5.325%
59	14.393	1917	1922	1928	rVB7	10827	18038	0.35%	0.039%
60	14.487	1931	1938	1947	rBV	3368410	4909205	94.77%	10.576%
61	14.563	1947	1951	1957	rVB9	9963	16748	0.32%	0.036%
62	14.610	1957	1959	1964	rVB6	7093	8602	0.17%	0.019%
63	14.687	1966	1972	1978	rBV2	132899	222584	4.30%	0.480%
64	14.840	1995	1998	2002	rBV6	9519	14575	0.28%	0.031%
65	14.887	2002	2006	2007	rVV4	6212	9225	0.18%	0.020%
66	14.910	2007	2010	2017	rVV8	21599	34593	0.67%	0.075%
67	14.963	2017	2019	2025	rVV6	6840	8508	0.16%	0.018%
68	15.016	2025	2028	2034	rVB8	3789	7408	0.14%	0.016%
69	15.163	2051	2053	2060	rVB8	5399	7674	0.15%	0.017%
70	15.351	2083	2085	2089	rVB4	11727	11659	0.23%	0.025%
71	15.481	2101	2107	2121	rVV	2070204	2980623	57.54%	6.421%
72	15.598	2121	2127	2137	rVV	106870	167573	3.23%	0.361%
73	15.722	2142	2148	2149	rBV6	8730	12348	0.24%	0.027%
74	15.822	2160	2165	2166	rBV5	6508	9457	0.18%	0.020%
75	15.975	2189	2191	2195	rBV5	4148	6440	0.12%	0.014%
76	16.057	2200	2205	2206	rBV5	6704	10351	0.20%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
 Data File : BP018463.D
 Acq On : 29 Nov 2023 04:17
 Operator : MA/JU
 Sample : 05416-21
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	16.222	2230	2233	2236	rBV5	13092	16364	0.32%	0.035%
78	16.651	2303	2306	2309	rBV5	5739	7739	0.15%	0.017%
79	16.716	2312	2317	2319	rBV5	7058	12211	0.24%	0.026%
80	16.792	2327	2330	2336	rVB8	10770	16250	0.31%	0.035%
81	16.986	2358	2363	2364	rBV5	5787	9223	0.18%	0.020%
82	17.034	2367	2371	2374	rVV5	16847	24414	0.47%	0.053%
83	17.139	2384	2389	2392	rBV6	6580	12402	0.24%	0.027%
84	17.251	2401	2408	2414	rBV	3404624	4866438	93.94%	10.484%
85	17.351	2419	2425	2437	rVV	1982265	2831222	54.65%	6.099%
86	17.457	2438	2443	2448	rVB8	26698	42157	0.81%	0.091%
87	17.645	2470	2475	2477	rBV6	6679	10284	0.20%	0.022%
88	17.957	2523	2528	2531	rBV7	9797	16623	0.32%	0.036%
89	18.057	2538	2545	2551	rBV7	14623	40777	0.79%	0.088%
90	18.181	2562	2566	2571	rBV2	94160	137266	2.65%	0.296%
91	18.486	2614	2618	2622	rVB7	18237	25053	0.48%	0.054%
92	18.628	2639	2642	2646	rVB5	15723	23076	0.45%	0.050%
93	18.739	2658	2661	2665	rVB4	15432	20279	0.39%	0.044%
94	18.963	2696	2699	2703	rBV2	21606	27668	0.53%	0.060%
95	19.010	2703	2707	2711	rBV4	11607	18205	0.35%	0.039%
96	19.204	2737	2740	2747	rBV4	28116	42248	0.82%	0.091%
97	19.304	2753	2757	2762	rVB	93667	133698	2.58%	0.288%
98	19.522	2789	2794	2799	rBV9	32372	63901	1.23%	0.138%
99	19.639	2808	2814	2825	rBV	2227871	3457345	66.74%	7.448%
100	21.610	3140	3149	3162	rBV	1827123	5180319	100.00%	11.160%




Sum of corrected areas: 46418716

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018463.D
Acq On : 29 Nov 2023 04:17
Operator : MA/JU
Sample : 05416-21
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

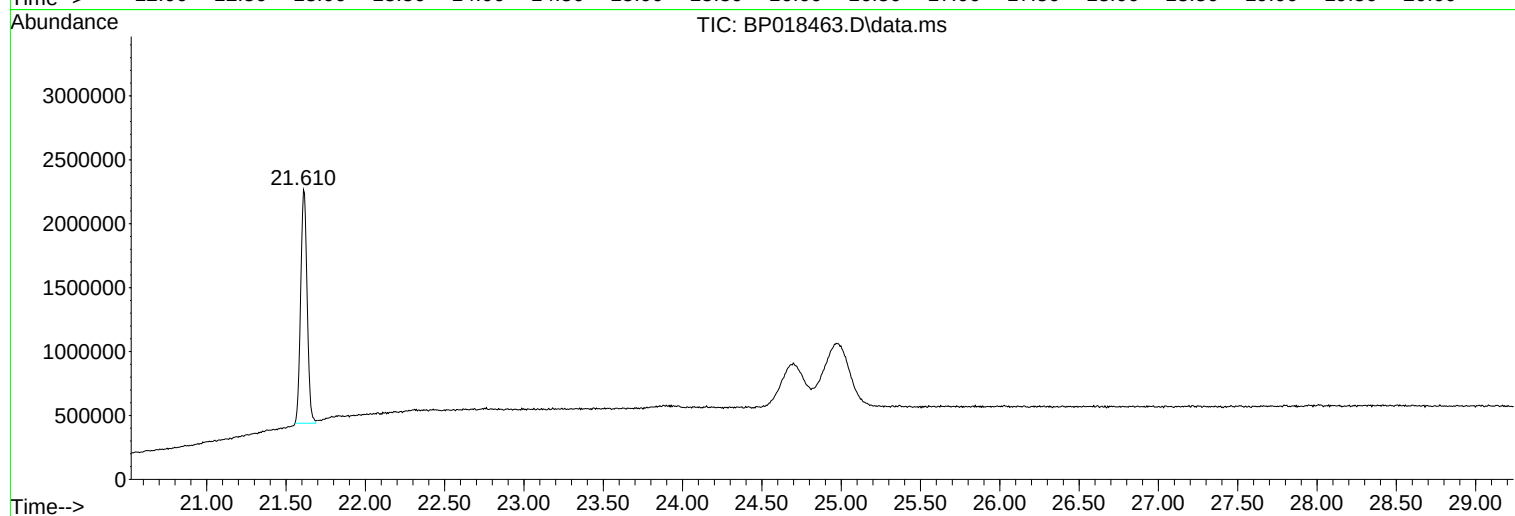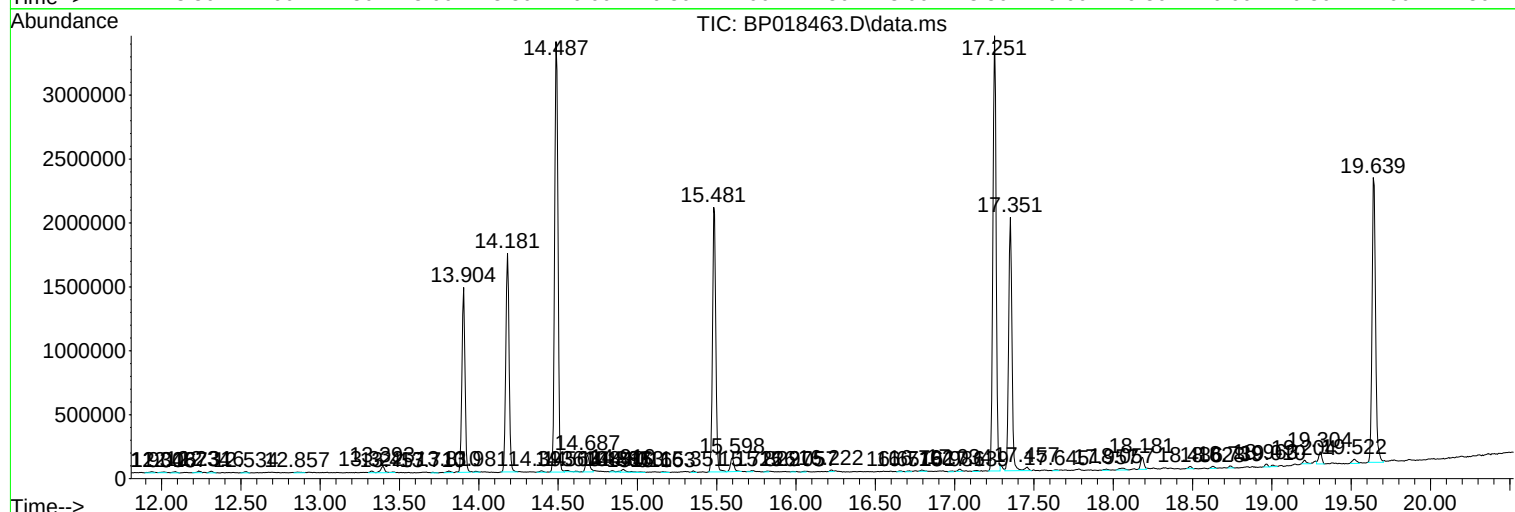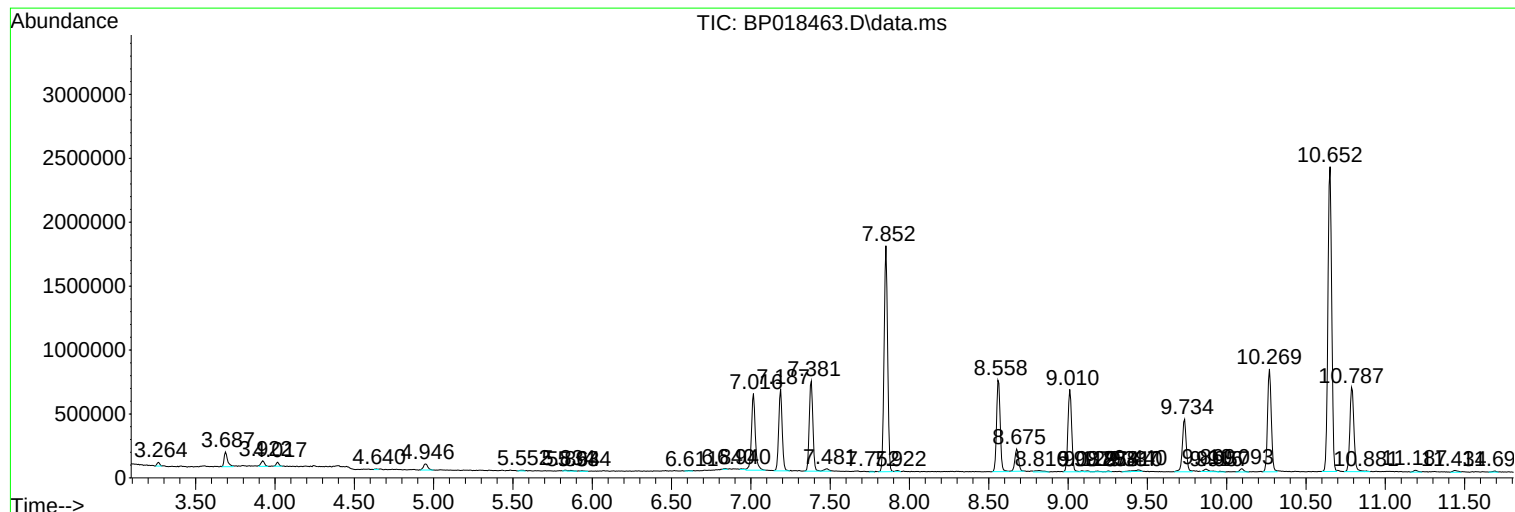

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018463.D
Acq On : 29 Nov 2023 04:17
Operator : MA/JU
Sample : 05416-21
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112723\
Data File : BP018463.D
Acq On : 29 Nov 2023 04:17
Operator : MA/JU
Sample : 05416-21
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------