
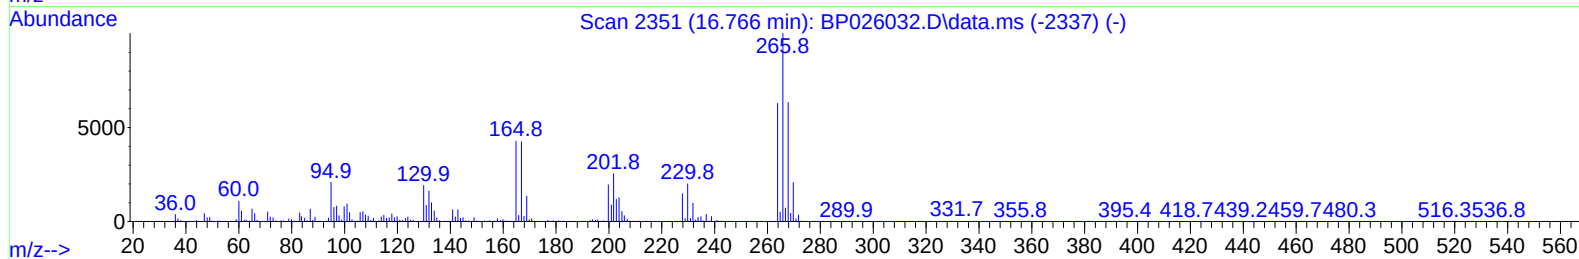
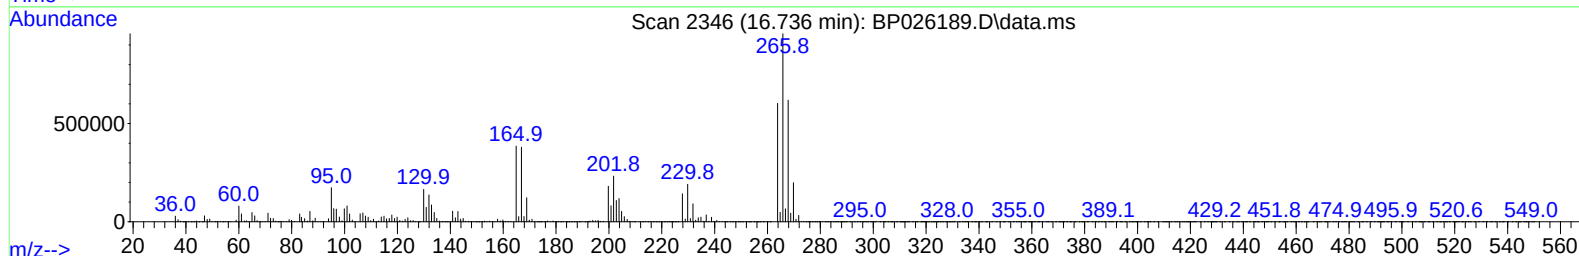


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112725\
Data File : BP026189.D
Acq On : 26 Nov 2025 13:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 15:09:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

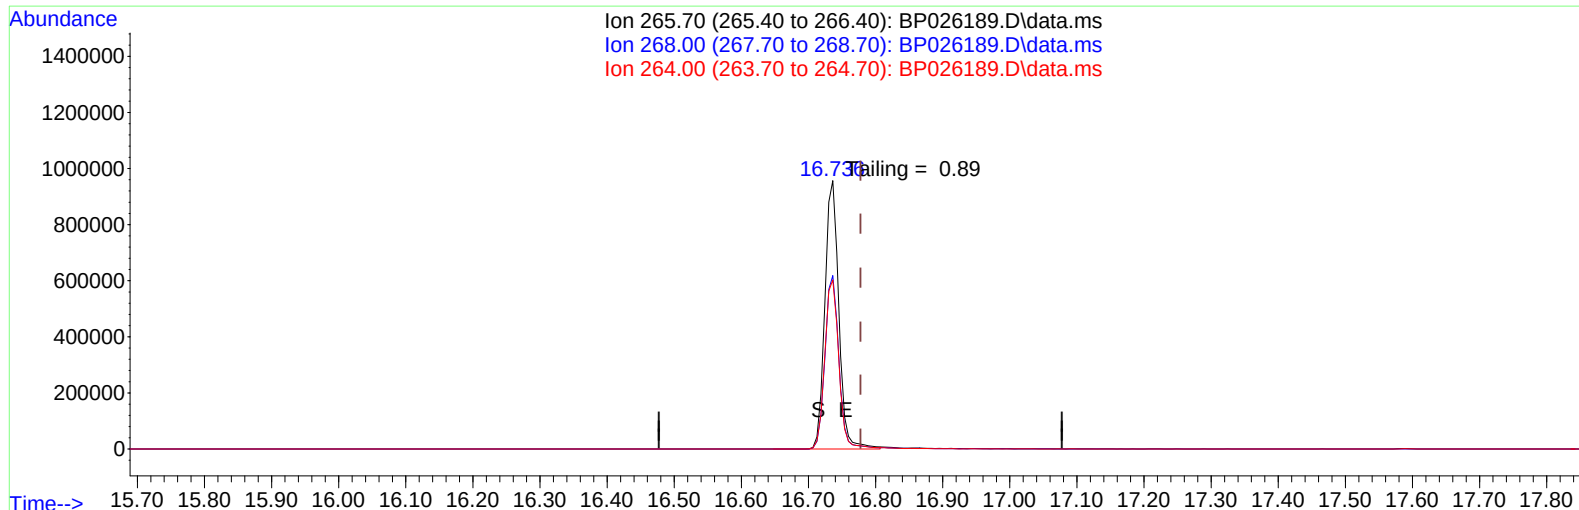

TIC: BP026189.D\data.ms

(70) Pentachlorophenol (C)




16.736min (-0.041) 64652.85 ng

response 1389037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.65
264.00	62.70	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112725\
Data File : BP026189.D
Acq On : 26 Nov 2025 13:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 15:09:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

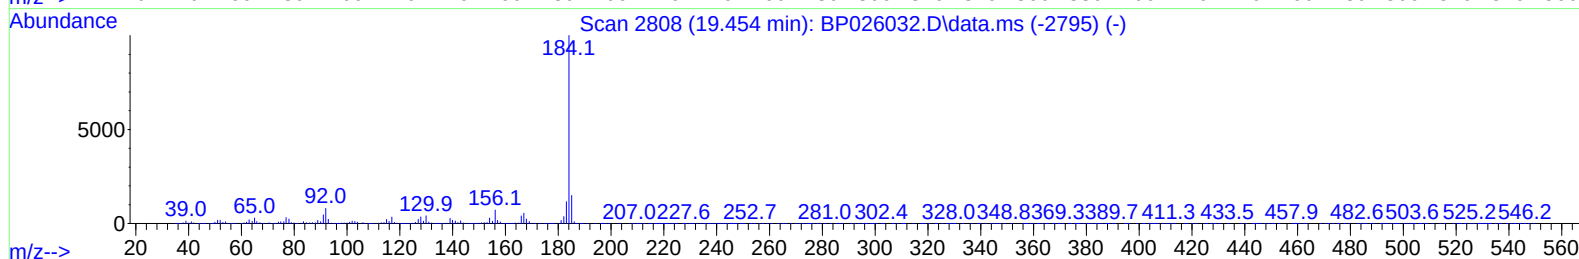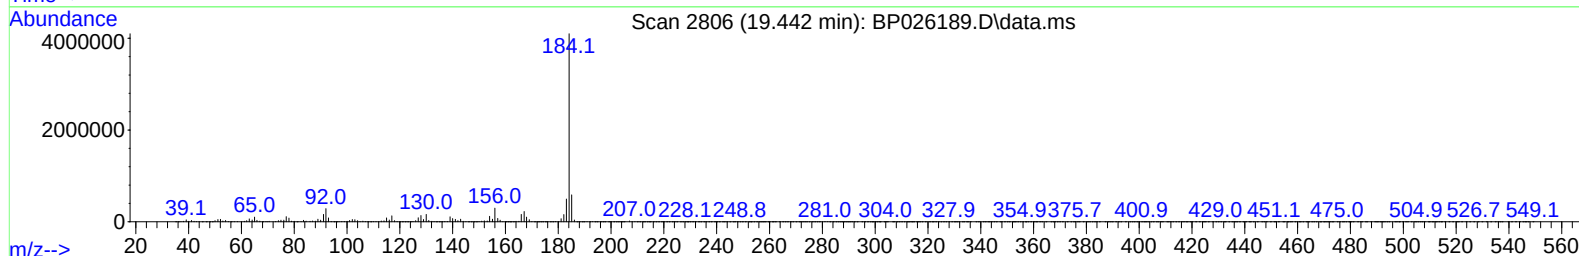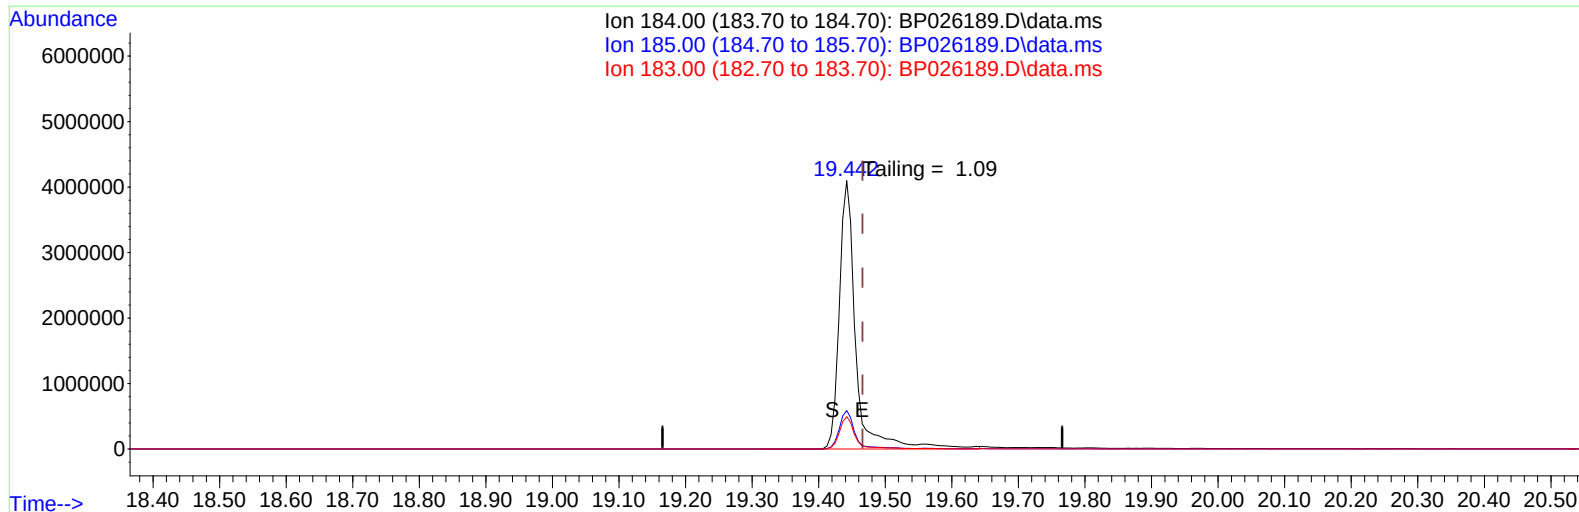

TIC: BP026189.D\data.ms

(77) Benzidine

19.442min (-0.024) 26907.41 ng

response 6791277

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.33
183.00	11.30	12.05
0.00	0.00	0.00