

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012845.D
 Acq On : 29 Nov 2022 11:13
 Operator : CG/JU
 Sample : N5666-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB28

Quant Time: Nov 29 21:56:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	645270	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	2874375	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	1904961	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.404	188	4029359	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	3286463	20.000	ng/ul	-0.01
88) Perylene-d12	23.998	264	2997135	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	55482	3.684	ng/uL	0.00
4) Pyridine-d5	3.822	84	260183	5.774	ng/ul	0.00
7) Phenol-d5	7.163	99	585043	11.034	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	1023504	31.326	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	1048585	25.953	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	808453	18.924	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	646183	36.730	ng/ul	0.00
24) 2-Nitrophenol-d4	9.905	143	566216	30.311	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	1246694	28.603	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1660106	27.814	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	4672861	35.638	ng/ul	0.00
49) Acenaphthylene-d8	14.340	160	5242474	34.266	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	108155	4.627	ng/ul	0.00
60) Fluorene-d10	15.639	176	4117590	35.857	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	63375	3.291	ng/ul	0.00
73) Anthracene-d10	17.504	188	6973182	39.315	ng/ul	0.00
81) Pyrene-d10	19.727	212	7594497	39.770	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.839	264	5984420	40.650	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.093	107	74423	1.628	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012845.D
Acq On : 29 Nov 2022 11:13
Operator : CG/JU
Sample : N5666-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB28

Quant Time: Nov 29 21:56:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

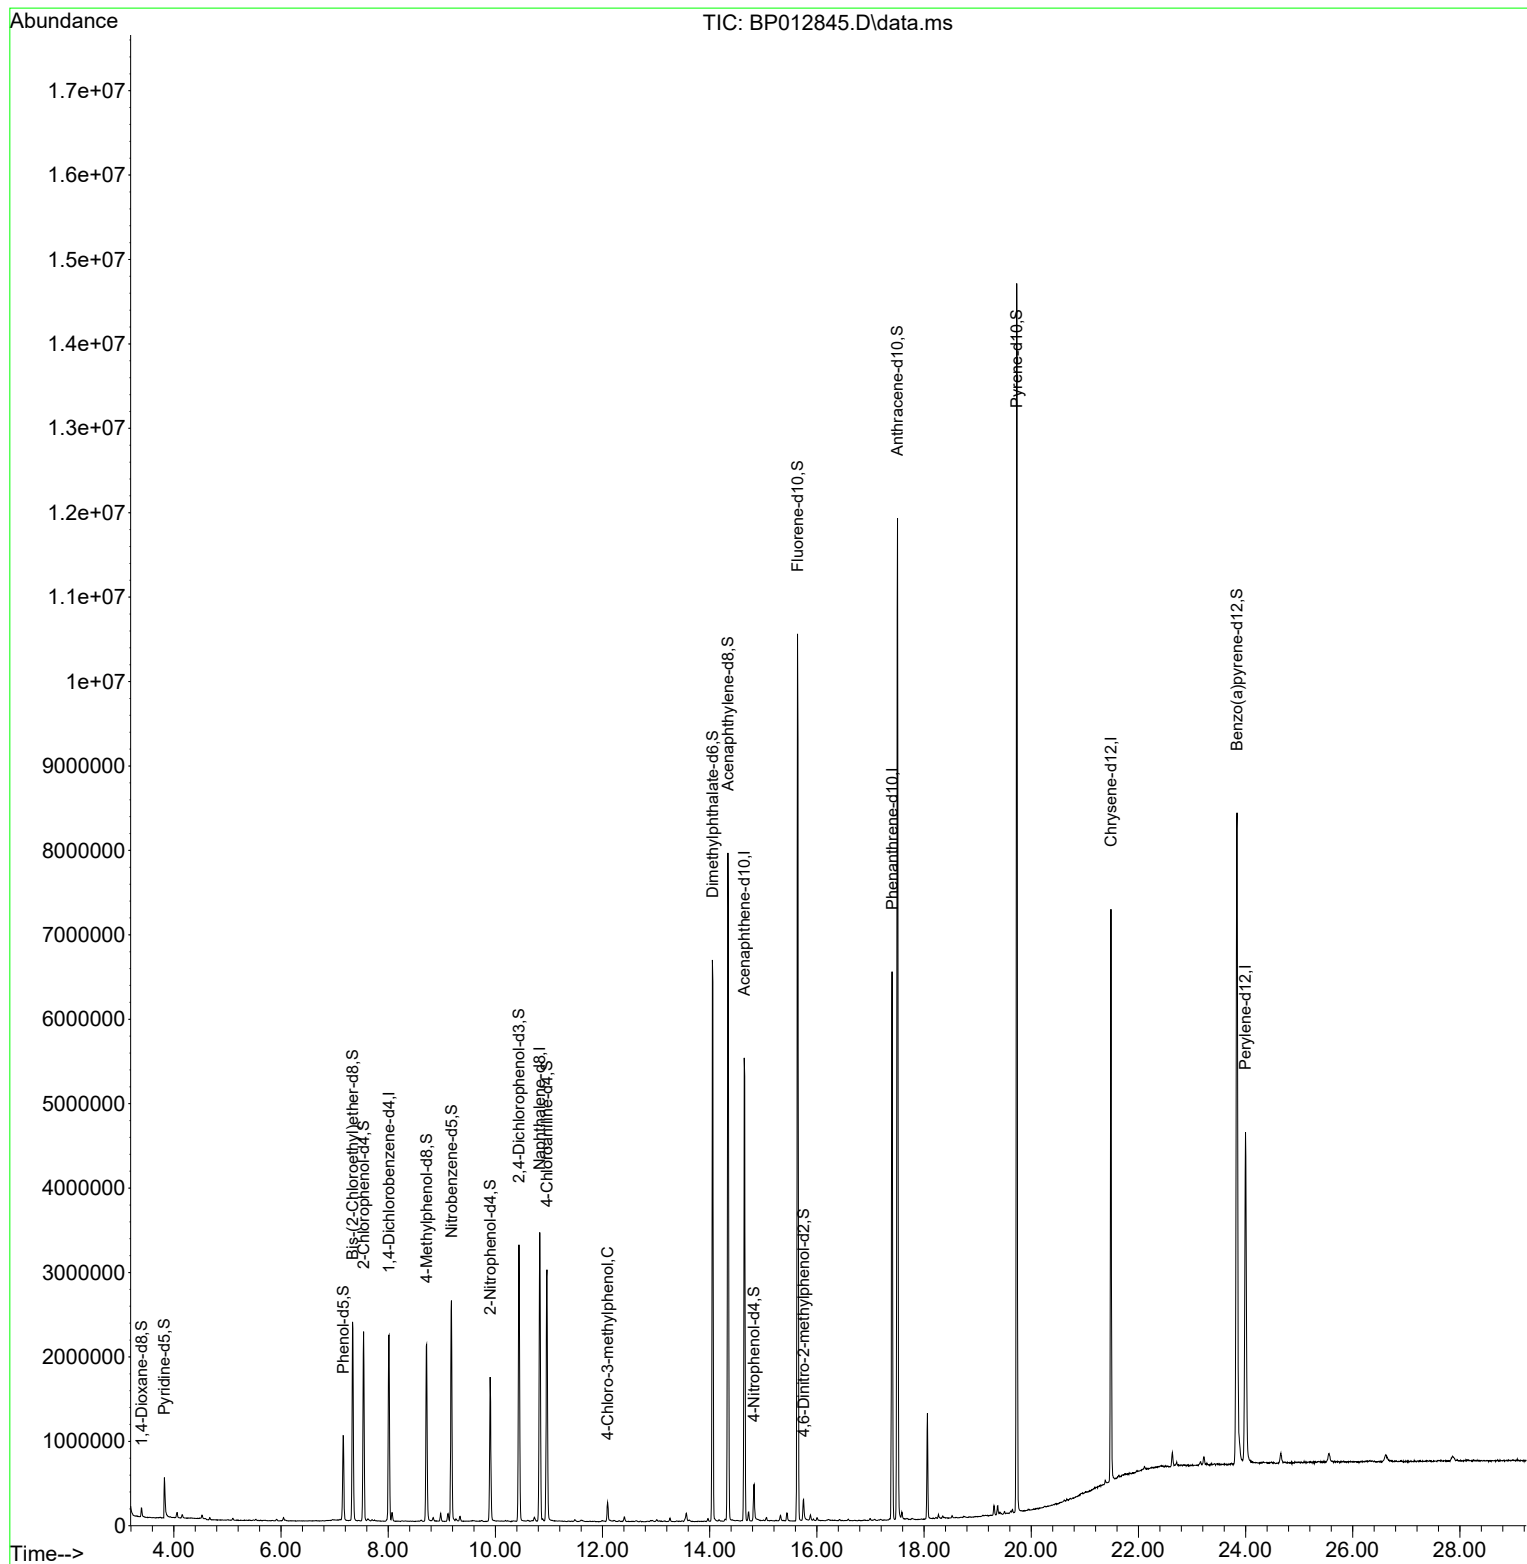

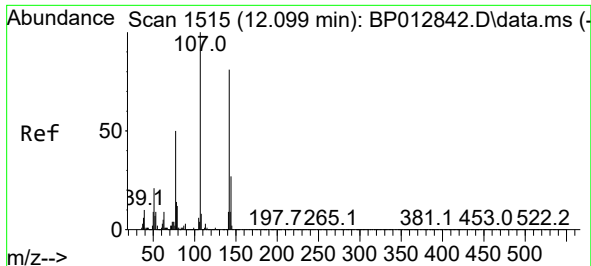

#35
 4-Chloro-3-methylphenol
 Concen: 1.628 ng/ul
 RT: 12.093 min Scan# 11
 Delta R.T. -0.012 min
 Lab File: BP012845.D
 Acq: 29 Nov 2022 11:13

Instrument :
 BNA_P
 ClientSampleId :
 BHB28

Tgt Ion:107 Resp: 74423
 Ion Ratio Lower Upper
 107 100
 144 29.0 21.4 32.2
 142 82.2 66.6 100.0

