

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012853.D
 Acq On : 29 Nov 2022 15:46
 Operator : CG/JU
 Sample : N5725-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB69

Quant Time: Nov 29 21:59:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	577455	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	2661367	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	1806513	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.404	188	4079711	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	4038249	20.000	ng/ul	-0.01
88) Perylene-d12	23.998	264	3765231	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	49740	3.691	ng/uL	0.00
4) Pyridine-d5	3.822	84	230224	5.709	ng/ul	0.00
7) Phenol-d5	7.157	99	236246	4.979	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	726953	24.862	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	697639	19.295	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	452933	11.847	ng/ul	-0.01
21) Nitrobenzene-d5	9.175	128	443065	27.200	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.904	143	451040	26.078	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	846269	20.970	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1153524	20.873	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	3283072	26.403	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	3667871	25.281	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	71359	3.219	ng/ul	0.00
60) Fluorene-d10	15.639	176	3044764	27.960	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	382225	19.602	ng/ul	0.00
73) Anthracene-d10	17.504	188	5176318	28.824	ng/ul	0.00
81) Pyrene-d10	19.727	212	6192889	26.393	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.833	264	5280262	28.550	ng/ul	-0.01
Target Compounds						
35) 4-Chloro-3-methylphenol	12.093	107	69627	1.645	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012853.D
Acq On : 29 Nov 2022 15:46
Operator : CG/JU
Sample : N5725-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB69

Quant Time: Nov 29 21:59:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

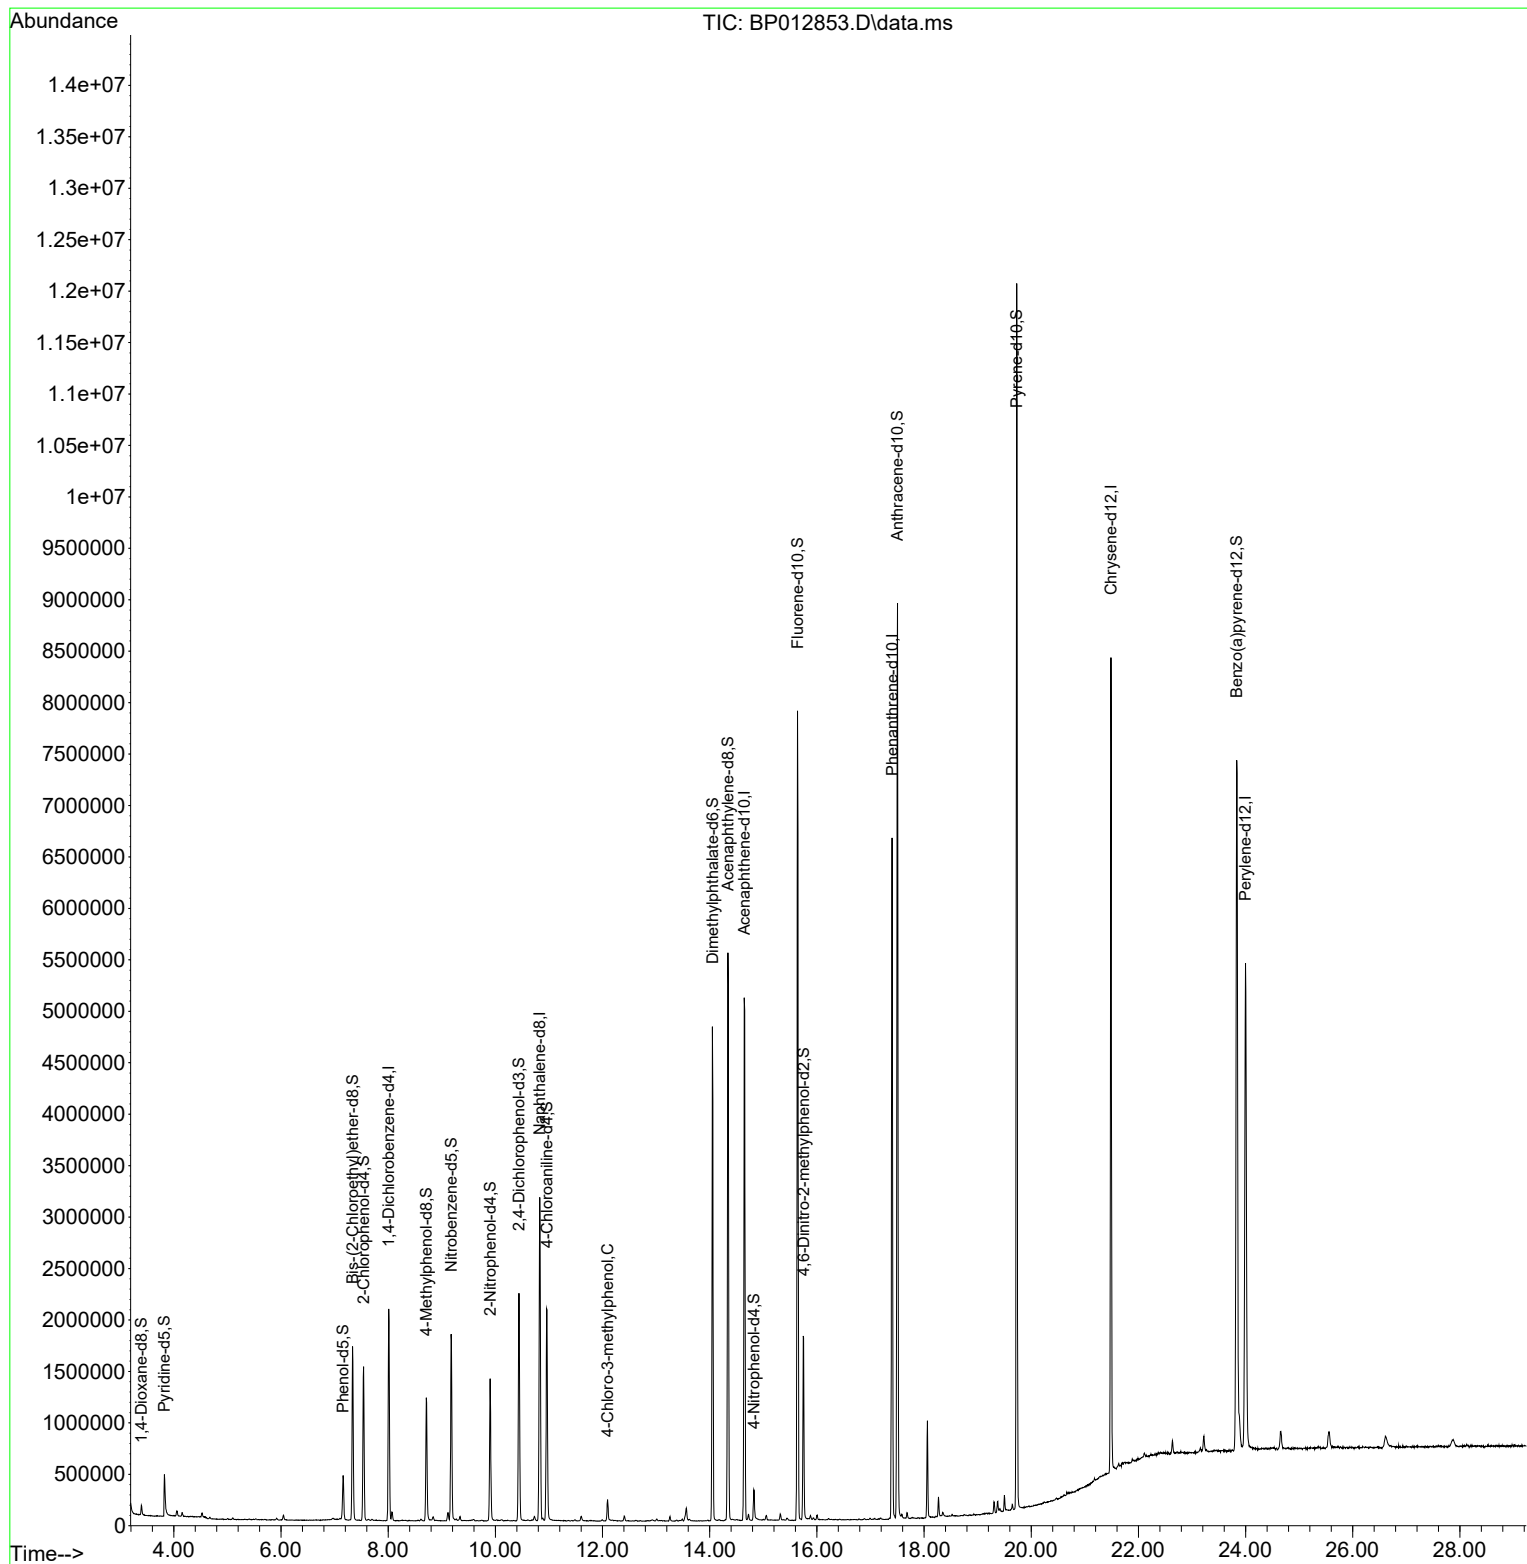

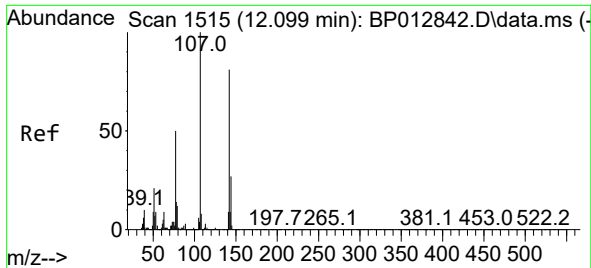

#35
 4-Chloro-3-methylphenol
 Concen: 1.645 ng/ul
 RT: 12.093 min Scan# 11
 Delta R.T. -0.012 min
 Lab File: BP012853.D
 Acq: 29 Nov 2022 15:46

Instrument :
 BNA_P
 ClientSampleId :
 BHB69

Tgt Ion:107 Resp: 69627
 Ion Ratio Lower Upper
 107 100
 144 26.0 21.4 32.2
 142 83.2 66.6 100.0

