

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012861.D
 Acq On : 29 Nov 2022 20:20
 Operator : CG/JU
 Sample : N5725-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB62

Quant Time: Nov 29 22:59:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	590879	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2693758	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	1864561	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.404	188	4105673	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	3959848	20.000	ng/u1	0.00
88) Perylene-d12	23.998	264	3758001	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	47560	3.449	ng/uL	0.00
4) Pyridine-d5	3.822	84	221915	5.378	ng/u1	0.00
7) Phenol-d5	7.158	99	244749	5.041	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	744027	24.868	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	735510	19.880	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	486154	12.427	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	457417	27.744	ng/u1	0.00
24) 2-Nitrophenol-d4	9.905	143	468711	26.774	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	900043	22.034	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	682277	12.198	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	3559092	27.731	ng/u1	0.00
49) Acenaphthylene-d8	14.340	160	3815767	25.481	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	72511	3.169	ng/u1	0.00
60) Fluorene-d10	15.640	176	3182087	28.311	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	356975	18.192	ng/u1	0.00
73) Anthracene-d10	17.498	188	5362054	29.669	ng/u1	0.00
81) Pyrene-d10	19.728	212	6361278	27.647	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	5598827	30.331	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.434	88	15792	1.066	ng/uL	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012861.D
Acq On : 29 Nov 2022 20:20
Operator : CG/JU
Sample : N5725-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB62

Quant Time: Nov 29 22:59:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

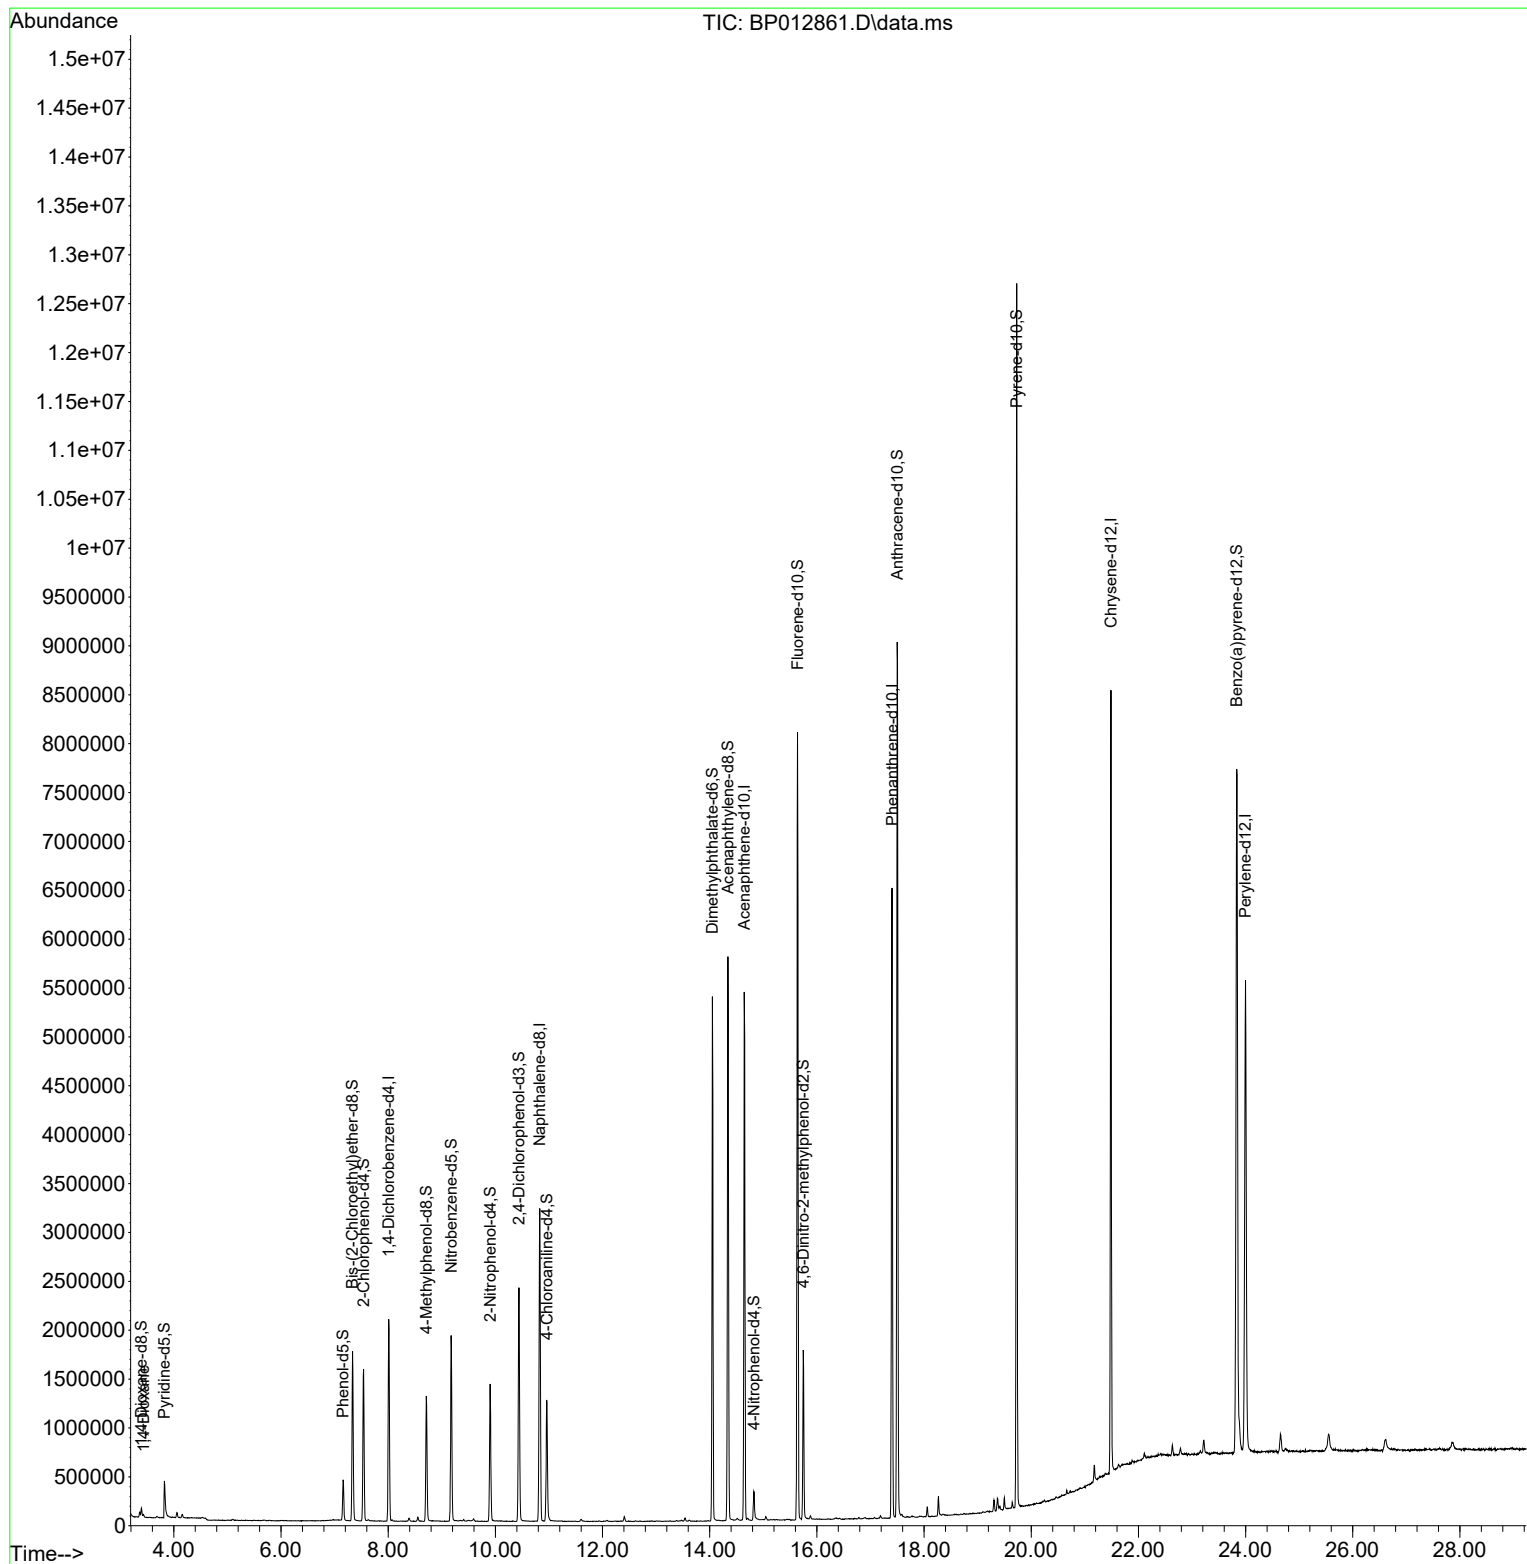

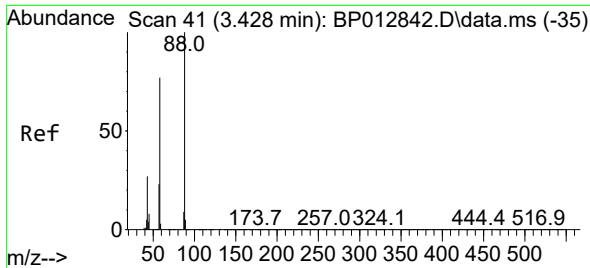

#2
 1,4-Dioxane
 Concen: 1.066 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: BP012861.D
 Acq: 29 Nov 2022 20:20

Instrument :
 BNA_P
 ClientSampleId :
 BHB62

Tgt Ion: 88 Resp: 15792
 Ion Ratio Lower Upper
 88 100
 43 28.9 22.6 34.0
 58 62.3 59.6 89.4

