

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012848.D
 Acq On : 29 Nov 2022 12:56
 Operator : CG/JU
 Sample : N5690-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGCE6

Quant Time: Nov 29 21:58:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	489180	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2242213	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	1519775	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.404	188	3444166	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	3478145	20.000	ng/u1	-0.01
88) Perylene-d12	23.998	264	3313102	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	46756	4.096	ng/uL	0.00
4) Pyridine-d5	3.822	84	240755	7.047	ng/u1	0.00
7) Phenol-d5	7.157	99	235703	5.864	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	704487	28.442	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	669033	21.843	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	457704	14.132	ng/u1	-0.01
21) Nitrobenzene-d5	9.181	128	451796	32.921	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	462058	31.709	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	830756	24.434	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	1072529	23.036	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	3314993	31.689	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	3729993	30.559	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	71633	3.841	ng/u1	0.00
60) Fluorene-d10	15.639	176	2996089	32.704	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	382179	23.217	ng/u1	0.00
73) Anthracene-d10	17.504	188	5051986	33.322	ng/u1	0.00
81) Pyrene-d10	19.727	212	6091243	30.140	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	5505520	33.831	ng/u1	-0.01


Target Compounds					Qvalue
78) Di-n-butylphthalate	18.345	149	284851	1.566 ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012848.D
Acq On : 29 Nov 2022 12:56
Operator : CG/JU
Sample : N5690-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGCE6

Quant Time: Nov 29 21:58:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

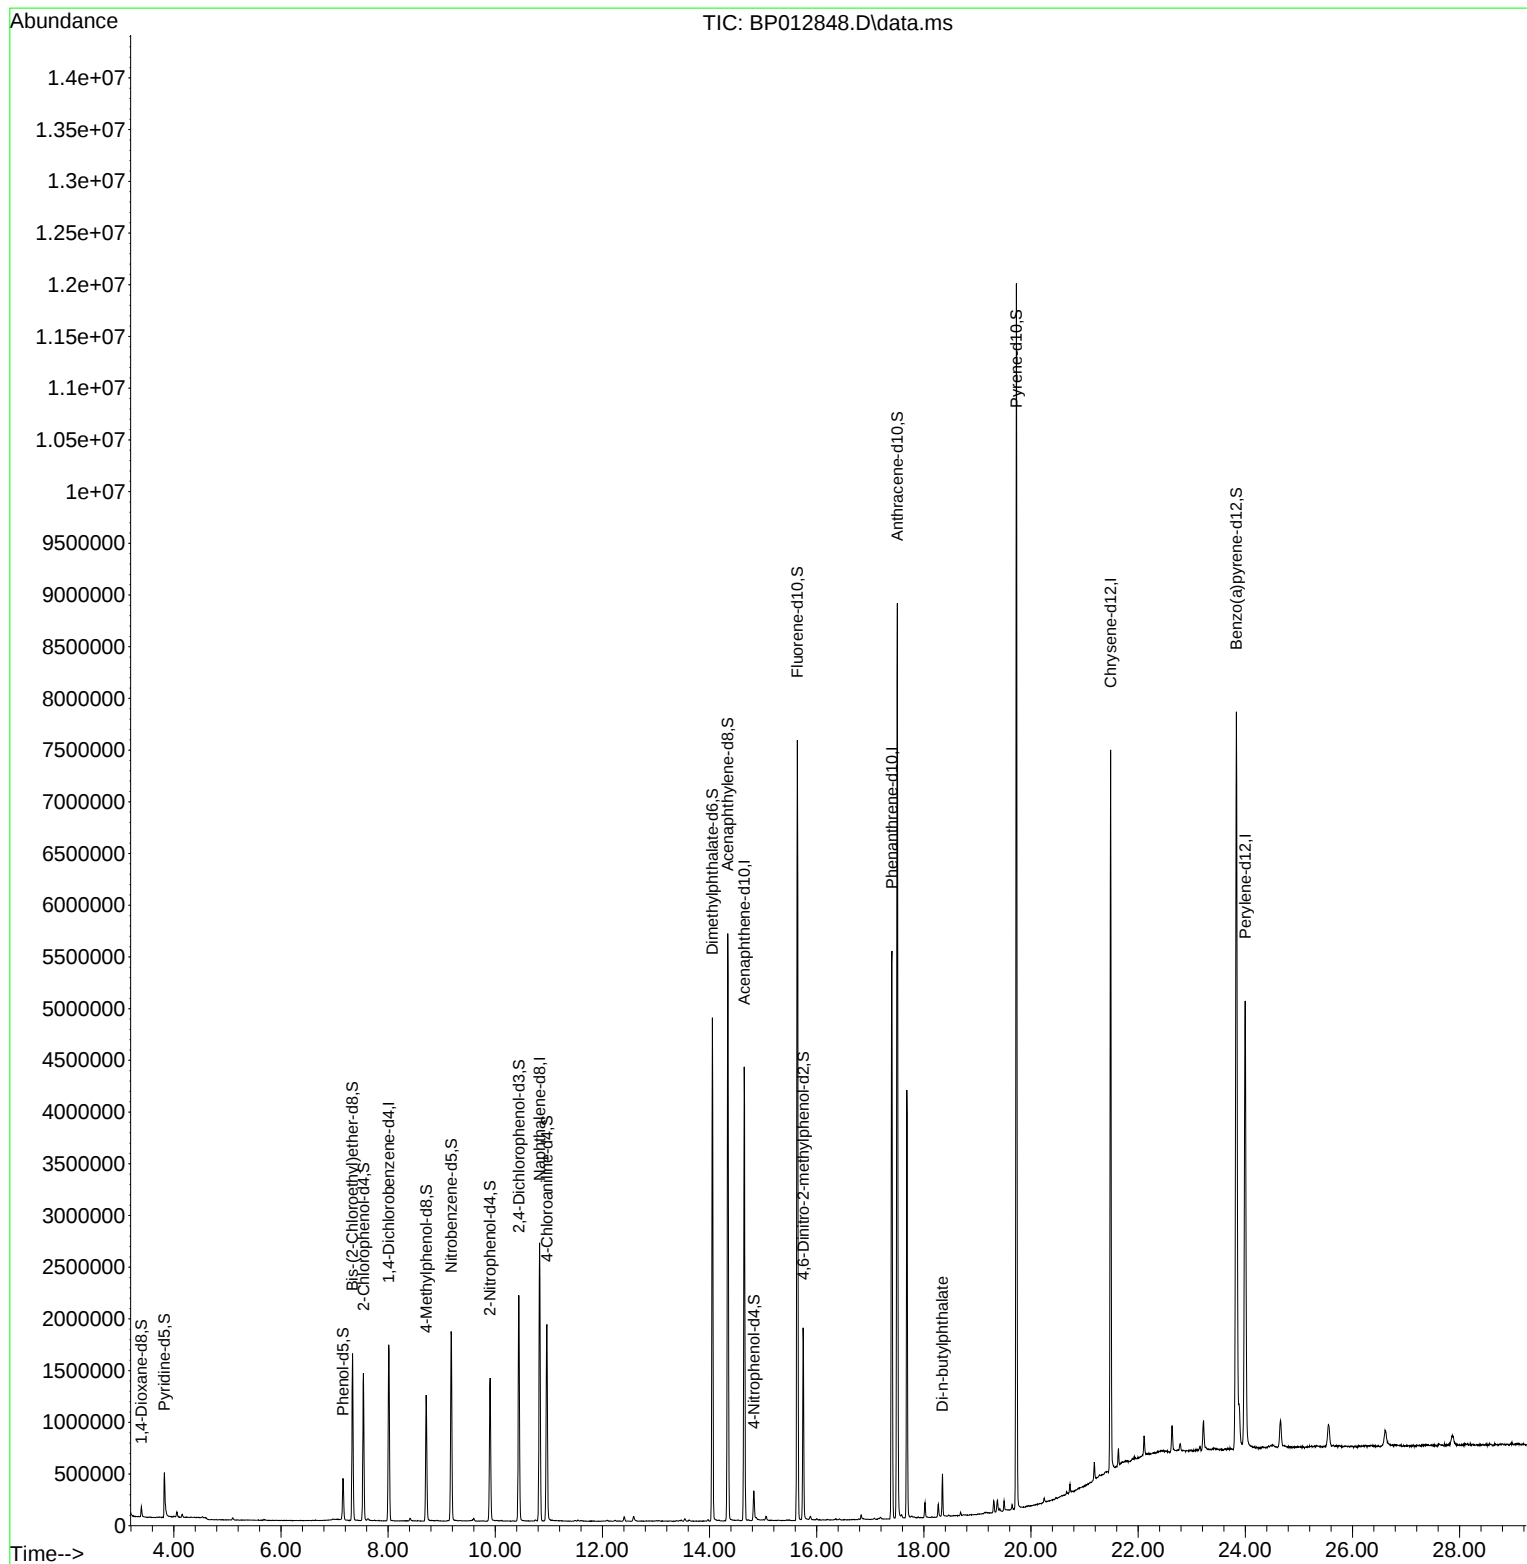

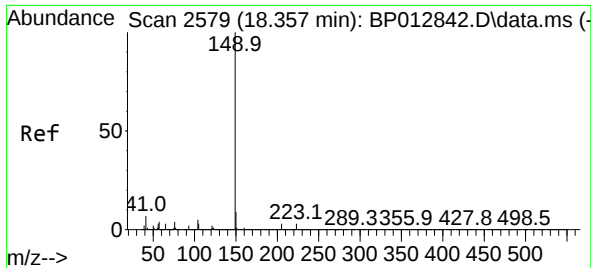

#78
 Di-n-butylphthalate
 Concen: 1.566 ng/ul
 RT: 18.345 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP012848.D
 Acq: 29 Nov 2022 12:56

Instrument :
 BNA_P
 ClientSampleId :
 BGCE6

Tgt Ion:149 Resp: 284851
 Ion Ratio Lower Upper
 149 100
 150 9.4 7.2 10.8
 104 5.3 3.7 5.5

