

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012863.D
 Acq On : 29 Nov 2022 21:28
 Operator : CG/JU
 Sample : N5725-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB66

Quant Time: Nov 29 23:00:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	459871	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2147077	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.646	164	1492579	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	3413002	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	3603783	20.000	ng/u1	0.00
88) Perylene-d12	23.998	264	3670950	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	38369	3.575	ng/uL	0.00
4) Pyridine-d5	3.823	84	236608	7.367	ng/u1	0.00
7) Phenol-d5	7.158	99	285686	7.560	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	719928	30.918	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	722604	25.095	ng/u1	0.00
15) 4-Methylphenol-d8	8.711	113	515138	16.919	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	436057	33.182	ng/u1	0.00
24) 2-Nitrophenol-d4	9.905	143	460973	33.036	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	884012	27.152	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	774838	17.379	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	3375601	32.857	ng/u1	0.00
49) Acenaphthylene-d8	14.340	160	3681156	30.709	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	102971	5.622	ng/u1	0.00
60) Fluorene-d10	15.640	176	3122748	34.707	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	465512	28.537	ng/u1	0.00
73) Anthracene-d10	17.498	188	5463996	36.369	ng/u1	0.00
81) Pyrene-d10	19.728	212	6593587	31.488	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	6480614	35.941	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	113046	9.808	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012863.D
Acq On : 29 Nov 2022 21:28
Operator : CG/JU
Sample : N5725-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB66


Quant Time: Nov 29 23:00:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

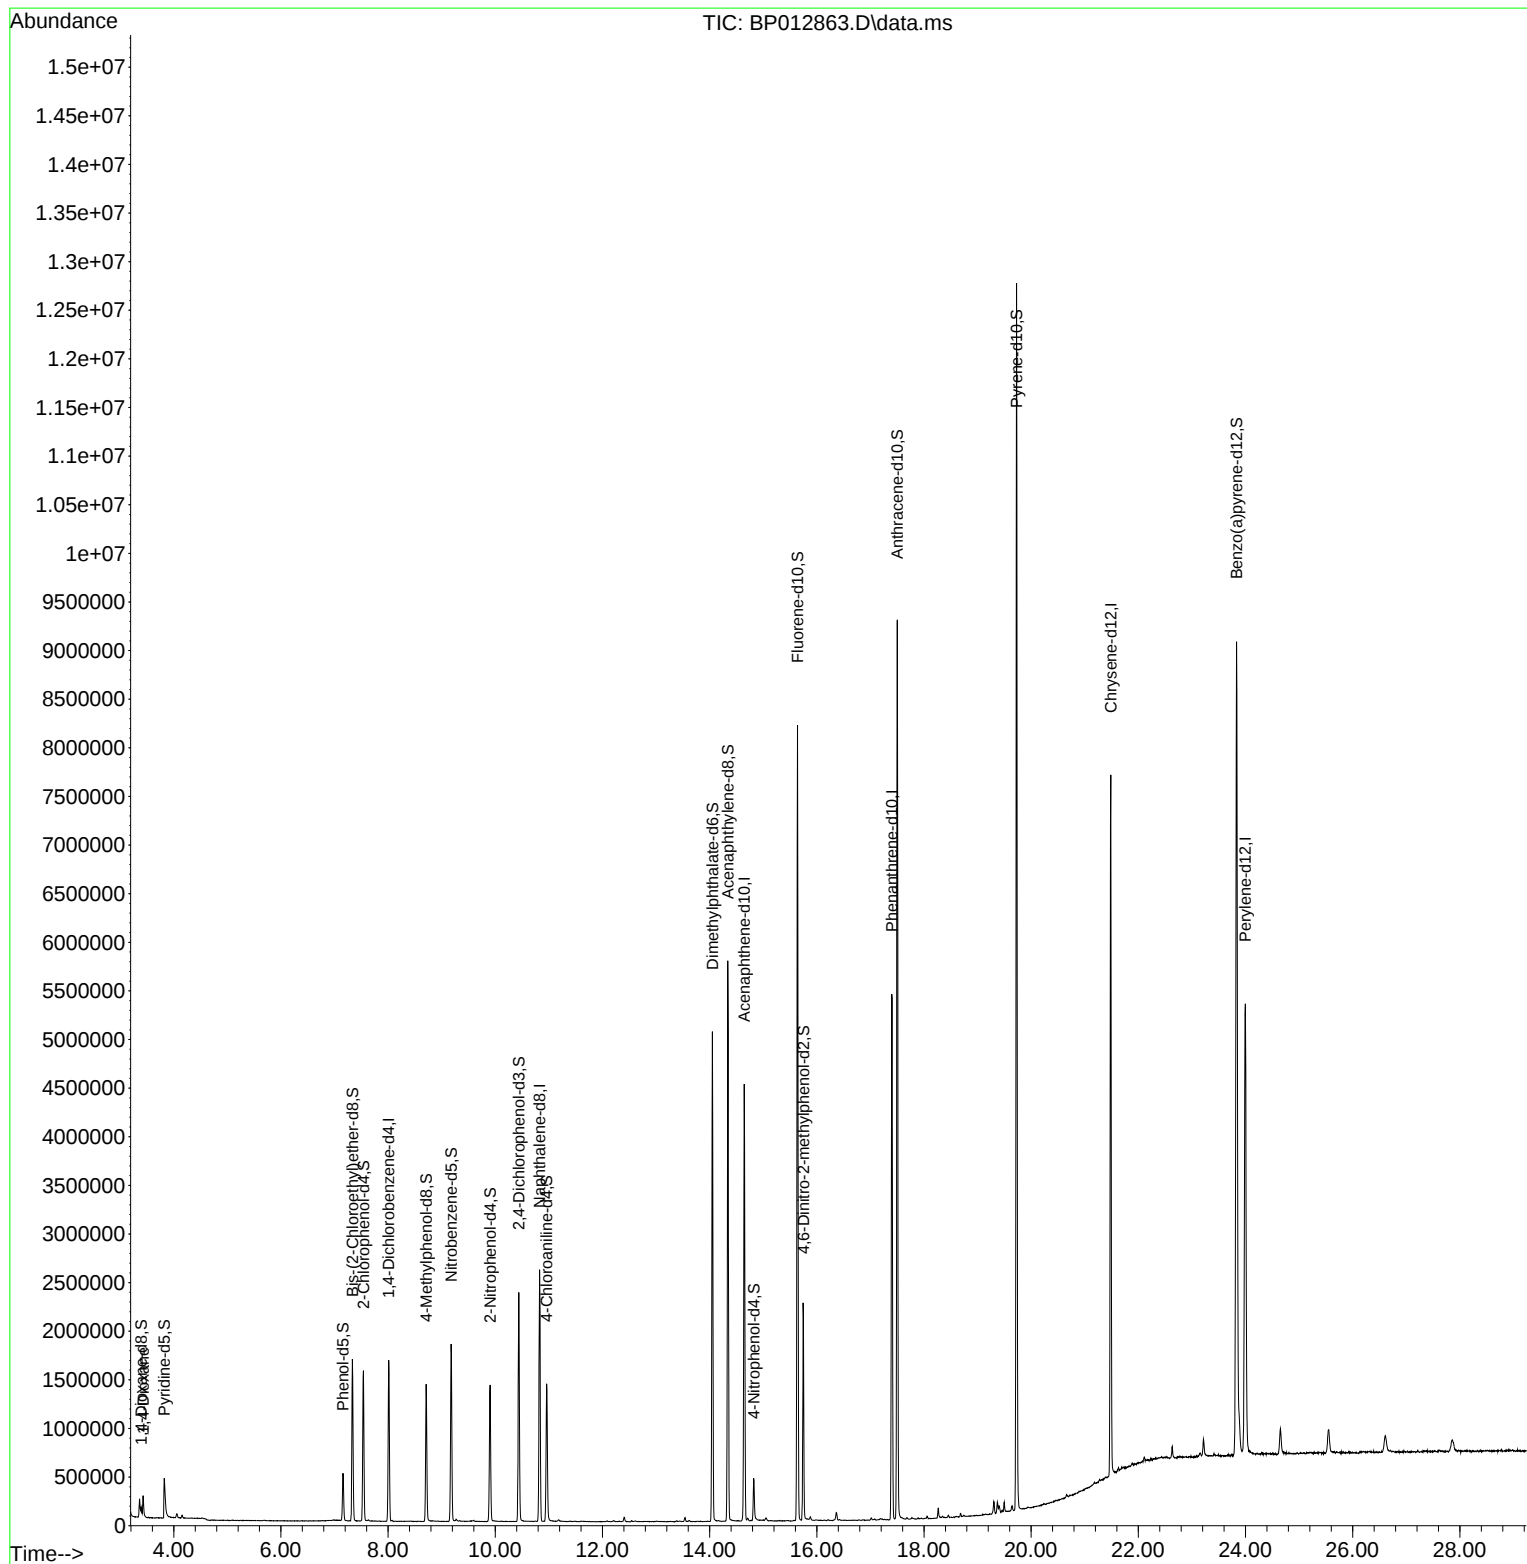

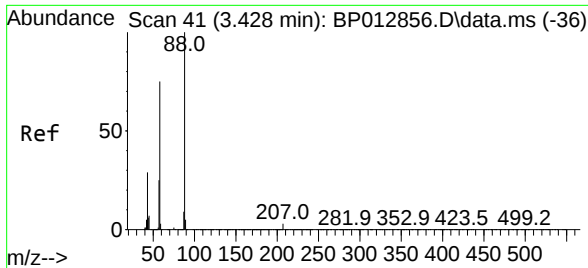

#2
 1,4-Dioxane
 Concen: 9.808 ng/uL
 RT: 3.428 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP012863.D
 Acq: 29 Nov 2022 21:28

Instrument :
 BNA_P
 ClientSampleId :
 BHB66

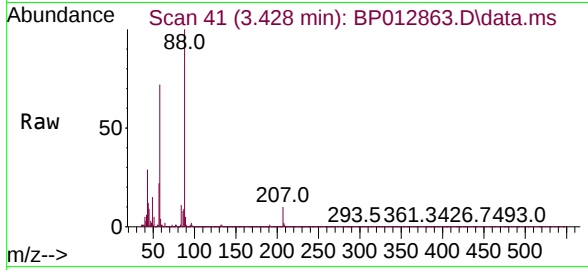

Tgt Ion: 88 Resp: 113046
 Ion Ratio Lower Upper
 88 100
 43 29.1 22.6 34.0
 58 72.4 59.6 89.4

