

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012866.D
 Acq On : 29 Nov 2022 23:10
 Operator : CG/JU
 Sample : N5725-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB65

Quant Time: Nov 30 00:49:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 29 22:53:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	657474	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2921708	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	1903508	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.404	188	3632403	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	2266105	20.000	ng/u1	0.00
88) Perylene-d12	23.992	264	2307677	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	76639	4.995	ng/uL	0.00
4) Pyridine-d5	3.822	84	291986	6.359	ng/u1	0.00
7) Phenol-d5	7.157	99	409325	7.576	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	1006311	30.228	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	1028138	24.975	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	721235	16.569	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	611418	34.191	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	656637	34.582	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	1190792	26.878	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	896233	14.772	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	4299878	32.818	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	4743199	31.026	ng/u1	0.00
54) 4-Nitrophenol-d4	14.822	143	107241	4.591	ng/u1	0.00
60) Fluorene-d10	15.639	176	3893816	33.935	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	525563	30.273	ng/u1	0.00
73) Anthracene-d10	17.498	188	6064380	37.927	ng/u1	0.00
81) Pyrene-d10	19.727	212	5765414	43.786	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	4276669	37.729	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.434	88	158582	9.624 ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012866.D
Acq On : 29 Nov 2022 23:10
Operator : CG/JU
Sample : N5725-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB65

Quant Time: Nov 30 00:49:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 29 22:53:34 2022
Response via : Initial Calibration

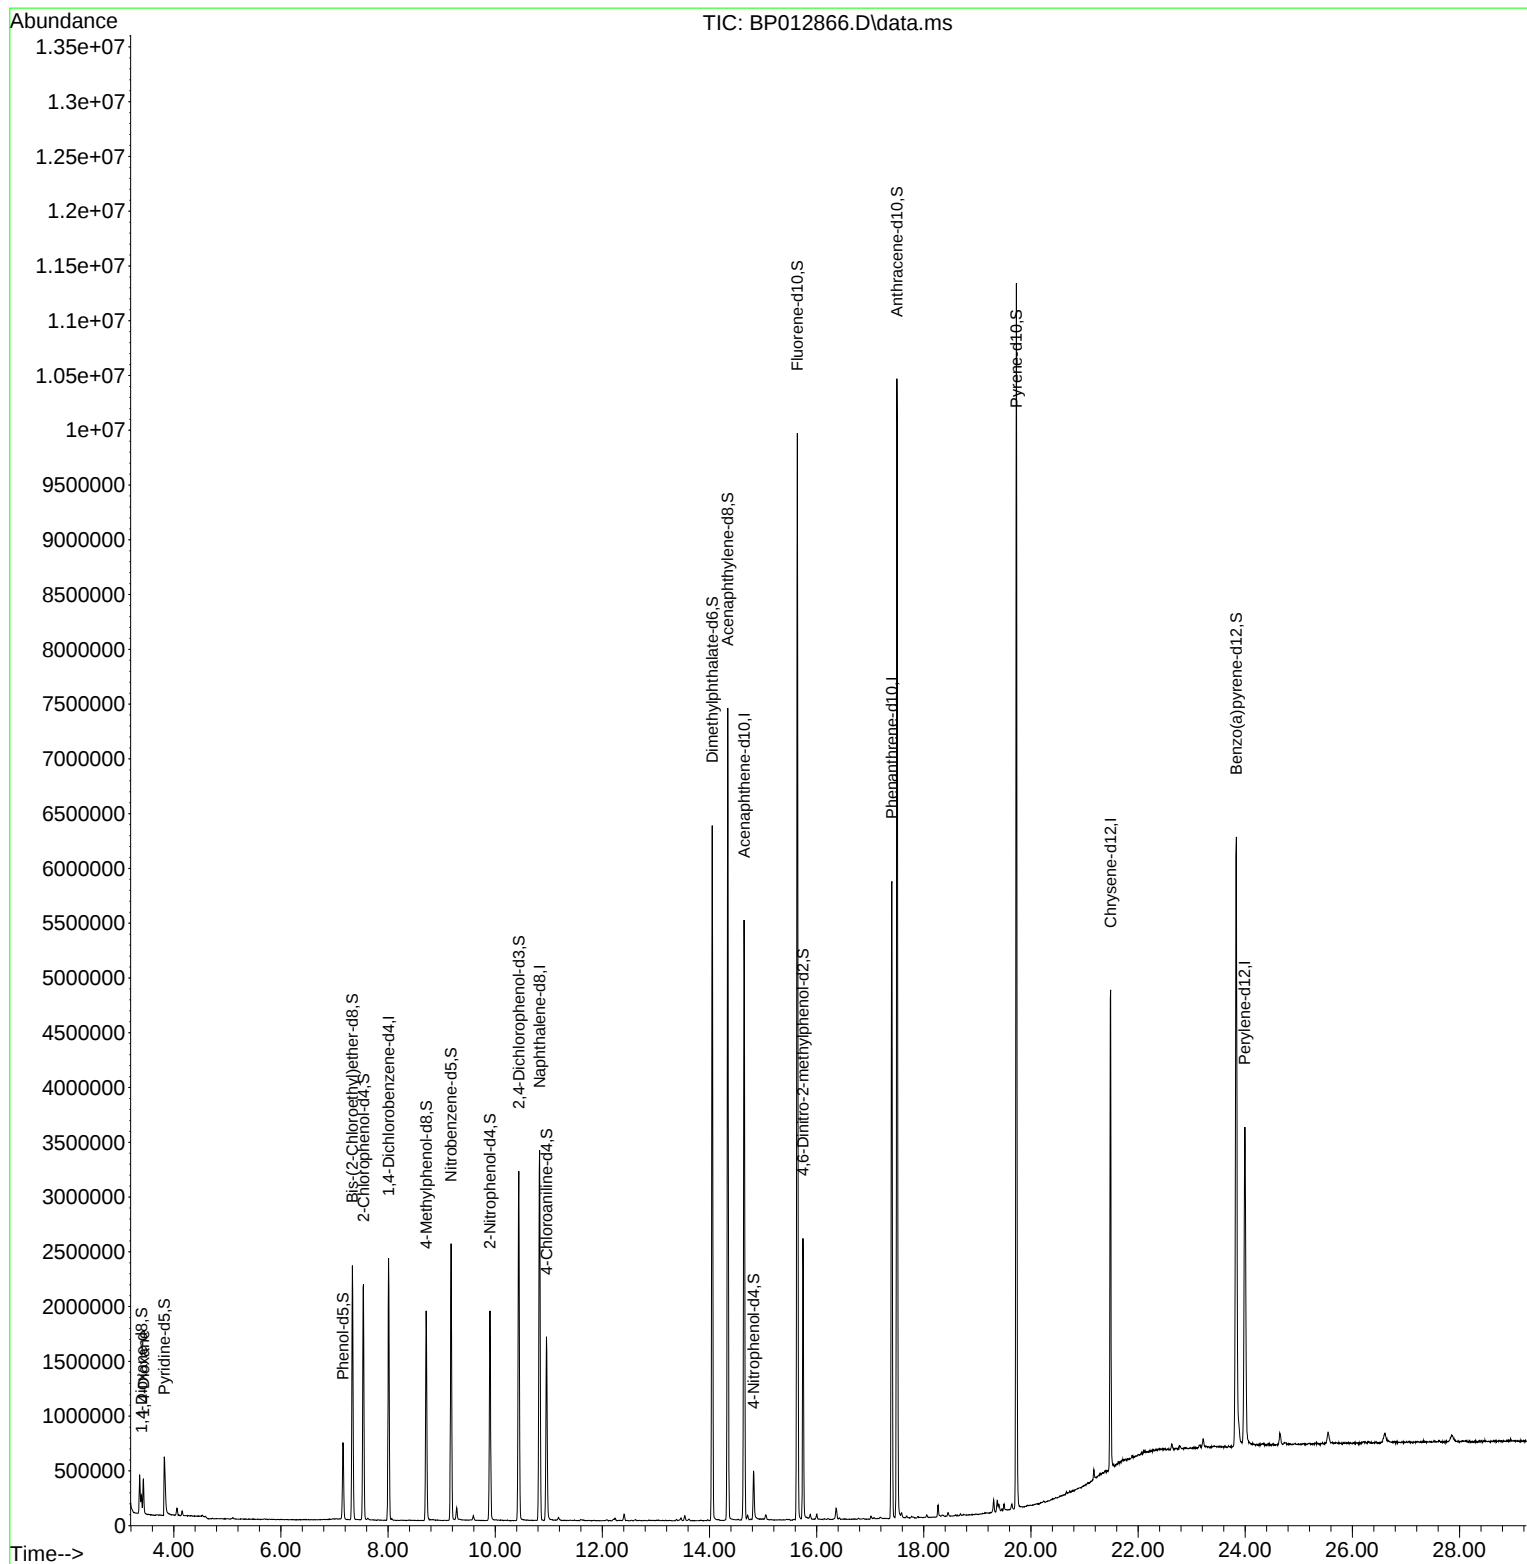

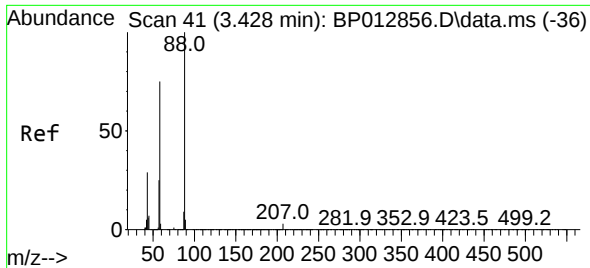

#2
 1,4-Dioxane
 Concen: 9.624 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: BP012866.D
 Acq: 29 Nov 2022 23:10

Instrument :
 BNA_P
 ClientSampleId :
 BHB65

Tgt Ion: 88 Resp: 158582
 Ion Ratio Lower Upper
 88 100
 43 28.4 22.6 34.0
 58 74.0 59.6 89.4

