

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012843.D
 Acq On : 29 Nov 2022 10:05
 Operator : CG/JU
 Sample : PB149186BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK186

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	42	rBV	111807	146955	1.29%	0.128%
2	3.817	104	107	127	rBV	1359326	2122262	18.56%	1.849%
3	4.158	162	165	173	rVB2	29768	50432	0.44%	0.044%
4	7.164	669	676	686	rVB	1647844	2511500	21.96%	2.188%
5	7.340	699	706	716	rVB	1459318	2255200	19.72%	1.965%
6	7.540	733	740	752	rBV	1683979	2600446	22.74%	2.266%
7	8.016	813	821	830	rBV	1656400	2638993	23.08%	2.300%
8	8.716	930	940	955	rBV	2081082	3280942	28.69%	2.859%
9	9.181	1011	1019	1031	rBV	1524152	2434074	21.29%	2.121%
10	9.911	1134	1143	1156	rBV	1142829	1923355	16.82%	1.676%
11	10.446	1224	1234	1246	rBV	2048755	3386641	29.62%	2.951%
12	10.834	1291	1300	1311	rBV	2466692	4140955	36.21%	3.608%
13	10.963	1314	1322	1340	rBV	2064028	3505257	30.65%	3.054%
14	12.081	1505	1512	1522	rVB8	10764	30945	0.27%	0.027%
15	12.410	1563	1568	1573	rBV	34103	55567	0.49%	0.048%
16	13.546	1753	1761	1767	rBV9	9180	20541	0.18%	0.018%
17	13.628	1769	1775	1780	rBV4	9725	15613	0.14%	0.014%
18	14.057	1841	1848	1863	rBV	4125972	5512044	48.20%	4.803%
19	14.346	1890	1897	1915	rBV	4536869	6519244	57.01%	5.681%
20	14.651	1942	1949	1959	rBV	3947752	5902433	51.62%	5.143%
21	14.828	1972	1979	2002	rBV	1438611	2246337	19.64%	1.957%
22	15.057	2013	2018	2024	rVB9	11336	22257	0.19%	0.019%
23	15.645	2111	2118	2126	rBV	6115729	8543382	74.71%	7.445%
24	15.751	2130	2136	2148	rVV	1348459	1809247	15.82%	1.577%
25	15.881	2155	2158	2163	rVB3	23486	32275	0.28%	0.028%
26	16.428	2248	2251	2256	rVB7	9603	14512	0.13%	0.013%
27	17.081	2359	2362	2367	rVB7	9363	13336	0.12%	0.012%
28	17.192	2377	2381	2386	rBV2	15413	22981	0.20%	0.020%
29	17.404	2410	2417	2427	rBV	5056466	7184348	62.83%	6.260%
30	17.504	2427	2434	2455	rVV	6673038	9612265	84.06%	8.376%
31	18.275	2561	2565	2569	rBV5	10637	16864	0.15%	0.015%
32	19.310	2737	2741	2747	rBV3	74184	99810	0.87%	0.087%
33	19.381	2748	2753	2756	rBV	67652	100199	0.88%	0.087%
34	19.733	2807	2813	2828	rBV	8685697	11434959	100.00%	9.964%
35	21.492	3106	3112	3122	rBV	5624614	7595822	66.43%	6.619%
36	23.839	3504	3511	3529	rBV2	4572216	9821432	85.89%	8.558%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012843.D
Acq On : 29 Nov 2022 10:05
Operator : CG/JU
Sample : PB149186BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK186

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37 24.004 3532 3539 3559 rVB2 3421088 7135582 62.40% 6.218%




Sum of corrected areas: 114759007

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012843.D
Acq On : 29 Nov 2022 10:05
Operator : CG/JU
Sample : PB149186BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK186

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

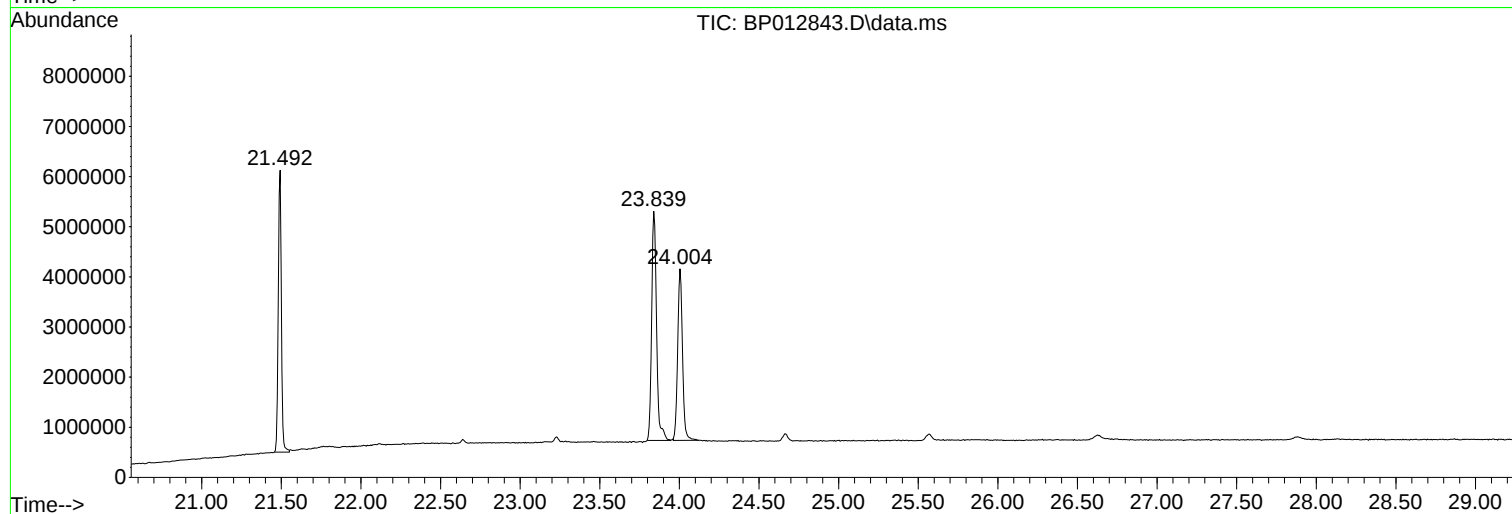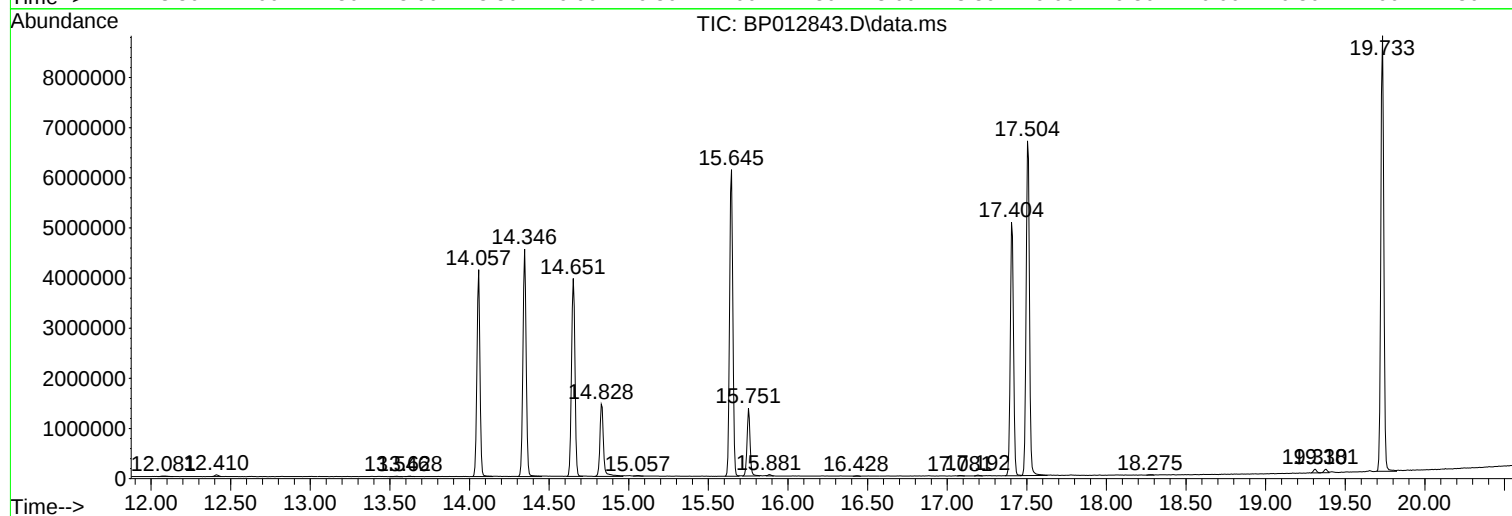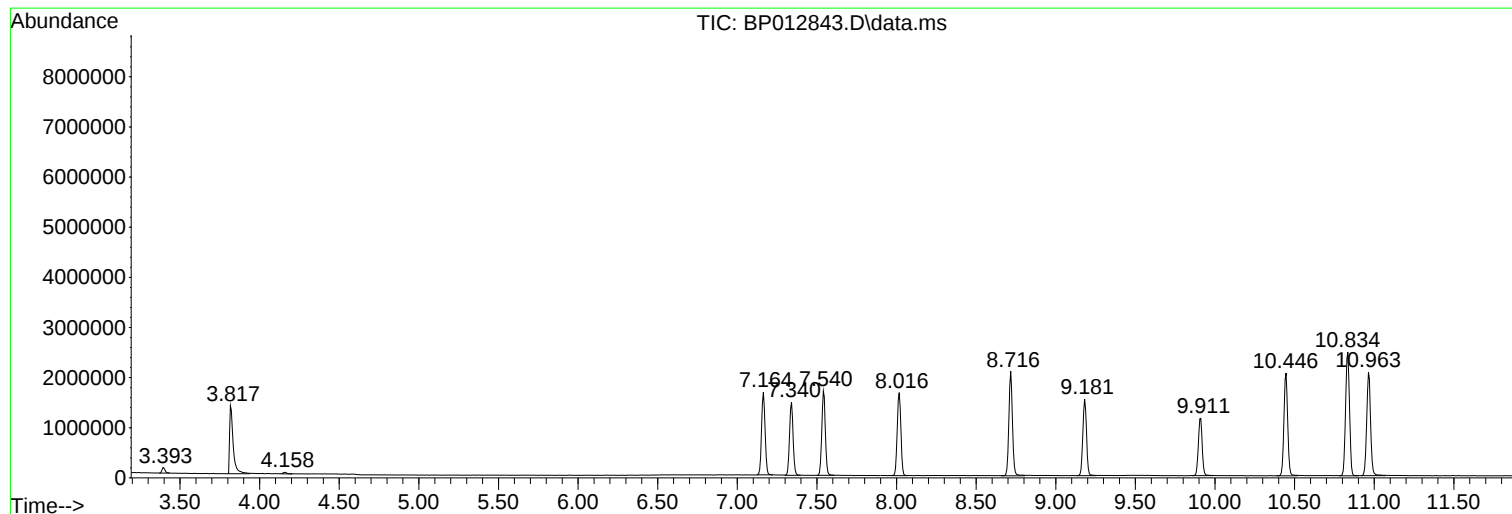

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012843.D
Acq On : 29 Nov 2022 10:05
Operator : CG/JU
Sample : PB149186BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK186

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012843.D
Acq On : 29 Nov 2022 10:05
Operator : CG/JU
Sample : PB149186BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK186

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc