

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012854.D
 Acq On : 29 Nov 2022 16:20
 Operator : CG/JU
 Sample : N5725-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	32	35	41	rBV	78607	104890	1.46%	0.132%
2	3.823	106	108	121	rBV	363221	539619	7.52%	0.678%
3	4.058	145	148	155	rVB2	24064	32278	0.45%	0.041%
4	4.158	161	165	169	rBV	29756	39818	0.56%	0.050%
5	4.528	224	228	231	rVB5	15453	17080	0.24%	0.021%
6	4.670	249	252	257	rVB4	8010	9592	0.13%	0.012%
7	5.099	320	325	332	rVB	133307	192358	2.68%	0.242%
8	5.481	385	390	392	rBV6	5088	7336	0.10%	0.009%
9	5.917	462	464	470	rVB4	7728	8834	0.12%	0.011%
10	6.046	482	486	490	rVB4	18031	22629	0.32%	0.028%
11	7.105	662	666	667	rBV3	6299	8105	0.11%	0.010%
12	7.158	669	675	684	rVB	512153	825606	11.51%	1.038%
13	7.334	699	705	714	rVB	889027	1373738	19.15%	1.726%
14	7.540	733	740	748	rBV	911153	1418838	19.78%	1.783%
15	7.622	752	754	762	rVV8	9672	16173	0.23%	0.020%
16	8.011	813	820	827	rBV	1666480	2651024	36.96%	3.332%
17	8.069	827	830	837	rVB	33209	44933	0.63%	0.056%
18	8.563	911	914	918	rBV6	4907	7399	0.10%	0.009%
19	8.616	918	923	926	rVV7	4842	8547	0.12%	0.011%
20	8.710	932	939	954	rBV	880994	1408319	19.64%	1.770%
21	8.834	957	960	964	rVB4	12238	18698	0.26%	0.023%
22	9.116	1001	1008	1011	rBV4	27069	48087	0.67%	0.060%
23	9.175	1011	1018	1031	rVV	875690	1458577	20.34%	1.833%
24	9.269	1031	1034	1038	rVV6	10377	16433	0.23%	0.021%
25	9.340	1042	1046	1054	rVB8	17914	29635	0.41%	0.037%
26	9.593	1087	1089	1095	rVB5	12048	15097	0.21%	0.019%
27	9.905	1134	1142	1154	rBV	666299	1088192	15.17%	1.368%
28	10.110	1171	1177	1181	rVB9	6053	12099	0.17%	0.015%
29	10.440	1226	1233	1245	rBV	1252219	2020007	28.17%	2.539%
30	10.681	1268	1274	1276	rBV7	4524	7928	0.11%	0.010%
31	10.728	1278	1282	1289	rVB3	12672	24934	0.35%	0.031%
32	10.828	1291	1299	1307	rBV	2488297	4180628	58.29%	5.254%
33	10.957	1313	1321	1334	rBV	1077111	1878109	26.19%	2.360%
34	11.475	1406	1409	1414	rBV7	6622	10301	0.14%	0.013%
35	11.599	1425	1430	1436	rBV6	19129	32248	0.45%	0.041%
36	12.093	1504	1514	1520	rBV3	64146	121037	1.69%	0.152%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012854.D
 Acq On : 29 Nov 2022 16:20
 Operator : CG/JU
 Sample : N5725-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	12.340	1550	1556	1564	rBV	71220	122113	1.70%	0.153%
38	12.410	1564	1568	1572	rVB3	22671	36149	0.50%	0.045%
39	12.846	1636	1642	1644	rBV7	4146	7813	0.11%	0.010%
40	12.934	1651	1657	1661	rVB9	4920	8706	0.12%	0.011%
41	13.010	1666	1670	1673	rVV5	8475	10828	0.15%	0.014%
42	13.263	1708	1713	1716	rVB4	10844	16166	0.23%	0.020%
43	13.387	1728	1734	1737	rBV7	9490	15947	0.22%	0.020%
44	13.540	1754	1760	1762	rBV	43599	70092	0.98%	0.088%
45	13.616	1770	1773	1781	rVB10	7953	15323	0.21%	0.019%
46	14.051	1837	1847	1859	rBV	2450206	3311467	46.17%	4.162%
47	14.181	1867	1869	1875	rVB7	7608	8524	0.12%	0.011%
48	14.340	1888	1896	1907	rBV	2748194	3901911	54.41%	4.904%
49	14.645	1941	1948	1956	rBV	4084236	5952901	83.00%	7.481%
50	14.722	1957	1961	1966	rVB5	21629	28638	0.40%	0.036%
51	14.828	1972	1979	1989	rBV	269313	485084	6.76%	0.610%
52	15.051	2013	2017	2023	rVB8	17862	33101	0.46%	0.042%
53	15.316	2058	2062	2068	rVB3	21066	35064	0.49%	0.044%
54	15.445	2080	2084	2090	rBV6	8298	14939	0.21%	0.019%
55	15.640	2110	2117	2128	rBV	3745497	5382522	75.05%	6.765%
56	15.745	2130	2135	2145	rVV	687036	965720	13.47%	1.214%
57	15.875	2154	2157	2163	rVB3	18165	30469	0.42%	0.038%
58	15.928	2165	2166	2174	rVB8	9552	13408	0.19%	0.017%
59	16.004	2175	2179	2182	rBV3	14008	19928	0.28%	0.025%
60	16.210	2211	2214	2218	rBV6	5612	9091	0.13%	0.011%
61	16.422	2246	2250	2255	rVB8	5697	9526	0.13%	0.012%
62	16.787	2309	2312	2315	rVB5	6046	7864	0.11%	0.010%
63	16.887	2324	2329	2333	rVB8	4809	8863	0.12%	0.011%
64	17.075	2358	2361	2364	rBV5	6406	7810	0.11%	0.010%
65	17.187	2377	2380	2386	rVB5	10188	18851	0.26%	0.024%
66	17.357	2404	2409	2410	rBV5	7068	10411	0.15%	0.013%
67	17.404	2410	2417	2427	rVV	4979968	7171921	100.00%	9.013%
68	17.498	2427	2433	2446	rBV	4215108	6014909	83.87%	7.559%
69	18.063	2524	2529	2538	rBV	254228	338329	4.72%	0.425%
70	18.269	2560	2564	2570	rBV2	101476	136262	1.90%	0.171%
71	18.339	2574	2576	2577	rBV2	11306	7395	0.10%	0.009%
72	19.304	2737	2740	2746	rVB3	46850	62626	0.87%	0.079%
73	19.375	2747	2752	2757	rBV3	49884	94618	1.32%	0.119%
74	19.498	2770	2773	2778	rBV5	56796	68809	0.96%	0.086%
75	19.645	2796	2798	2801	rVB4	27620	27136	0.38%	0.034%
76	19.728	2806	2812	2821	rBV	5400678	7075776	98.66%	8.893%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012854.D
Acq On : 29 Nov 2022 16:20
Operator : CG/JU
Sample : N5725-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB70

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

77	21.486	3106	3111	3121	rBV	5242230	6911971	96.38%	8.687%
78	23.833	3503	3510	3517	rBV	2523079	5212381	72.68%	6.551%
79	23.998	3531	3538	3552	rVB	2988765	6188796	86.29%	7.778%




Sum of corrected areas: 79569284

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012854.D
Acq On : 29 Nov 2022 16:20
Operator : CG/JU
Sample : N5725-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB70

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

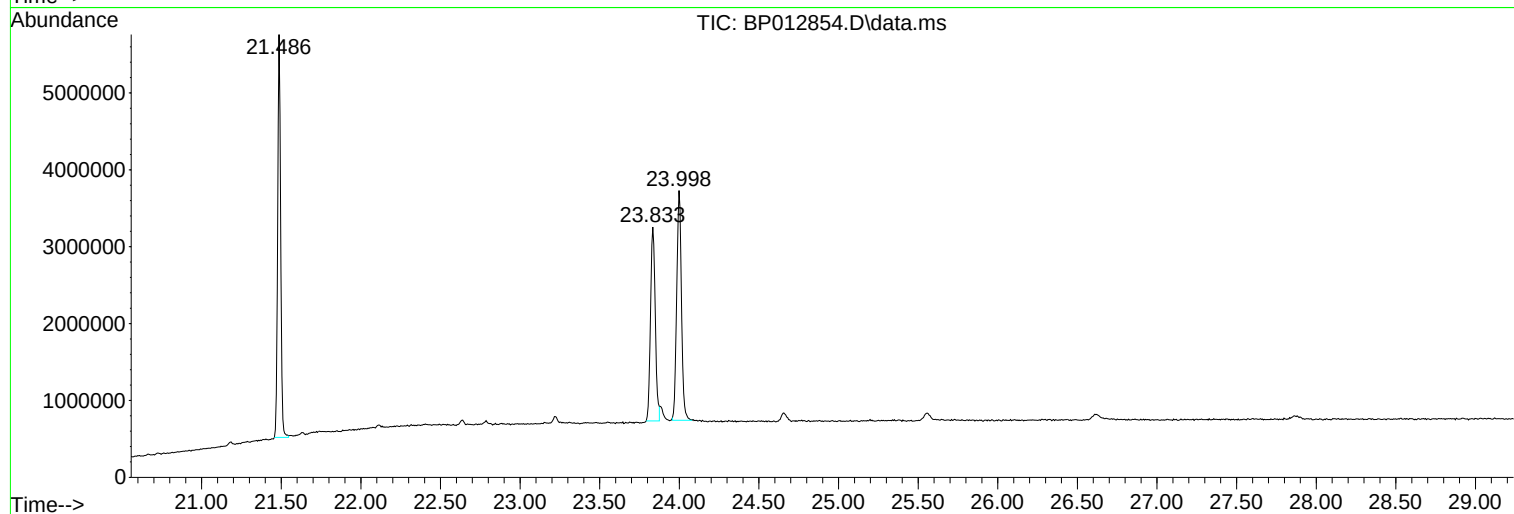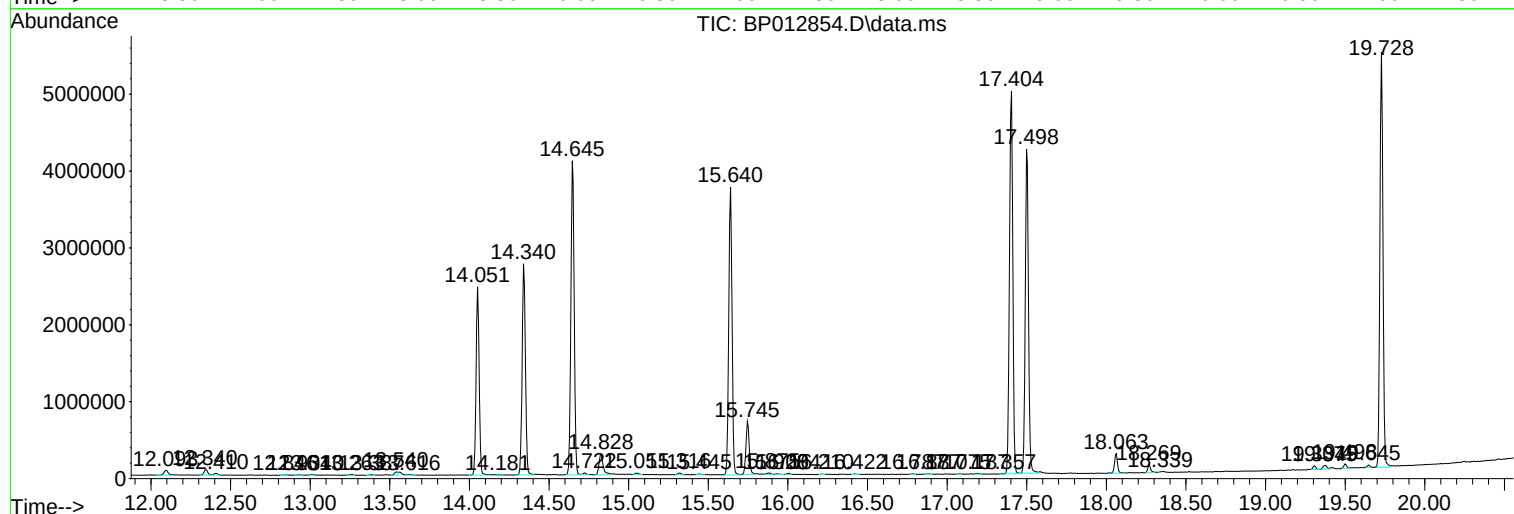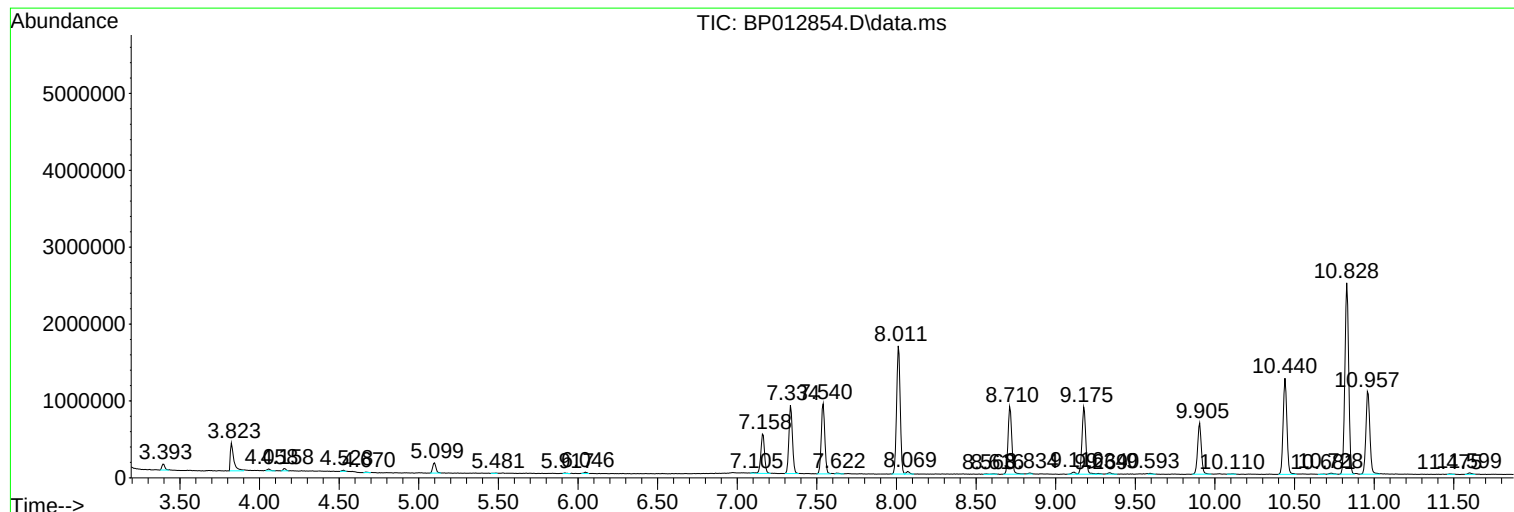

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012854.D
Acq On : 29 Nov 2022 16:20
Operator : CG/JU
Sample : N5725-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB70

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012854.D
Acq On : 29 Nov 2022 16:20
Operator : CG/JU
Sample : N5725-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB70

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc