

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012857.D
 Acq On : 29 Nov 2022 18:03
 Operator : CG/JU
 Sample : PB149233BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	32	35	49	rVB	135875	212690	1.47%	0.146%
2	3.822	104	108	131	rBV	1539514	2704459	18.70%	1.858%
3	4.158	161	165	171	rVB	30889	43909	0.30%	0.030%
4	7.163	669	676	686	rBV	1982099	3160375	21.85%	2.171%
5	7.334	699	705	716	rVB	1750036	2728467	18.87%	1.874%
6	7.540	733	740	749	rBV	2079460	3200541	22.13%	2.198%
7	8.010	813	820	828	rVB	1823866	2919693	20.19%	2.005%
8	8.716	932	940	956	rBV	2494860	4128750	28.55%	2.836%
9	9.181	1012	1019	1030	rBV	1872457	3063750	21.18%	2.104%
10	9.904	1135	1142	1154	rBV	1530114	2491242	17.23%	1.711%
11	10.440	1224	1233	1241	rBV	2666553	4306226	29.78%	2.958%
12	10.828	1290	1299	1307	rBV	2783349	4657913	32.21%	3.199%
13	10.963	1314	1322	1335	rBV	2678022	4601158	31.82%	3.160%
14	12.410	1559	1568	1575	rBV	45791	79132	0.55%	0.054%
15	13.381	1727	1733	1735	rBV6	8909	15427	0.11%	0.011%
16	13.539	1755	1760	1765	rVB5	16146	25804	0.18%	0.018%
17	13.622	1768	1774	1778	rVV5	11650	16854	0.12%	0.012%
18	14.051	1841	1847	1862	rBV	4999180	6835987	47.27%	4.695%
19	14.339	1889	1896	1907	rBV	5724031	8353211	57.76%	5.738%
20	14.645	1941	1948	1958	rBV	4714996	6859943	47.43%	4.712%
21	14.716	1958	1960	1967	rVB7	8927	16599	0.11%	0.011%
22	14.828	1972	1979	1992	rBV	2152169	3193273	22.08%	2.193%
23	15.051	2015	2017	2024	rVB8	10901	17458	0.12%	0.012%
24	15.639	2108	2117	2128	rBV	7781935	10863391	75.12%	7.462%
25	15.745	2129	2135	2143	rBV	1963883	2684168	18.56%	1.844%
26	15.881	2153	2158	2164	rVB2	35466	63633	0.44%	0.044%
27	17.075	2358	2361	2367	rVB8	12706	16830	0.12%	0.012%
28	17.186	2376	2380	2384	rBV2	12715	16571	0.11%	0.011%
29	17.404	2409	2417	2425	rBV	5816148	8432696	58.31%	5.792%
30	17.498	2427	2433	2448	rVV2	8197473	12069970	83.46%	8.291%
31	18.269	2560	2564	2573	rBV10	14201	27812	0.19%	0.019%
32	19.304	2736	2740	2747	rBV	101762	135478	0.94%	0.093%
33	19.374	2747	2752	2757	rBV	97675	160414	1.11%	0.110%
34	19.727	2806	2812	2822	rBV	11113253	14461903	100.00%	9.933%
35	21.486	3105	3111	3121	rBV	7134440	9588396	66.30%	6.586%
36	23.833	3502	3510	3529	rBV	6635315	13952857	96.48%	9.584%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012857.D
Acq On : 29 Nov 2022 18:03
Operator : CG/JU
Sample : PB149233BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK233

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	23.998	3530	3538	3558	rVB2	4458616	9480920	65.56%	6.512%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 145587900

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012857.D
Acq On : 29 Nov 2022 18:03
Operator : CG/JU
Sample : PB149233BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK233

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

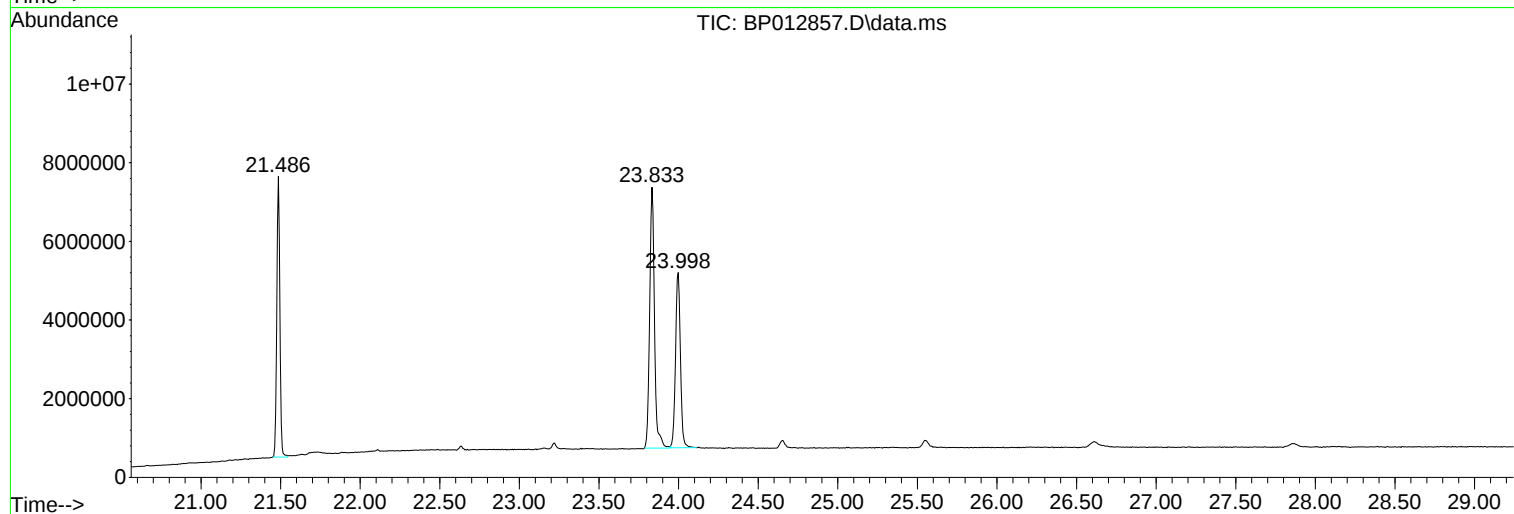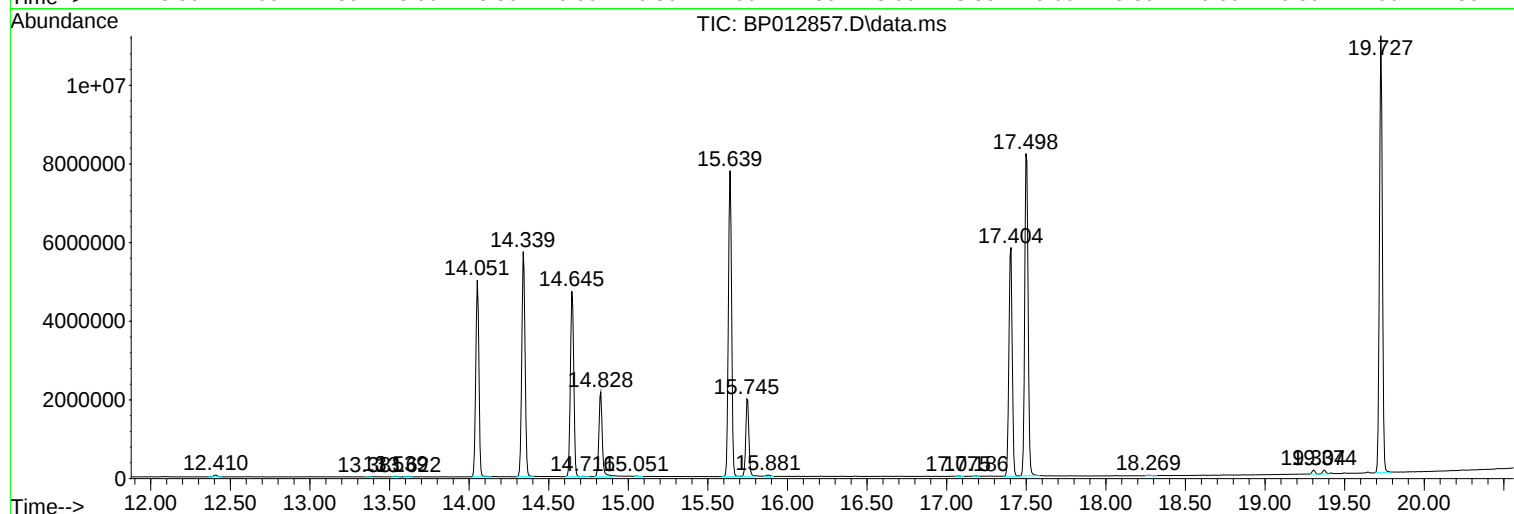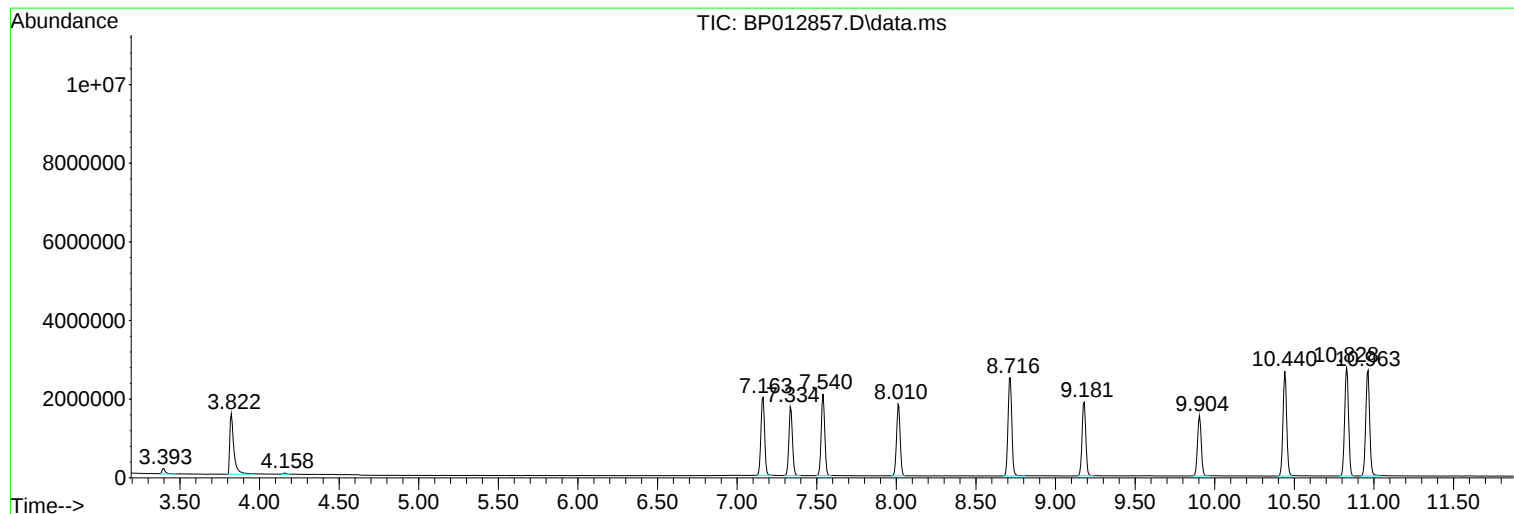

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012857.D
Acq On : 29 Nov 2022 18:03
Operator : CG/JU
Sample : PB149233BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK233

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012857.D
Acq On : 29 Nov 2022 18:03
Operator : CG/JU
Sample : PB149233BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK233

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc