

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012858.D
 Acq On : 29 Nov 2022 18:37
 Operator : CG/JU
 Sample : PB149234BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK234

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	43	rVB	167384	221242	1.49%	0.148%
2	3.817	104	107	124	rBV	1403691	2136713	14.38%	1.429%
3	4.158	161	165	171	rVB	35264	50864	0.34%	0.034%
4	7.163	669	676	685	rBV	2321216	3698724	24.90%	2.473%
5	7.334	698	705	714	rBV	2066154	3246901	21.85%	2.171%
6	7.540	733	740	749	rBV	2423333	3783623	25.47%	2.530%
7	8.010	813	820	828	rBV	2049293	3226204	21.72%	2.157%
8	8.710	932	939	957	rBV	3031348	4871587	32.79%	3.258%
9	9.175	1010	1018	1031	rBV	2192433	3686301	24.81%	2.465%
10	9.905	1134	1142	1152	rBV	1812223	2978972	20.05%	1.992%
11	10.440	1224	1233	1247	rBV	3076495	5072182	34.14%	3.392%
12	10.828	1291	1299	1309	rBV	3103568	5201204	35.01%	3.478%
13	10.957	1313	1321	1338	rBV	2477284	4331107	29.15%	2.896%
14	12.404	1559	1567	1573	rBV2	55360	93317	0.63%	0.062%
15	12.622	1597	1604	1610	rVB2	9052	19437	0.13%	0.013%
16	13.540	1755	1760	1764	rBV4	16173	24665	0.17%	0.016%
17	13.616	1768	1773	1779	rBV3	13169	21159	0.14%	0.014%
18	14.051	1840	1847	1857	rBV	5793761	8136767	54.77%	5.441%
19	14.340	1888	1896	1913	rBV	6949675	9898780	66.63%	6.619%
20	14.645	1940	1948	1957	rBV	5110504	7565867	50.93%	5.059%
21	14.722	1957	1961	1967	rVB8	10806	19081	0.13%	0.013%
22	14.828	1970	1979	2000	rBV	2353446	3541635	23.84%	2.368%
23	15.640	2107	2117	2129	rBV	8875678	12700919	85.49%	8.493%
24	15.745	2129	2135	2151	rVV	2192747	3133533	21.09%	2.095%
25	15.881	2153	2158	2163	rVB3	40852	67884	0.46%	0.045%
26	17.081	2356	2362	2364	rBV5	13209	21144	0.14%	0.014%
27	17.192	2377	2381	2386	rVB2	12512	20446	0.14%	0.014%
28	17.404	2409	2417	2427	rBV	6256171	8943838	60.20%	5.981%
29	17.504	2427	2434	2451	rVV	9414401	13578978	91.40%	9.080%
30	17.781	2477	2481	2487	rVB4	8523	17361	0.12%	0.012%
31	18.269	2561	2564	2569	rBV7	13064	19268	0.13%	0.013%
32	19.304	2736	2740	2745	rVB2	99726	130799	0.88%	0.087%
33	19.369	2747	2751	2756	rBV	95374	140865	0.95%	0.094%
34	19.645	2796	2798	2802	rBV5	21635	21412	0.14%	0.014%
35	19.728	2806	2812	2823	rBV	11214494	14856584	100.00%	9.934%
36	21.486	3106	3111	3120	rBV	5866209	7706525	51.87%	5.153%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012858.D
Acq On : 29 Nov 2022 18:37
Operator : CG/JU
Sample : PB149234BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	23.833	3503	3510	3525	rVB	4929642	10023798	67.47%	6.703%
38	23.998	3531	3538	3554	rVB2	2924598	6337865	42.66%	4.238%




Sum of corrected areas: 149547551

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012858.D
Acq On : 29 Nov 2022 18:37
Operator : CG/JU
Sample : PB149234BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

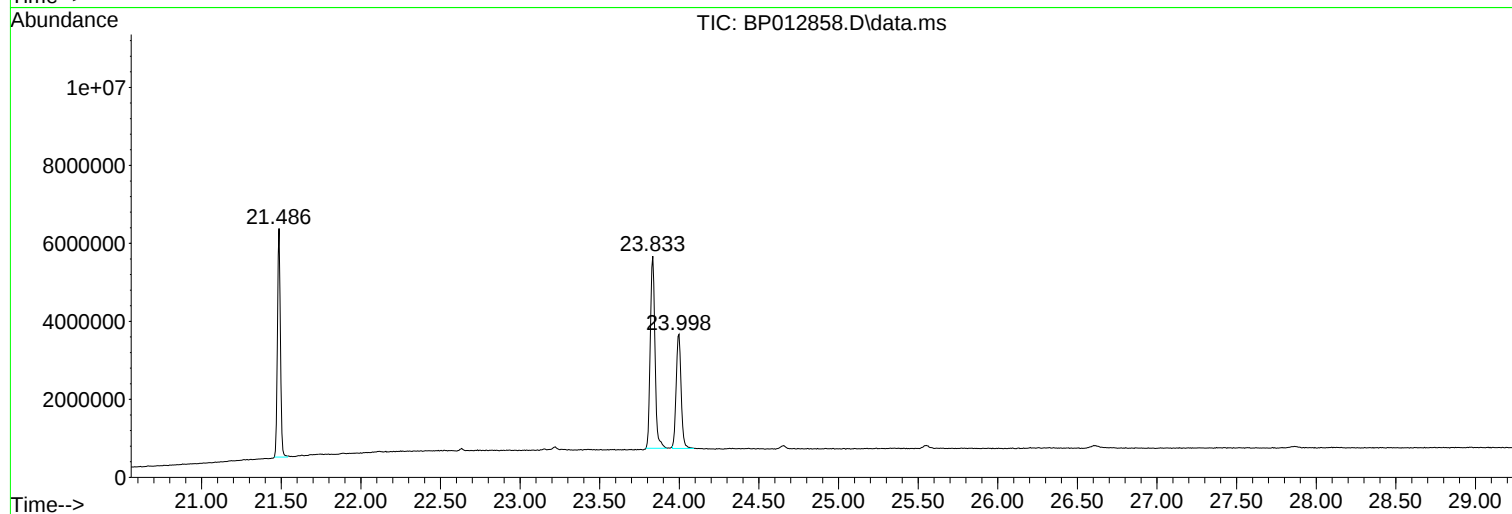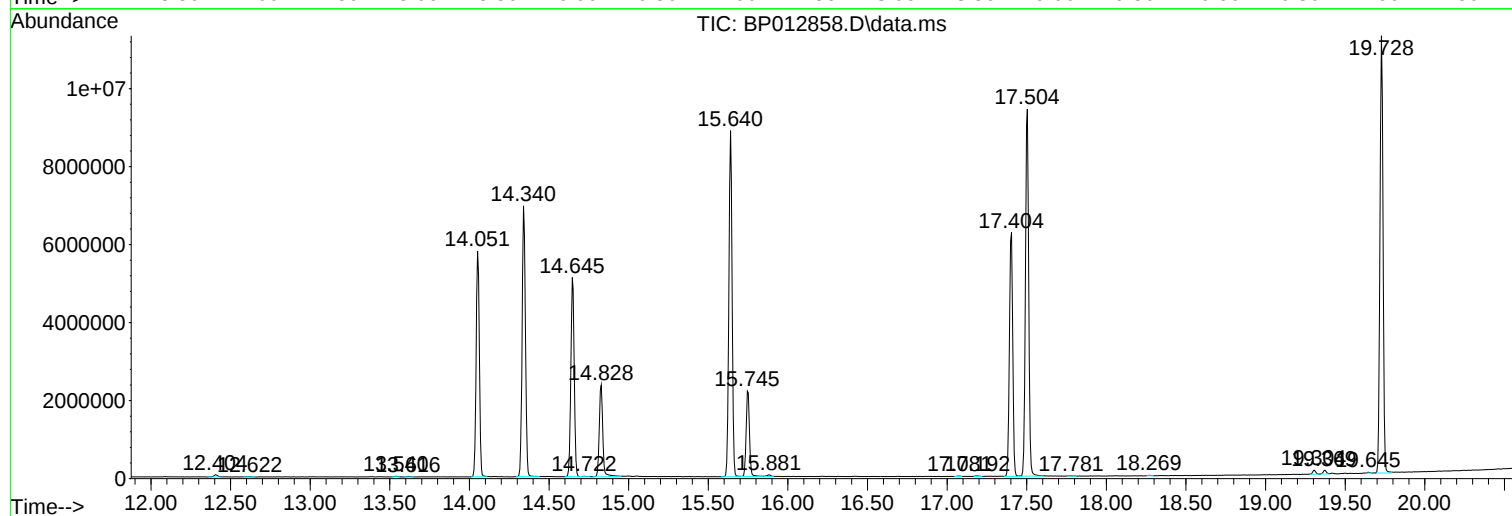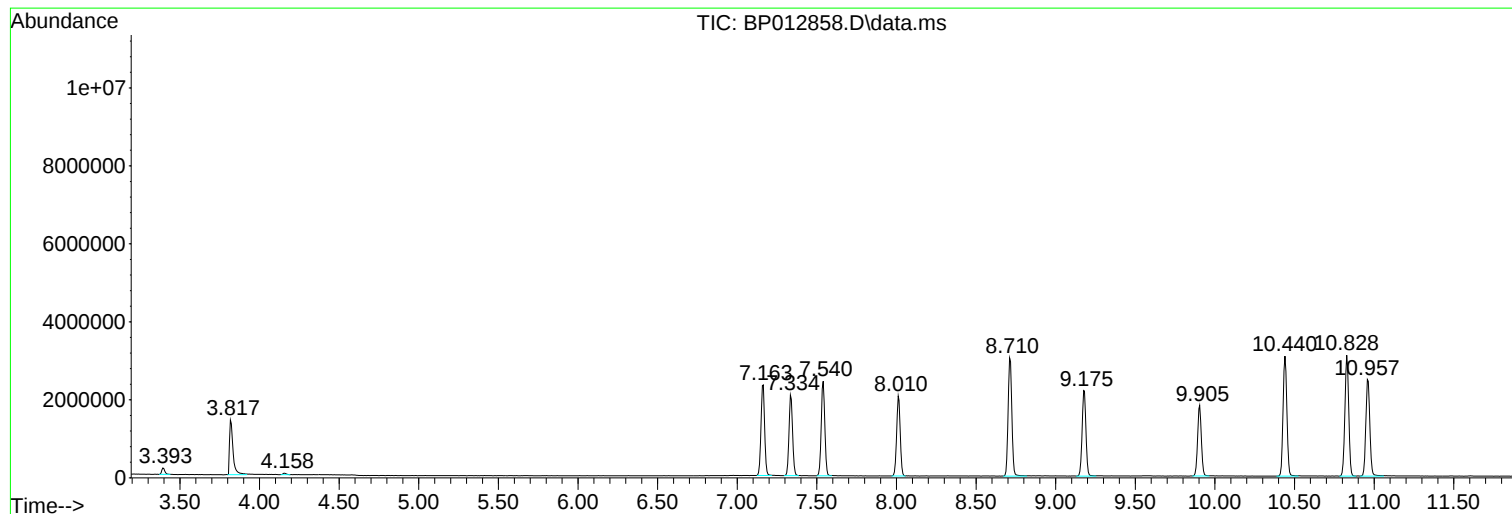

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012858.D
Acq On : 29 Nov 2022 18:37
Operator : CG/JU
Sample : PB149234BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012858.D
Acq On : 29 Nov 2022 18:37
Operator : CG/JU
Sample : PB149234BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
