

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012861.D
 Acq On : 29 Nov 2022 20:20
 Operator : CG/JU
 Sample : N5725-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	26	30	32	rBV2	49641	65740	0.41%	0.046%
2	3.393	32	35	39	rVV	93995	132246	0.82%	0.092%
3	3.434	39	42	49	rVB2	32354	46524	0.29%	0.032%
4	3.687	81	85	89	rBV	10992	18345	0.11%	0.013%
5	3.823	106	108	129	rBV	379319	668063	4.16%	0.466%
6	4.058	143	148	154	rBV	51801	80710	0.50%	0.056%
7	4.158	160	165	171	rBV	34646	53133	0.33%	0.037%
8	5.099	322	325	330	rVB3	11436	18175	0.11%	0.013%
9	7.158	667	675	687	rVB	416851	674069	4.19%	0.470%
10	7.334	698	705	725	rVB	1735404	2688710	16.73%	1.874%
11	7.540	732	740	750	rBV	1550738	2445711	15.22%	1.704%
12	7.628	750	755	760	rVB6	11309	19061	0.12%	0.013%
13	8.011	813	820	828	rBV	2063945	3320190	20.66%	2.314%
14	8.075	828	831	835	rVB4	13334	17367	0.11%	0.012%
15	8.393	880	885	893	rVB2	32179	57176	0.36%	0.040%
16	8.552	904	912	918	rBV	43039	73469	0.46%	0.051%
17	8.710	931	939	952	rBV	1284183	2077819	12.93%	1.448%
18	9.175	1010	1018	1030	rBV	1900612	3068369	19.09%	2.138%
19	9.410	1054	1058	1063	rVB2	17598	23641	0.15%	0.016%
20	9.505	1068	1074	1078	rBV5	7839	16323	0.10%	0.011%
21	9.593	1084	1089	1095	rVB4	25179	47702	0.30%	0.033%
22	9.905	1134	1142	1154	rBV	1403997	2307078	14.36%	1.608%
23	10.440	1225	1233	1245	rBV	2391432	3905894	24.30%	2.722%
24	10.828	1291	1299	1307	rBV	3199392	5345915	33.26%	3.726%
25	10.957	1314	1321	1333	rBV	1239856	2170786	13.51%	1.513%
26	11.599	1424	1430	1435	rBV6	22260	42126	0.26%	0.029%
27	12.093	1508	1514	1518	rVB8	9917	16628	0.10%	0.012%
28	12.404	1562	1567	1575	rVB2	47712	73652	0.46%	0.051%
29	12.610	1598	1602	1613	rVB2	6598	18066	0.11%	0.013%
30	13.381	1728	1733	1738	rBV8	9990	17999	0.11%	0.013%
31	13.469	1744	1748	1754	rVB7	10317	16934	0.11%	0.012%
32	13.540	1754	1760	1768	rVB3	33239	50238	0.31%	0.035%
33	13.616	1768	1773	1777	rBV4	11919	19287	0.12%	0.013%
34	14.051	1840	1847	1864	rBV	5364885	7203780	44.82%	5.021%
35	14.340	1889	1896	1915	rBV	5769007	8472087	52.72%	5.904%
36	14.516	1921	1926	1932	rVB5	17534	32213	0.20%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012861.D
 Acq On : 29 Nov 2022 20:20
 Operator : CG/JU
 Sample : N5725-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.645	1941	1948	1956	rBV	5401023	7862708	48.92%	5.480%
38	14.710	1956	1959	1967	rVB5	20529	34706	0.22%	0.024%
39	14.822	1972	1978	1997	rBV	295384	540254	3.36%	0.377%
40	15.045	2012	2016	2022	rVB6	36460	62945	0.39%	0.044%
41	15.440	2076	2083	2084	rBV6	8998	16218	0.10%	0.011%
42	15.640	2110	2117	2129	rBV	8055168	11506380	71.60%	8.019%
43	15.745	2129	2135	2146	rBV	1733596	2358279	14.67%	1.644%
44	15.881	2154	2158	2164	rVB2	34399	53388	0.33%	0.037%
45	16.781	2308	2311	2316	rBV5	13911	19644	0.12%	0.014%
46	17.075	2358	2361	2367	rVB8	12406	17472	0.11%	0.012%
47	17.187	2376	2380	2387	rVB2	27993	40524	0.25%	0.028%
48	17.404	2410	2417	2426	rBV	6446370	9646601	60.02%	6.723%
49	17.498	2427	2433	2445	rBV	8950666	13212997	82.21%	9.209%
50	17.681	2462	2464	2472	rVB8	9487	17435	0.11%	0.012%
51	18.057	2524	2528	2534	rBV	101713	131988	0.82%	0.092%
52	18.269	2559	2564	2573	rBV	201080	274557	1.71%	0.191%
53	19.304	2736	2740	2744	rBV3	114654	154670	0.96%	0.108%
54	19.369	2746	2751	2756	rBV	131889	225984	1.41%	0.157%
55	19.498	2769	2773	2778	rBV2	123259	156183	0.97%	0.109%
56	19.645	2795	2798	2802	rBV3	61147	64624	0.40%	0.045%
57	19.728	2806	2812	2822	rBV	12522885	16071357	100.00%	11.201%
58	21.175	3056	3058	3066	rVB3	144445	176324	1.10%	0.123%
59	21.486	3105	3111	3121	rBV	8014594	10557913	65.69%	7.358%
60	23.833	3502	3510	3525	rBV2	6985008	15005565	93.37%	10.458%
61	23.998	3531	3538	3554	rVB	4808931	9973021	62.05%	6.950%




Sum of corrected areas: 143486963

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012861.D
Acq On : 29 Nov 2022 20:20
Operator : CG/JU
Sample : N5725-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

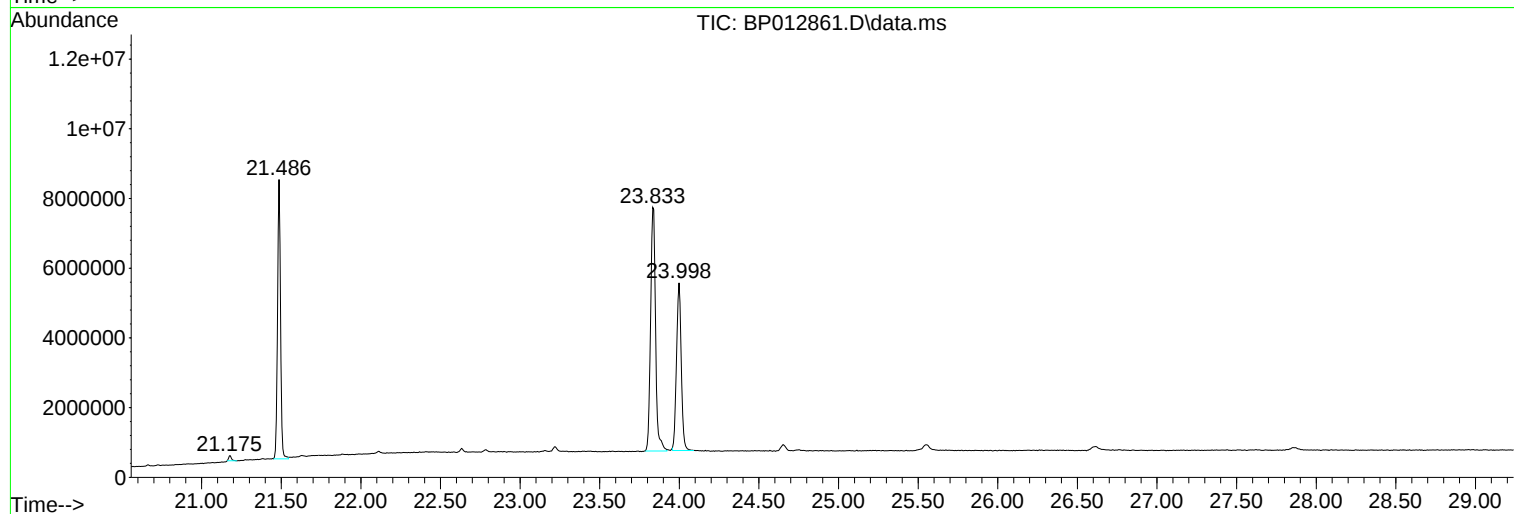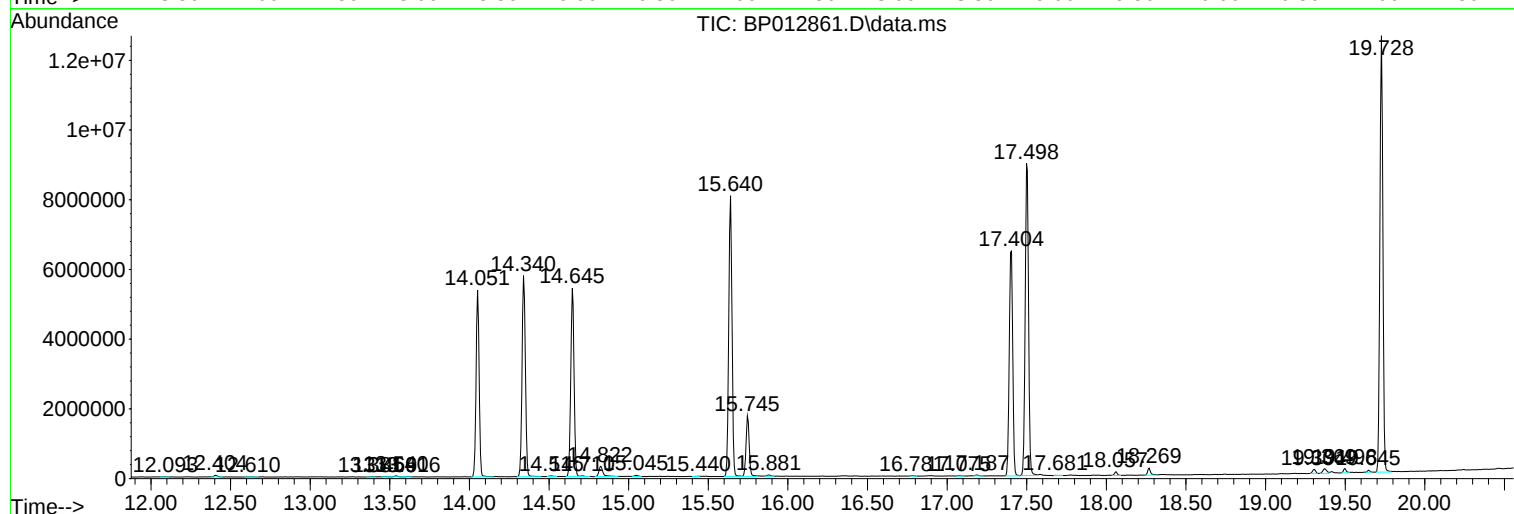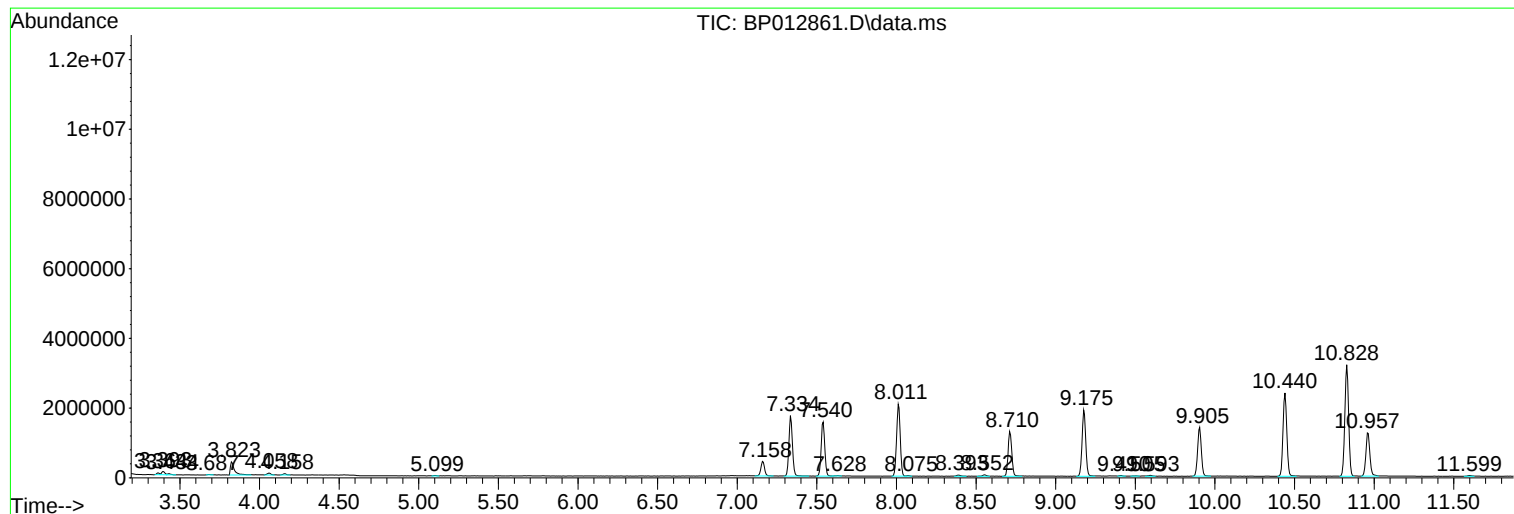

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012861.D
Acq On : 29 Nov 2022 20:20
Operator : CG/JU
Sample : N5725-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012861.D
Acq On : 29 Nov 2022 20:20
Operator : CG/JU
Sample : N5725-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc