

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012862.D
 Acq On : 29 Nov 2022 20:54
 Operator : CG/JU
 Sample : N5725-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	47	rVB	137847	200104	1.14%	0.129%
2	3.823	104	108	123	rBV	611485	945540	5.39%	0.611%
3	4.058	144	148	156	rVB	68005	104945	0.60%	0.068%
4	4.158	160	165	170	rBV	41692	62210	0.35%	0.040%
5	6.969	637	643	648	rBV10	8828	22736	0.13%	0.015%
6	7.158	669	675	685	rVB	654844	1015724	5.79%	0.657%
7	7.334	699	705	717	rBV	2208821	3418922	19.50%	2.210%
8	7.540	730	740	749	rBV	1893266	3032367	17.29%	1.960%
9	7.628	751	755	761	rVB5	14285	26569	0.15%	0.017%
10	8.011	811	820	827	rBV	2290890	3548423	20.23%	2.294%
11	8.387	879	884	893	rVB3	23202	44785	0.26%	0.029%
12	8.558	906	913	919	rBV6	13409	26969	0.15%	0.017%
13	8.711	932	939	949	rBV	1769017	2790300	15.91%	1.804%
14	9.175	1010	1018	1030	rBV	2420264	3935336	22.44%	2.544%
15	9.593	1082	1089	1097	rVB	43076	77816	0.44%	0.050%
16	9.905	1133	1142	1154	rBV	1749316	2928591	16.70%	1.893%
17	10.022	1156	1162	1167	rVV2	18769	38054	0.22%	0.025%
18	10.440	1225	1233	1246	rBV	2917063	4801225	27.38%	3.103%
19	10.828	1291	1299	1306	rBV	3420699	5706026	32.54%	3.688%
20	10.881	1306	1308	1314	rVB7	19314	26706	0.15%	0.017%
21	10.958	1314	1321	1335	rBV	1599634	2819681	16.08%	1.823%
22	11.599	1424	1430	1437	rVB8	15657	33400	0.19%	0.022%
23	12.404	1560	1567	1576	rVB	58707	100835	0.57%	0.065%
24	12.999	1660	1668	1671	rBV10	9461	22632	0.13%	0.015%
25	13.616	1767	1773	1778	rBV6	13862	26209	0.15%	0.017%
26	14.051	1840	1847	1860	rBV	6549060	8851041	50.47%	5.721%
27	14.340	1888	1896	1909	rBV2	7084721	10490087	59.82%	6.780%
28	14.534	1925	1929	1934	rVB6	13509	23500	0.13%	0.015%
29	14.646	1938	1948	1955	rVV	5693488	8266439	47.14%	5.343%
30	14.710	1955	1959	1966	rVB5	31358	60690	0.35%	0.039%
31	14.828	1971	1979	1986	rBV	504997	803056	4.58%	0.519%
32	14.993	2001	2007	2012	rBV8	15669	36333	0.21%	0.023%
33	15.046	2012	2016	2022	rVB4	41531	71503	0.41%	0.046%
34	15.545	2098	2101	2107	rBV3	16055	23493	0.13%	0.015%
35	15.640	2110	2117	2129	rBV	9852228	13805966	78.72%	8.924%
36	15.745	2129	2135	2148	rBV	2530678	3440962	19.62%	2.224%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012862.D
 Acq On : 29 Nov 2022 20:54
 Operator : CG/JU
 Sample : N5725-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.881	2154	2158	2163	rBV2	40340	64013	0.37%	0.041%
38	16.351	2236	2238	2245	rVV6	14901	22613	0.13%	0.015%
39	16.422	2248	2250	2254	rVB5	15099	18980	0.11%	0.012%
40	16.604	2277	2281	2286	rVB7	27183	36624	0.21%	0.024%
41	16.898	2327	2331	2336	rVB3	36152	71027	0.41%	0.046%
42	17.151	2371	2374	2377	rBV4	16844	21513	0.12%	0.014%
43	17.187	2377	2380	2387	rVB5	29960	52910	0.30%	0.034%
44	17.398	2410	2416	2423	rBV	6507476	9806906	55.92%	6.339%
45	17.498	2427	2433	2449	rVV	10365759	15399141	87.81%	9.953%
46	18.057	2525	2528	2532	rVB4	41588	50449	0.29%	0.033%
47	18.269	2559	2564	2569	rBV	222406	297152	1.69%	0.192%
48	18.351	2574	2578	2583	rVV5	24843	48136	0.27%	0.031%
49	18.681	2631	2634	2638	rBV3	73299	89245	0.51%	0.058%
50	19.304	2736	2740	2745	rBV	146405	194327	1.11%	0.126%
51	19.369	2747	2751	2756	rBV	143474	234843	1.34%	0.152%
52	19.498	2769	2773	2778	rBV	170613	220842	1.26%	0.143%
53	19.645	2795	2798	2805	rVB4	60629	73142	0.42%	0.047%
54	19.728	2806	2812	2822	rBV	13551148	17537358	100.00%	11.336%
55	21.486	3105	3111	3123	rBV	6606899	8992099	51.27%	5.812%
56	23.833	3502	3510	3527	rVV2	5854697	12387326	70.63%	8.007%
57	23.992	3530	3537	3552	rVB2	3521395	7463787	42.56%	4.824%




Sum of corrected areas: 154711608

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012862.D
Acq On : 29 Nov 2022 20:54
Operator : CG/JU
Sample : N5725-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB59

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

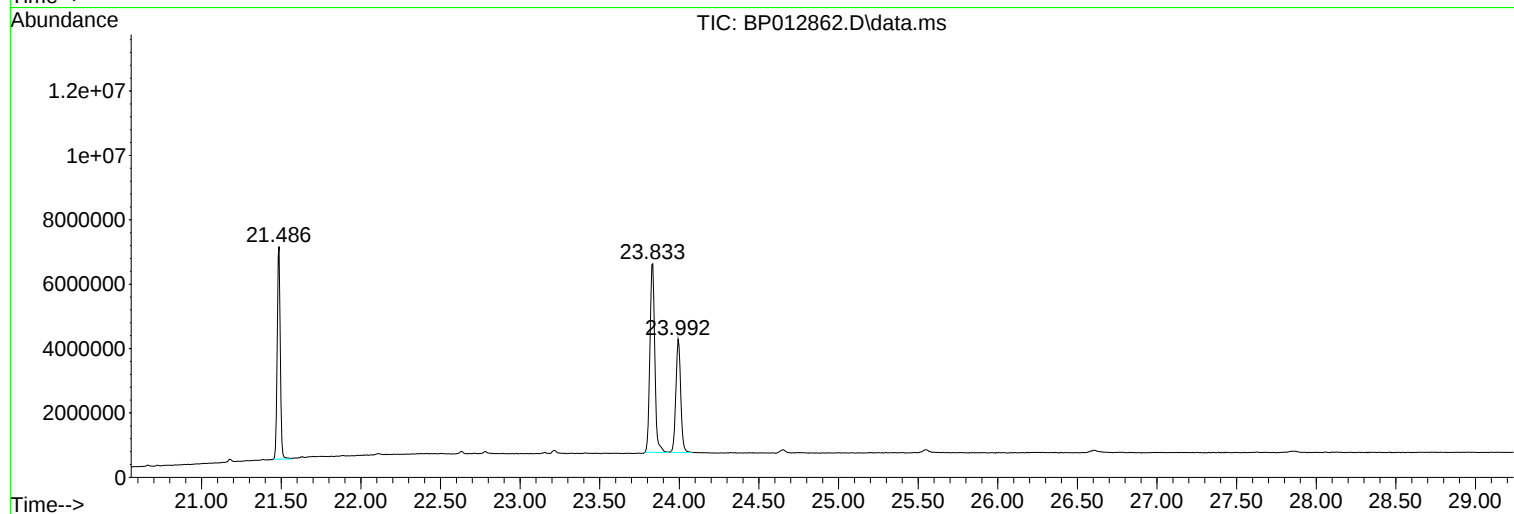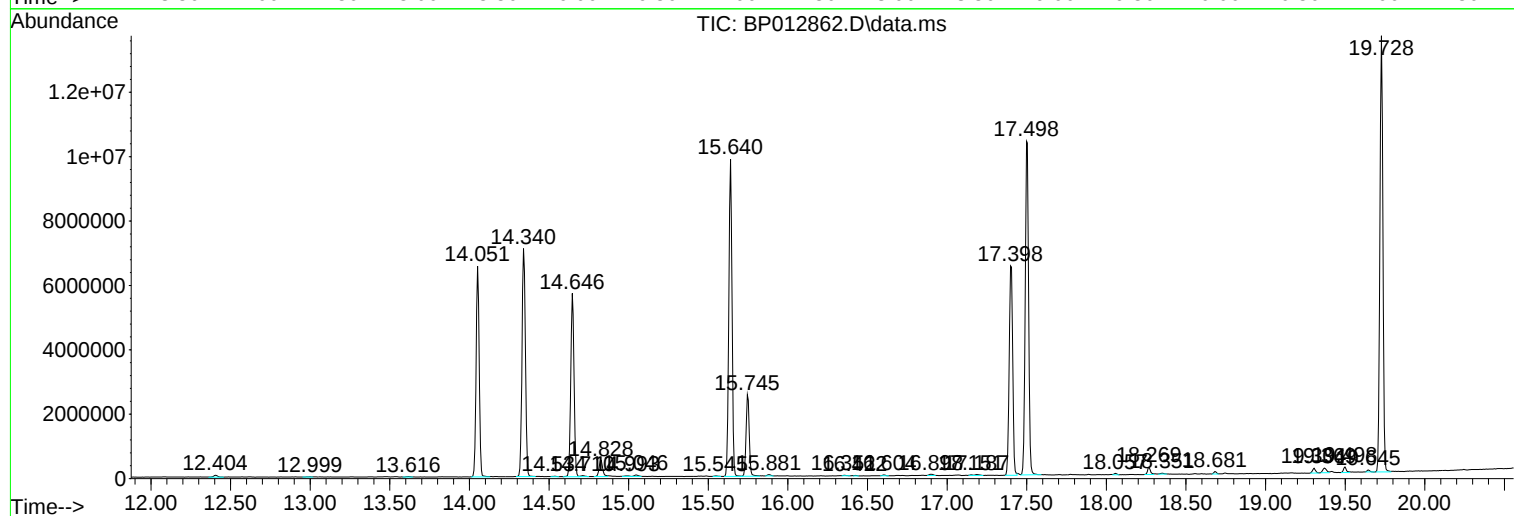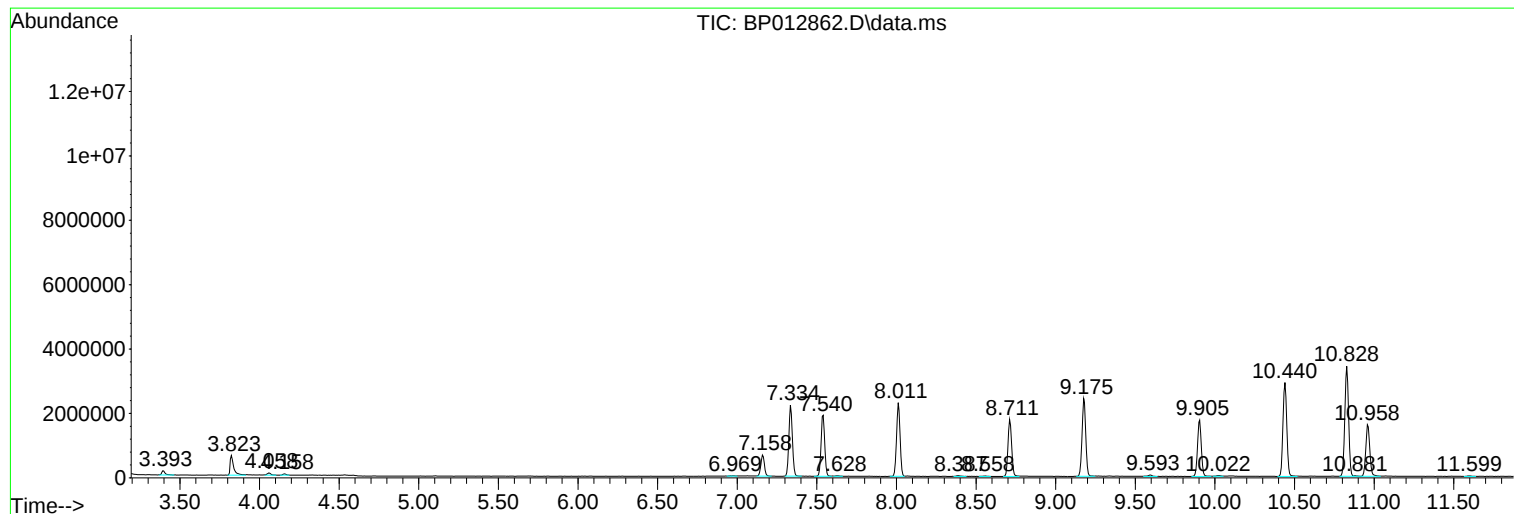

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012862.D
Acq On : 29 Nov 2022 20:54
Operator : CG/JU
Sample : N5725-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB59

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012862.D
Acq On : 29 Nov 2022 20:54
Operator : CG/JU
Sample : N5725-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB59

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc