

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012863.D
 Acq On : 29 Nov 2022 21:28
 Operator : CG/JU
 Sample : N5725-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	25	30	33	rBV	189211	272078	1.56%	0.193%
2	3.393	33	35	38	rVV	104997	128754	0.74%	0.091%
3	3.428	38	41	54	rVB	226849	328985	1.88%	0.233%
4	3.823	106	108	126	rBV2	407104	779380	4.45%	0.553%
5	4.058	143	148	154	rBV2	40441	66629	0.38%	0.047%
6	4.158	161	165	170	rVB2	30045	41813	0.24%	0.030%
7	7.158	669	675	683	rBV	484900	752897	4.30%	0.534%
8	7.334	699	705	716	rVB	1664971	2568091	14.68%	1.821%
9	7.540	730	740	749	rBV	1546468	2431685	13.90%	1.724%
10	7.628	752	755	762	rVB8	12178	19928	0.11%	0.014%
11	8.011	812	820	827	rBV	1657422	2601710	14.87%	1.845%
12	8.075	827	831	836	rVB8	10126	19088	0.11%	0.014%
13	8.711	929	939	953	rBV	1412856	2200679	12.58%	1.561%
14	9.175	1009	1018	1030	rBV	1823424	2937933	16.79%	2.083%
15	9.269	1030	1034	1040	rVB2	19624	35023	0.20%	0.025%
16	9.905	1134	1142	1150	rBV	1403465	2270903	12.98%	1.610%
17	10.440	1225	1233	1248	rBV	2356389	3827828	21.88%	2.715%
18	10.828	1292	1299	1308	rBV	2587896	4256373	24.33%	3.018%
19	10.957	1314	1321	1334	rBV	1414759	2440449	13.95%	1.731%
20	11.181	1352	1359	1367	rBV8	15981	33088	0.19%	0.023%
21	12.210	1525	1534	1540	rBV8	13137	32509	0.19%	0.023%
22	12.404	1558	1567	1574	rVB	47402	85458	0.49%	0.061%
23	12.540	1586	1590	1595	rBV6	12345	20025	0.11%	0.014%
24	13.540	1754	1760	1764	rBV	41981	61578	0.35%	0.044%
25	13.616	1769	1773	1778	rVB2	11160	17692	0.10%	0.013%
26	14.051	1839	1847	1858	rBV	5037805	6830234	39.04%	4.844%
27	14.340	1889	1896	1912	rBV	5763227	8137242	46.51%	5.771%
28	14.646	1937	1948	1956	rBV	4494155	6347160	36.28%	4.501%
29	14.710	1956	1959	1965	rVB4	28284	48117	0.28%	0.034%
30	14.822	1972	1978	1992	rBV	436231	711508	4.07%	0.505%
31	15.051	2012	2017	2024	rVB7	30393	60489	0.35%	0.043%
32	15.640	2110	2117	2129	rBV	8181631	11253480	64.32%	7.980%
33	15.745	2129	2135	2145	rBV	2235616	3008998	17.20%	2.134%
34	15.881	2154	2158	2165	rVB	35357	55651	0.32%	0.039%
35	16.204	2209	2213	2219	rBV8	10085	19720	0.11%	0.014%
36	16.363	2231	2240	2248	rBV3	79370	148678	0.85%	0.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012863.D
 Acq On : 29 Nov 2022 21:28
 Operator : CG/JU
 Sample : N5725-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	17.016	2346	2351	2356	rBV3	25414	41487	0.24%	0.029%
38	17.398	2410	2416	2425	rBV	5403428	7970097	45.56%	5.652%
39	17.504	2427	2434	2447	rBV	9244576	13458791	76.93%	9.544%
40	17.681	2460	2464	2471	rVB	17441	24734	0.14%	0.018%
41	17.775	2478	2480	2489	rVB6	15883	29519	0.17%	0.021%
42	17.892	2496	2500	2503	rBV4	13677	17807	0.10%	0.013%
43	18.057	2525	2528	2532	rVB3	25727	33856	0.19%	0.024%
44	18.269	2559	2564	2568	rBV	102541	141826	0.81%	0.101%
45	18.457	2592	2596	2599	rVB2	24413	31537	0.18%	0.022%
46	18.681	2631	2634	2638	rBV4	35460	43877	0.25%	0.031%
47	19.304	2736	2740	2745	rVB3	122871	173512	0.99%	0.123%
48	19.369	2747	2751	2754	rVV	113248	162304	0.93%	0.115%
49	19.404	2754	2757	2762	rVB2	68948	109409	0.63%	0.078%
50	19.498	2769	2773	2778	rBV3	98936	118988	0.68%	0.084%
51	19.645	2795	2798	2803	rVB3	51937	71104	0.41%	0.050%
52	19.728	2806	2812	2827	rVV	12615822	16778933	95.91%	11.899%
53	21.486	3105	3111	3122	rBV	7211793	9709247	55.50%	6.885%
54	23.833	3502	3510	3527	rBV2	8351703	17495007	100.00%	12.407%
55	23.998	3530	3538	3550	rVB2	4609620	9749360	55.73%	6.914%




Sum of corrected areas: 141013248

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012863.D
Acq On : 29 Nov 2022 21:28
Operator : CG/JU
Sample : N5725-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

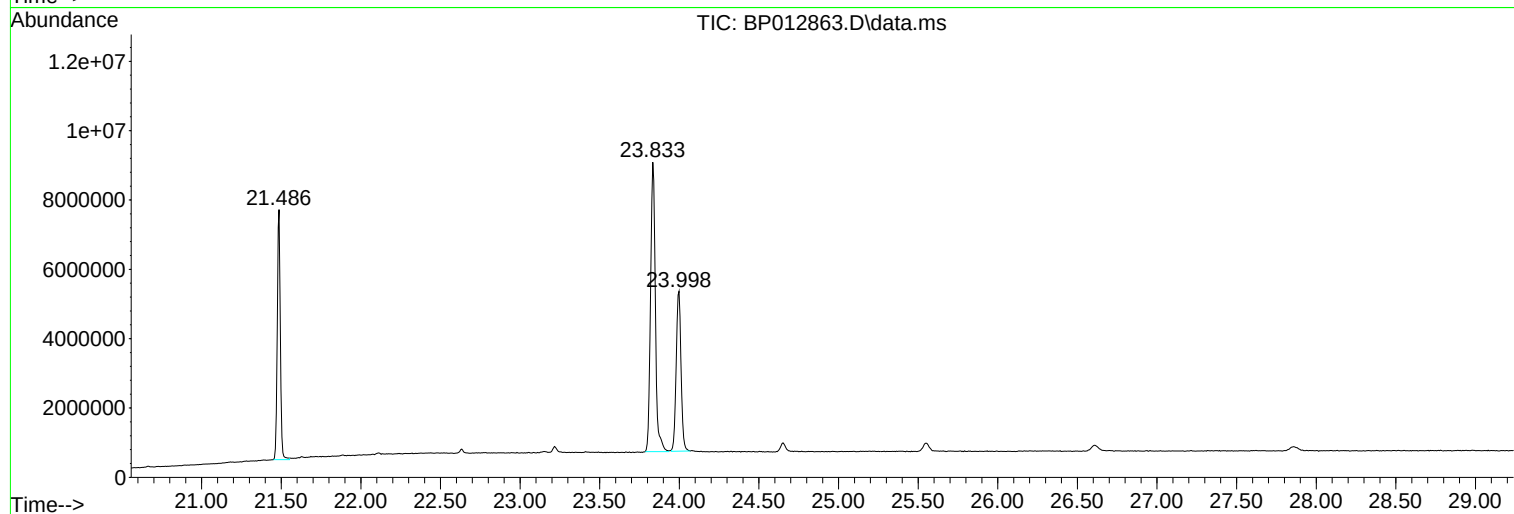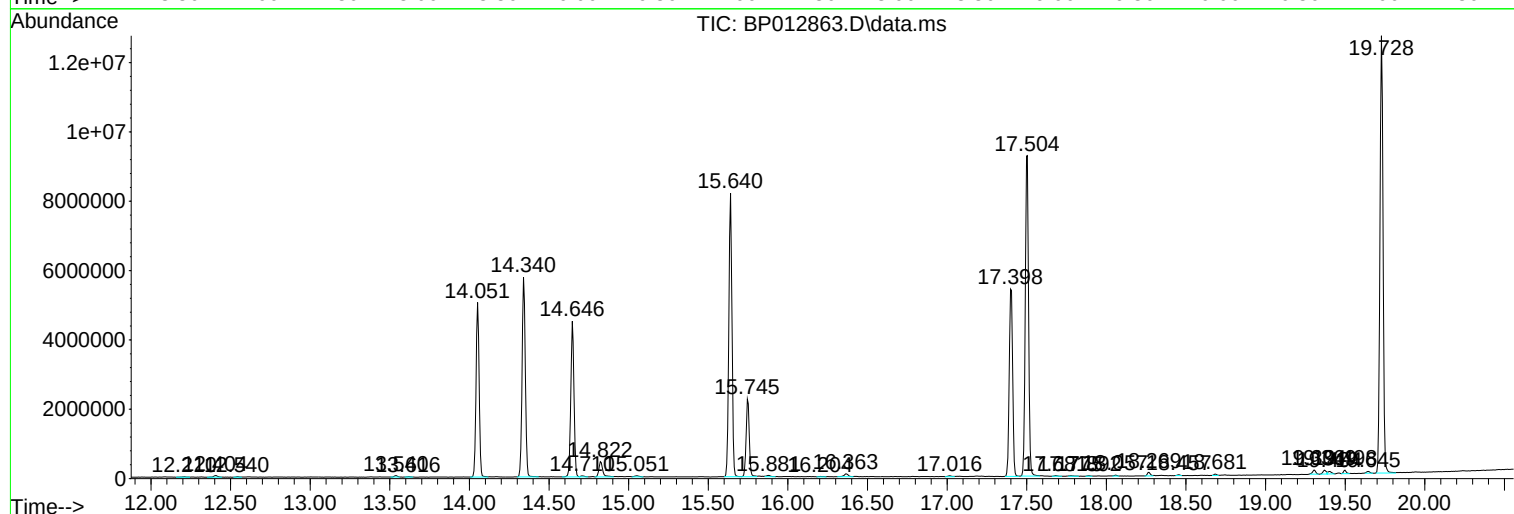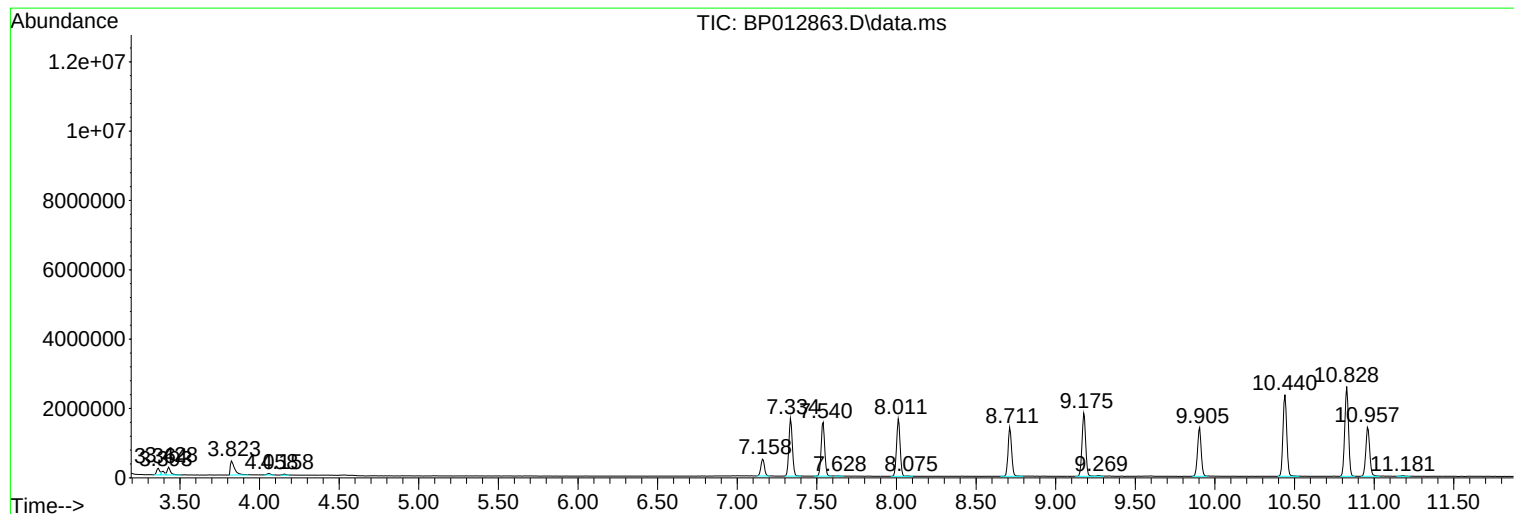

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012863.D
Acq On : 29 Nov 2022 21:28
Operator : CG/JU
Sample : N5725-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012863.D
Acq On : 29 Nov 2022 21:28
Operator : CG/JU
Sample : N5725-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc