

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012866.D
 Acq On : 29 Nov 2022 23:10
 Operator : CG/JU
 Sample : N5725-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	25	30	33	rBV	351850	484583	3.23%	0.328%
2	3.399	33	36	38	rVV	168589	215508	1.44%	0.146%
3	3.434	38	42	51	rVB	324396	443782	2.96%	0.301%
4	3.822	106	108	122	rBV2	536102	978304	6.52%	0.663%
5	4.058	144	148	152	rVB	65046	95736	0.64%	0.065%
6	4.158	161	165	171	rVB	42678	57581	0.38%	0.039%
7	4.534	227	229	236	rVB6	15679	21550	0.14%	0.015%
8	7.157	668	675	688	rVB	703454	1121676	7.48%	0.760%
9	7.334	697	705	713	rBV	2321729	3599860	24.01%	2.439%
10	7.540	733	740	749	rBV	2146977	3420008	22.81%	2.317%
11	7.622	750	754	760	rVB8	14729	25437	0.17%	0.017%
12	8.010	812	820	828	rBV	2394490	3714079	24.77%	2.517%
13	8.069	828	830	835	rVB4	15287	17941	0.12%	0.012%
14	8.710	930	939	951	rBV	1915006	3053192	20.36%	2.069%
15	9.175	1010	1018	1029	rBV	2526365	4055250	27.04%	2.748%
16	9.281	1030	1036	1042	rVV	106072	162162	1.08%	0.110%
17	9.593	1083	1089	1095	rVB	44608	73509	0.49%	0.050%
18	9.904	1132	1142	1154	rBV	1914046	3186968	21.25%	2.160%
19	10.440	1225	1233	1247	rBV	3191361	5161184	34.42%	3.497%
20	10.828	1291	1299	1307	rBV	3378210	5807431	38.73%	3.935%
21	10.957	1312	1321	1332	rBV	1678048	2830257	18.87%	1.918%
22	11.181	1353	1359	1365	rBV3	25686	41805	0.28%	0.028%
23	11.598	1425	1430	1436	rBV10	11460	23990	0.16%	0.016%
24	12.087	1505	1513	1517	rVB6	9727	21853	0.15%	0.015%
25	12.210	1527	1534	1536	rBV5	15378	29341	0.20%	0.020%
26	12.240	1536	1539	1543	rVB2	22813	30809	0.21%	0.021%
27	12.404	1559	1567	1572	rBV2	58072	95017	0.63%	0.064%
28	12.616	1596	1603	1607	rBV10	11593	25961	0.17%	0.018%
29	13.387	1728	1734	1736	rBV5	12543	18821	0.13%	0.013%
30	13.469	1738	1748	1753	rVV4	26551	52500	0.35%	0.036%
31	13.540	1753	1760	1765	rVV2	46903	78688	0.52%	0.053%
32	13.616	1767	1773	1778	rVB4	14434	28588	0.19%	0.019%
33	13.963	1829	1832	1837	rBV7	9842	15372	0.10%	0.010%
34	14.051	1840	1847	1862	rBV	6346290	8735841	58.26%	5.920%
35	14.339	1889	1896	1907	rBV	7412154	10481876	69.90%	7.103%
36	14.645	1939	1948	1955	rBV	5479046	8039237	53.61%	5.448%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012866.D
 Acq On : 29 Nov 2022 23:10
 Operator : CG/JU
 Sample : N5725-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.710	1955	1959	1964	rVB	41599	65560	0.44%	0.044%
38	14.822	1973	1978	1987	rBV	444528	707992	4.72%	0.480%
39	15.051	2011	2017	2022	rVB4	42852	75376	0.50%	0.051%
40	15.575	2102	2106	2110	rBV5	9689	18948	0.13%	0.013%
41	15.639	2110	2117	2129	rBV	9921556	14069451	93.83%	9.534%
42	15.745	2129	2135	2146	rBV	2562048	3372714	22.49%	2.285%
43	15.881	2154	2158	2165	rVB2	45609	71936	0.48%	0.049%
44	16.004	2173	2179	2183	rVB	46883	65451	0.44%	0.044%
45	16.210	2209	2214	2220	rVB9	9585	18667	0.12%	0.013%
46	16.363	2232	2240	2247	rBV2	100345	190536	1.27%	0.129%
47	16.422	2247	2250	2254	rVB6	14412	20669	0.14%	0.014%
48	16.786	2306	2312	2315	rBV8	12183	23551	0.16%	0.016%
49	17.010	2347	2350	2355	rBV	29380	48455	0.32%	0.033%
50	17.186	2376	2380	2383	rBV2	12263	20984	0.14%	0.014%
51	17.404	2410	2417	2427	rBV	5817445	8539257	56.95%	5.786%
52	17.498	2427	2433	2444	rVV	10403267	14994893	100.00%	10.161%
53	17.586	2444	2448	2456	rVV5	47474	90096	0.60%	0.061%
54	17.680	2460	2464	2469	rBV	17817	25752	0.17%	0.017%
55	17.892	2496	2500	2504	rBV5	13634	22046	0.15%	0.015%
56	18.057	2524	2528	2534	rVB7	24544	35054	0.23%	0.024%
57	18.269	2559	2564	2568	rBV2	110601	150555	1.00%	0.102%
58	18.451	2592	2595	2602	rVB2	33170	52336	0.35%	0.035%
59	18.686	2631	2635	2639	rBV6	18358	24377	0.16%	0.017%
60	18.745	2643	2645	2651	rVV7	10675	15262	0.10%	0.010%
61	19.304	2736	2740	2746	rVB	111787	150250	1.00%	0.102%
62	19.369	2747	2751	2754	rBV2	105151	160964	1.07%	0.109%
63	19.498	2769	2773	2777	rBV5	62148	83287	0.56%	0.056%
64	19.645	2794	2798	2803	rVB5	48184	66708	0.44%	0.045%
65	19.727	2806	2812	2821	rBV	11181905	14689499	97.96%	9.954%
66	21.486	3105	3111	3119	rBV	4378275	6073838	40.51%	4.116%
67	23.833	3502	3510	3524	rBV	5539556	11373408	75.85%	7.707%
68	23.992	3530	3537	3548	rVB2	2861573	6010085	40.08%	4.073%




Sum of corrected areas: 147573654

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012866.D
Acq On : 29 Nov 2022 23:10
Operator : CG/JU
Sample : N5725-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

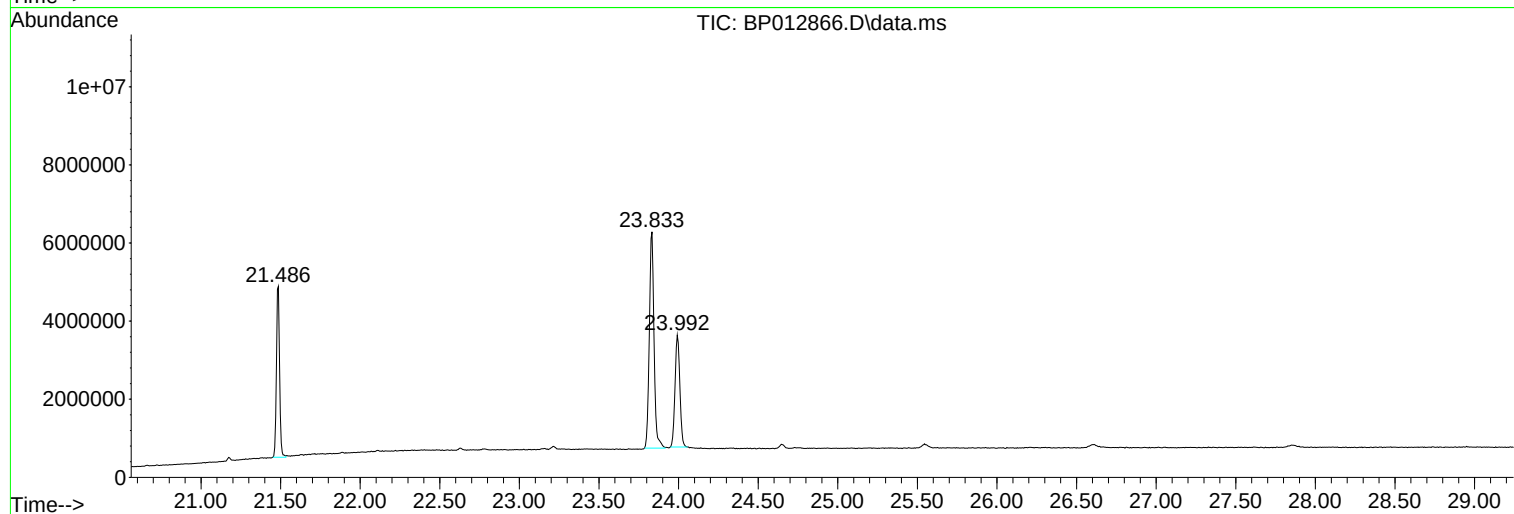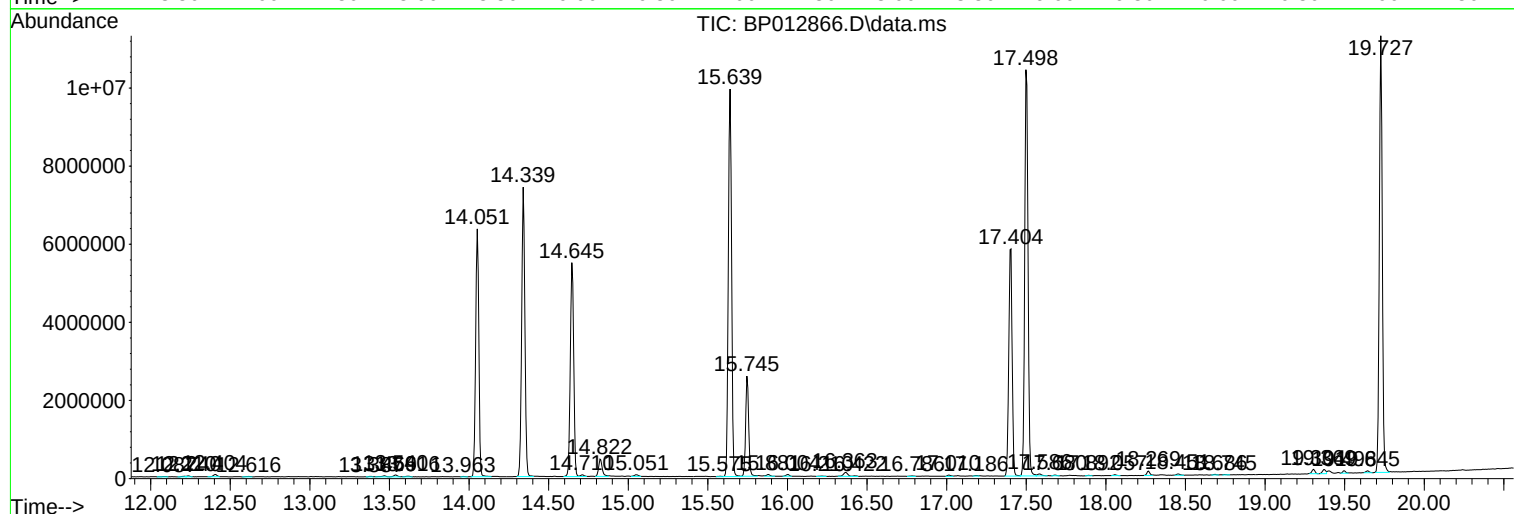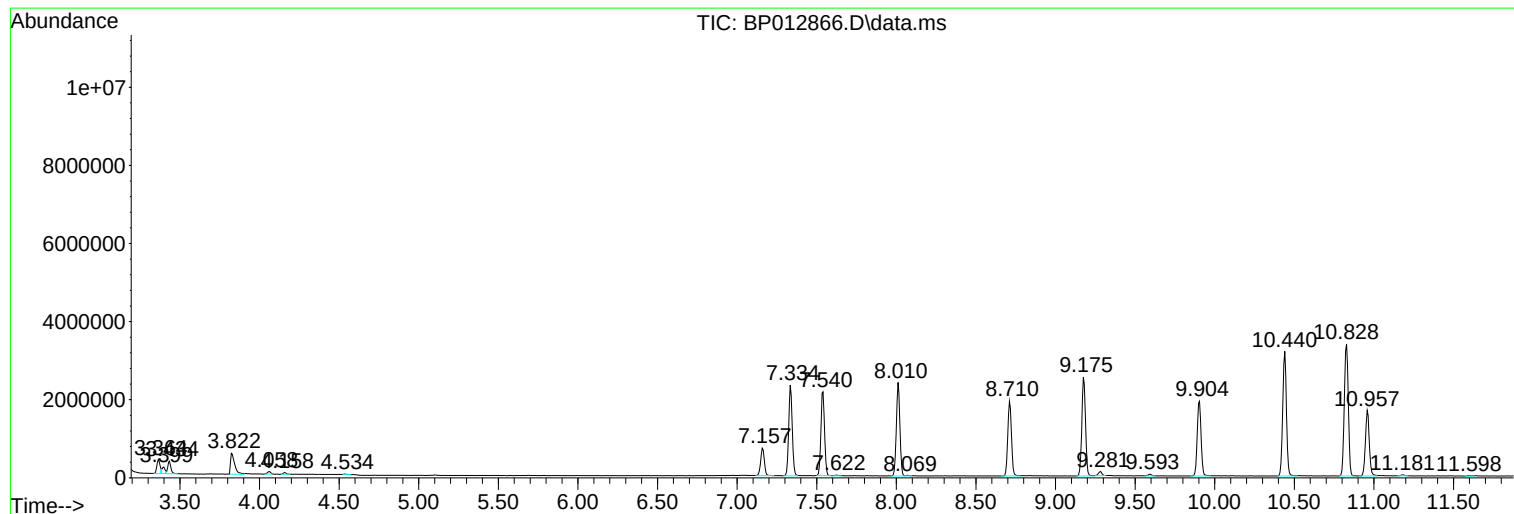

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012866.D
Acq On : 29 Nov 2022 23:10
Operator : CG/JU
Sample : N5725-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012866.D
Acq On : 29 Nov 2022 23:10
Operator : CG/JU
Sample : N5725-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc