

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012868.D
 Acq On : 30 Nov 2022 00:19
 Operator : CG/JU
 Sample : N5725-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	48	rVB	111875	163721	0.98%	0.108%
2	3.681	81	84	89	rBV	15867	26310	0.16%	0.017%
3	3.823	105	108	128	rBV	653220	1036022	6.23%	0.681%
4	4.058	143	148	161	rVB	68969	108935	0.65%	0.072%
5	4.158	161	165	169	rVB2	39882	54783	0.33%	0.036%
6	4.534	225	229	234	rVB7	11858	18722	0.11%	0.012%
7	5.099	321	325	330	rVB6	10794	16830	0.10%	0.011%
8	7.158	669	675	689	rVB	475838	751996	4.52%	0.494%
9	7.334	698	705	714	rBV	2044319	3155446	18.96%	2.074%
10	7.534	731	739	748	rBV	1733975	2804319	16.85%	1.843%
11	7.628	750	755	762	rVB9	15941	32869	0.20%	0.022%
12	8.011	812	820	827	rBV	2221036	3491522	20.98%	2.295%
13	8.069	827	830	838	rVB6	17236	30809	0.19%	0.020%
14	8.710	931	939	948	rBV	1518208	2361775	14.19%	1.552%
15	9.175	1010	1018	1027	rBV	2315389	3685146	22.14%	2.422%
16	9.269	1031	1034	1040	rVV8	14706	29565	0.18%	0.019%
17	9.593	1082	1089	1094	rBV	27701	47405	0.28%	0.031%
18	9.899	1134	1141	1155	rBV	1732104	2883611	17.33%	1.895%
19	10.440	1224	1233	1248	rBV	2891314	4747658	28.53%	3.120%
20	10.828	1291	1299	1307	rBV	3323582	5633560	33.85%	3.703%
21	10.957	1312	1321	1336	rBV	2193375	3677289	22.10%	2.417%
22	11.599	1424	1430	1436	rBV6	24833	43166	0.26%	0.028%
23	12.234	1534	1538	1543	rVB4	15297	25806	0.16%	0.017%
24	12.404	1561	1567	1574	rVV	59124	96929	0.58%	0.064%
25	13.469	1744	1748	1752	rVB2	16010	22028	0.13%	0.014%
26	13.534	1754	1759	1764	rVV	41097	68152	0.41%	0.045%
27	13.616	1768	1773	1779	rBV6	14014	24955	0.15%	0.016%
28	14.051	1839	1847	1862	rBV	6348837	8557912	51.43%	5.625%
29	14.340	1889	1896	1911	rBV	7021317	10407694	62.54%	6.841%
30	14.645	1941	1948	1956	rVB	5625401	8236305	49.49%	5.413%
31	14.828	1972	1979	1985	rBV	326792	537563	3.23%	0.353%
32	15.051	2012	2017	2022	rVB4	33199	55409	0.33%	0.036%
33	15.440	2080	2083	2087	rVV3	12497	17910	0.11%	0.012%
34	15.640	2110	2117	2128	rBV	9658432	13447118	80.81%	8.838%
35	15.745	2129	2135	2148	rVV	2417052	3189033	19.16%	2.096%
36	15.881	2154	2158	2162	rVB3	37762	56425	0.34%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012868.D
 Acq On : 30 Nov 2022 00:19
 Operator : CG/JU
 Sample : N5725-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	16.422	2244	2250	2257	rVB8	13854	31878	0.19%	0.021%
38	16.604	2277	2281	2285	rBV7	15542	20563	0.12%	0.014%
39	16.781	2308	2311	2316	rBV7	16124	21354	0.13%	0.014%
40	17.075	2356	2361	2366	rBV8	13985	22353	0.13%	0.015%
41	17.187	2375	2380	2388	rVB2	33464	54688	0.33%	0.036%
42	17.398	2409	2416	2426	rBV	6918474	9845361	59.16%	6.471%
43	17.498	2427	2433	2447	rVV	9991286	14755842	88.67%	9.698%
44	17.775	2477	2480	2488	rVB5	14889	25022	0.15%	0.016%
45	18.057	2525	2528	2533	rVB3	47866	59372	0.36%	0.039%
46	18.269	2559	2564	2573	rBV	276013	386155	2.32%	0.254%
47	19.304	2736	2740	2745	rVB	135545	173275	1.04%	0.114%
48	19.369	2747	2751	2756	rBV	130820	217721	1.31%	0.143%
49	19.498	2769	2773	2780	rBV2	134316	212100	1.27%	0.139%
50	19.645	2795	2798	2802	rVB3	57887	63594	0.38%	0.042%
51	19.728	2806	2812	2821	rBV	12513289	16641349	100.00%	10.938%
52	21.175	3054	3058	3066	rBV	536217	842880	5.06%	0.554%
53	21.486	3105	3111	3122	rBV	6774190	9204118	55.31%	6.050%
54	23.833	3502	3510	3525	rBV2	5748372	12321303	74.04%	8.098%
55	23.992	3530	3537	3550	rVB2	3632726	7702573	46.29%	5.063%




Sum of corrected areas: 152146199

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012868.D
Acq On : 30 Nov 2022 00:19
Operator : CG/JU
Sample : N5725-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

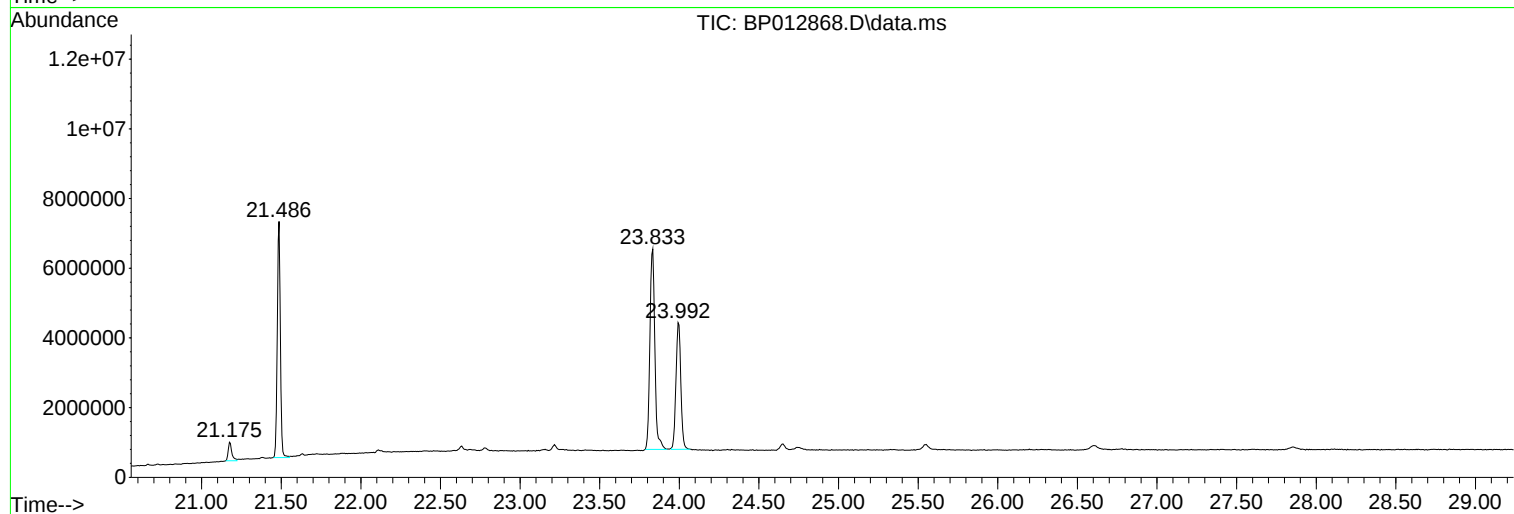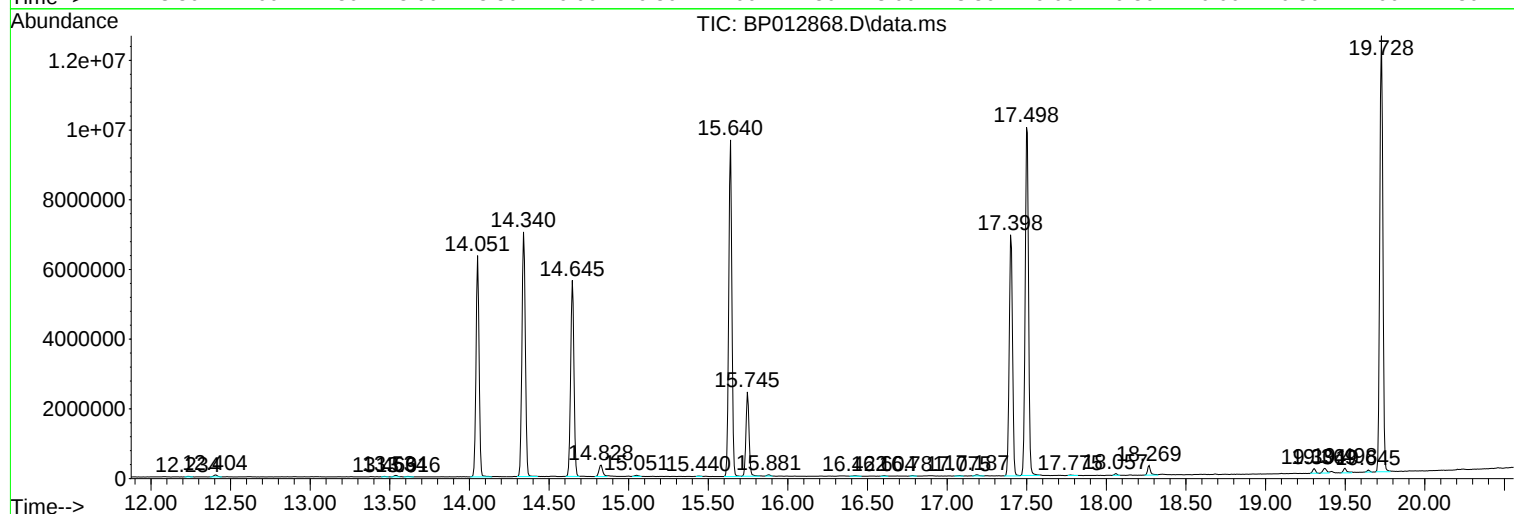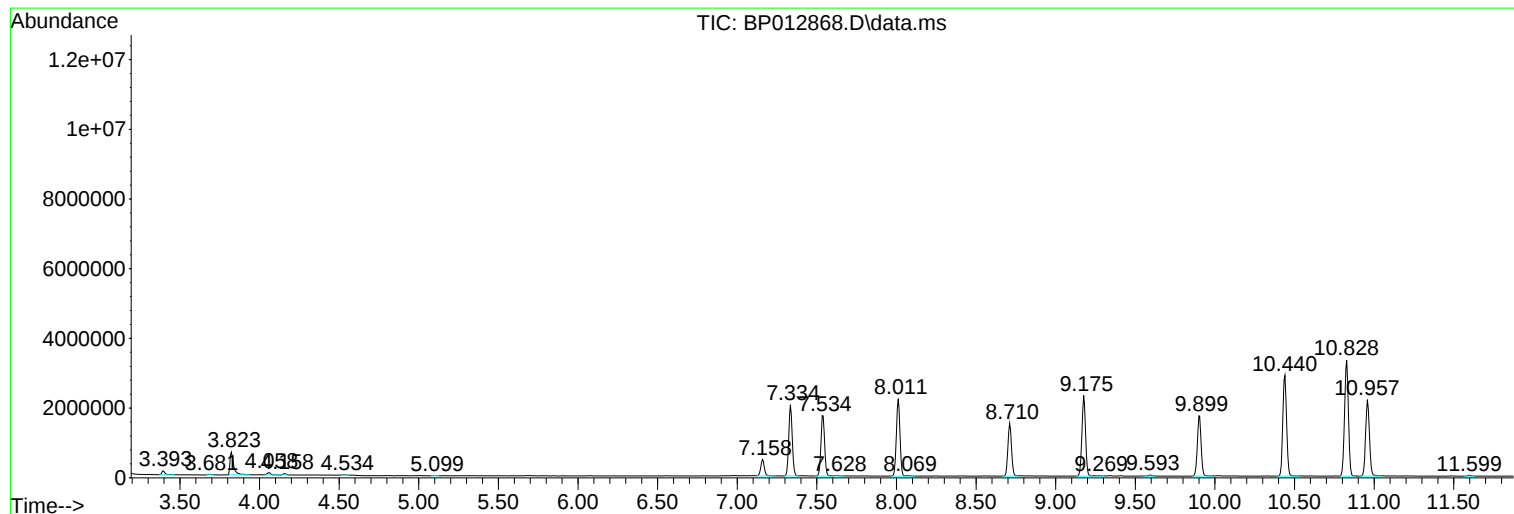

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012868.D
Acq On : 30 Nov 2022 00:19
Operator : CG/JU
Sample : N5725-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012868.D
Acq On : 30 Nov 2022 00:19
Operator : CG/JU
Sample : N5725-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc