

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012870.D
 Acq On : 30 Nov 2022 01:27
 Operator : CG/JU
 Sample : N5725-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	40	rBV	152512	209471	1.45%	0.138%
2	3.823	105	108	125	rBV	711347	1064187	7.38%	0.700%
3	4.058	144	148	156	rVB	73792	109715	0.76%	0.072%
4	4.158	161	165	173	rVB	50382	69383	0.48%	0.046%
5	6.969	637	643	644	rBV5	10494	15565	0.11%	0.010%
6	7.158	667	675	686	rVB	754018	1186572	8.23%	0.781%
7	7.334	697	705	714	rBV	2420963	3740273	25.93%	2.461%
8	7.540	732	740	749	rBV	2200003	3542669	24.56%	2.331%
9	7.611	749	752	763	rVB3	33196	72194	0.50%	0.048%
10	8.011	812	820	827	rBV	2591875	4012969	27.82%	2.641%
11	8.558	906	913	920	rBV	112734	178568	1.24%	0.117%
12	8.710	932	939	955	rBV	2105496	3370837	23.37%	2.218%
13	9.175	1011	1018	1026	rBV	2685241	4257304	29.52%	2.801%
14	9.593	1084	1089	1093	rVB2	30737	48295	0.33%	0.032%
15	9.899	1134	1141	1151	rBV	2031572	3358727	23.29%	2.210%
16	10.440	1225	1233	1250	rBV	3529165	5799862	40.21%	3.816%
17	10.610	1254	1262	1264	rBV8	8980	16815	0.12%	0.011%
18	10.828	1289	1299	1305	rBV	3753726	6349205	44.02%	4.178%
19	10.881	1305	1308	1312	rVV2	37554	52983	0.37%	0.035%
20	10.957	1314	1321	1336	rVV	1368485	2360903	16.37%	1.553%
21	11.075	1336	1341	1348	rVB9	11237	25799	0.18%	0.017%
22	11.593	1425	1429	1435	rBV4	20127	35373	0.25%	0.023%
23	12.404	1558	1567	1574	rBV	68876	125280	0.87%	0.082%
24	12.693	1612	1616	1621	rVB8	7927	15663	0.11%	0.010%
25	12.993	1661	1667	1669	rBV7	10711	18133	0.13%	0.012%
26	13.387	1728	1734	1737	rBV8	9942	20319	0.14%	0.013%
27	13.534	1755	1759	1764	rVB2	32492	50955	0.35%	0.034%
28	13.622	1766	1774	1779	rBV4	16318	39605	0.27%	0.026%
29	14.051	1840	1847	1864	rBV	6887954	9396048	65.15%	6.183%
30	14.340	1888	1896	1907	rBV	7970288	11393154	78.99%	7.497%
31	14.551	1926	1932	1933	rBV6	13769	24797	0.17%	0.016%
32	14.645	1941	1948	1955	rBV	6148952	8668995	60.10%	5.704%
33	14.710	1956	1959	1966	rVB4	25707	45466	0.32%	0.030%
34	14.822	1973	1978	1993	rBV	428135	737895	5.12%	0.486%
35	14.981	2002	2005	2011	rBV6	21007	42474	0.29%	0.028%
36	15.051	2012	2017	2022	rVB3	44394	77486	0.54%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
 Data File : BP012870.D
 Acq On : 30 Nov 2022 01:27
 Operator : CG/JU
 Sample : N5725-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.298	2055	2059	2063	rVB6	27955	40803	0.28%	0.027%
38	15.545	2097	2101	2109	rBV	32546	53637	0.37%	0.035%
39	15.640	2110	2117	2124	rBV	10083266	14409635	99.91%	9.482%
40	15.745	2129	2135	2143	rBV	2563136	3428150	23.77%	2.256%
41	15.881	2154	2158	2163	rVB2	42766	64459	0.45%	0.042%
42	16.898	2328	2331	2337	rVB5	45916	82593	0.57%	0.054%
43	17.187	2376	2380	2385	rVB4	32220	46467	0.32%	0.031%
44	17.398	2410	2416	2422	rBV	6248160	9087315	63.00%	5.980%
45	17.498	2427	2433	2447	rVB	10160781	14423236	100.00%	9.491%
46	18.269	2559	2564	2568	rBV	195772	273900	1.90%	0.180%
47	19.304	2736	2740	2746	rBV2	127600	165633	1.15%	0.109%
48	19.369	2747	2751	2756	rBV	116304	187652	1.30%	0.123%
49	19.439	2761	2763	2769	rVB2	66859	74709	0.52%	0.049%
50	19.498	2769	2773	2778	rBV2	145154	200382	1.39%	0.132%
51	19.645	2796	2798	2803	rVB3	56134	60043	0.42%	0.040%
52	19.728	2806	2812	2824	rBV	10819060	14043356	97.37%	9.241%
53	21.486	3105	3111	3119	rBV	4795640	6631529	45.98%	4.364%
54	23.827	3502	3509	3524	rBV2	5401255	11330543	78.56%	7.456%
55	23.992	3530	3537	3551	rVB2	3176067	6835775	47.39%	4.498%




Sum of corrected areas: 151973756

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012870.D
Acq On : 30 Nov 2022 01:27
Operator : CG/JU
Sample : N5725-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

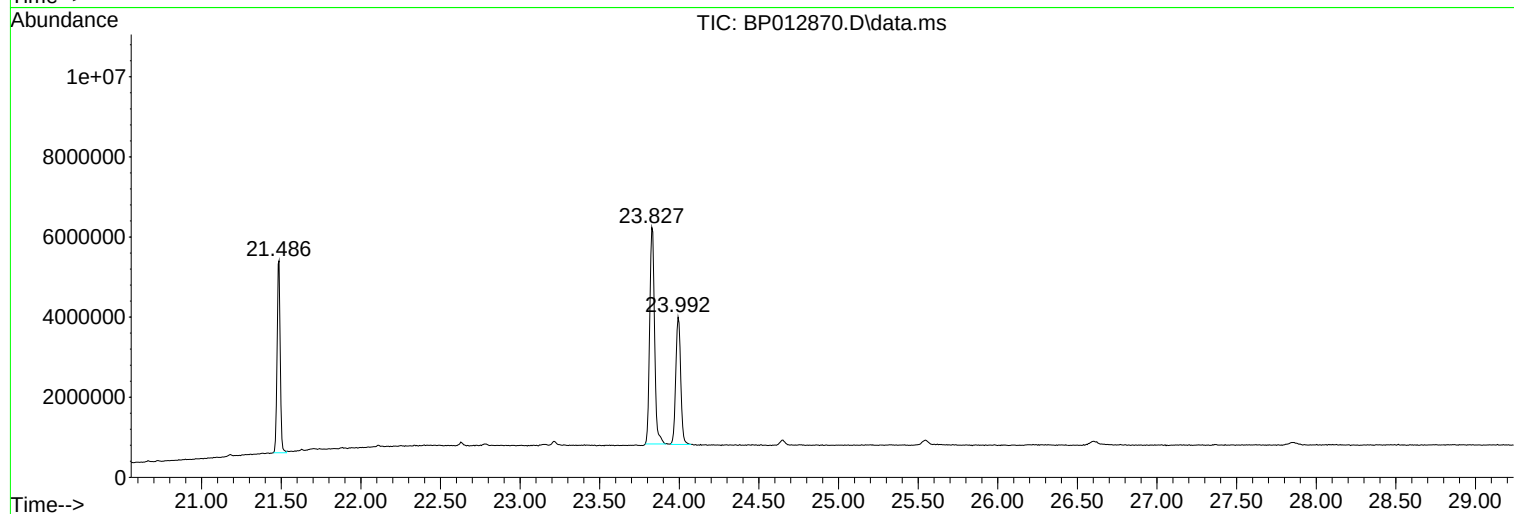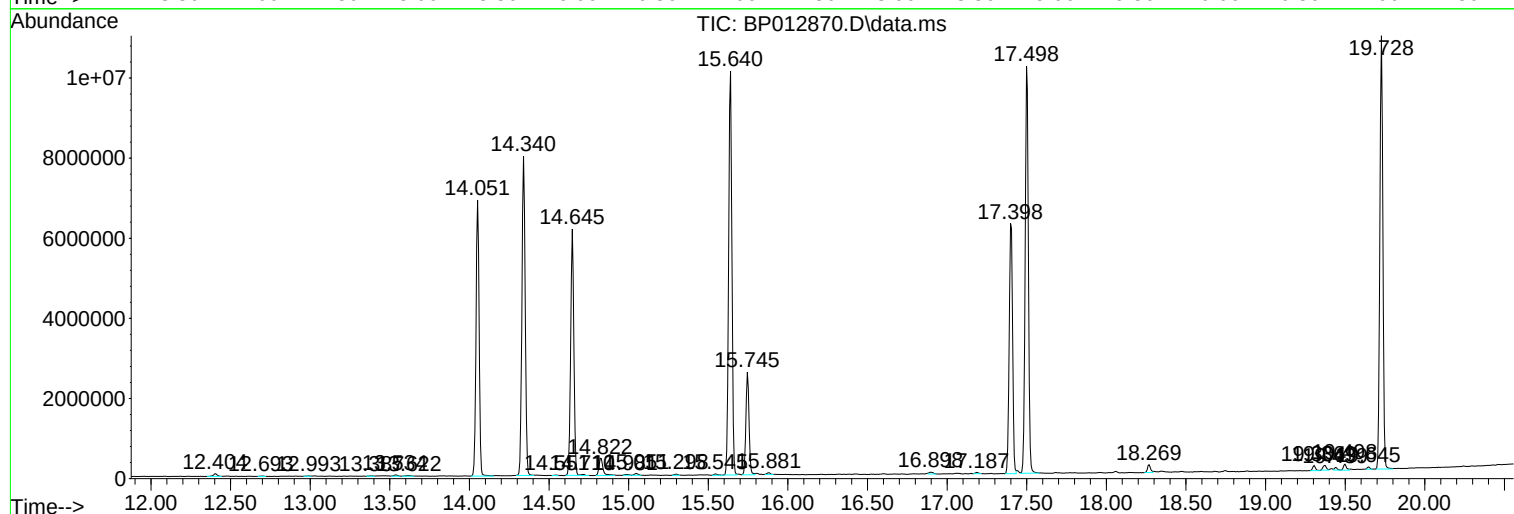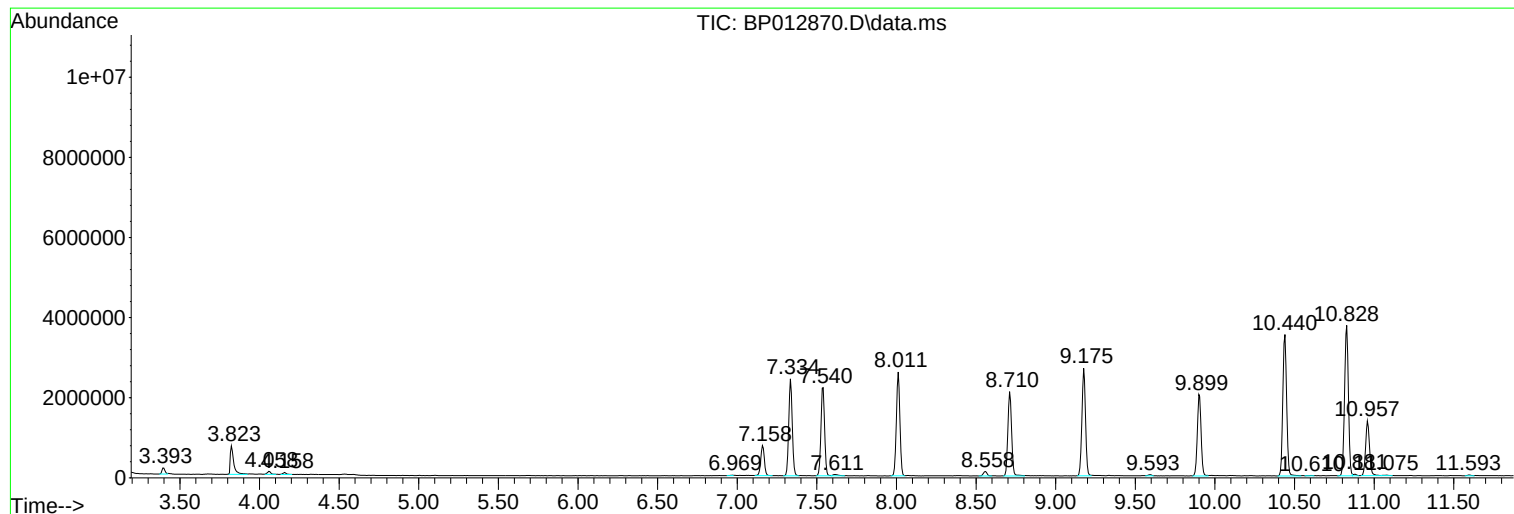

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012870.D
Acq On : 30 Nov 2022 01:27
Operator : CG/JU
Sample : N5725-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112922\
Data File : BP012870.D
Acq On : 30 Nov 2022 01:27
Operator : CG/JU
Sample : N5725-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc