

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018511.D
 Acq On : 02 Dec 2023 12:05
 Operator : MA/JU
 Sample : 05416-16
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH2

Quant Time: Dec 02 21:30:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 01 21:56:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	466907	20.000	ng/ul	0.00
20) Naphthalene-d8	10.657	136	2070107	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	1414508	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	2988791	20.000	ng/ul	0.00
79) Chrysene-d12	21.321	240	2063056	20.000	ng/ul	0.00
88) Perylene-d12	23.692	264	2021993	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	21078	1.538	ng/uL	0.00
4) Pyridine-d5	3.699	84	101398	2.763	ng/ul	0.00
7) Phenol-d5	7.028	99	554378	11.832	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	351517	12.658	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	416551	11.393	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	349698	9.222	ng/ul	-0.01
21) Nitrobenzene-d5	9.022	128	211389	11.473	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143	216995	11.360	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.281	165	435066	11.139	ng/ul	0.00
31) 4-Chloroaniline-d4	10.798	131	522477	10.235	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	1569132	12.429	ng/ul	0.00
49) Acenaphthylene-d8	14.181	160	1675052	12.050	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.686	143	194572	9.389	ng/ul	0.00
60) Fluorene-d10	15.481	176	1333537	12.584	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	139464	7.782	ng/ul	-0.01
73) Anthracene-d10	17.333	188	1991194	12.673	ng/ul	0.00
81) Pyrene-d10	19.569	212	2261532	14.082	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	1540251	13.064	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.687	105	186416	3.299	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018511.D
Acq On : 02 Dec 2023 12:05
Operator : MA/JU
Sample : 05416-16
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COAH2

Quant Time: Dec 02 21:30:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 01 21:56:43 2023
Response via : Initial Calibration

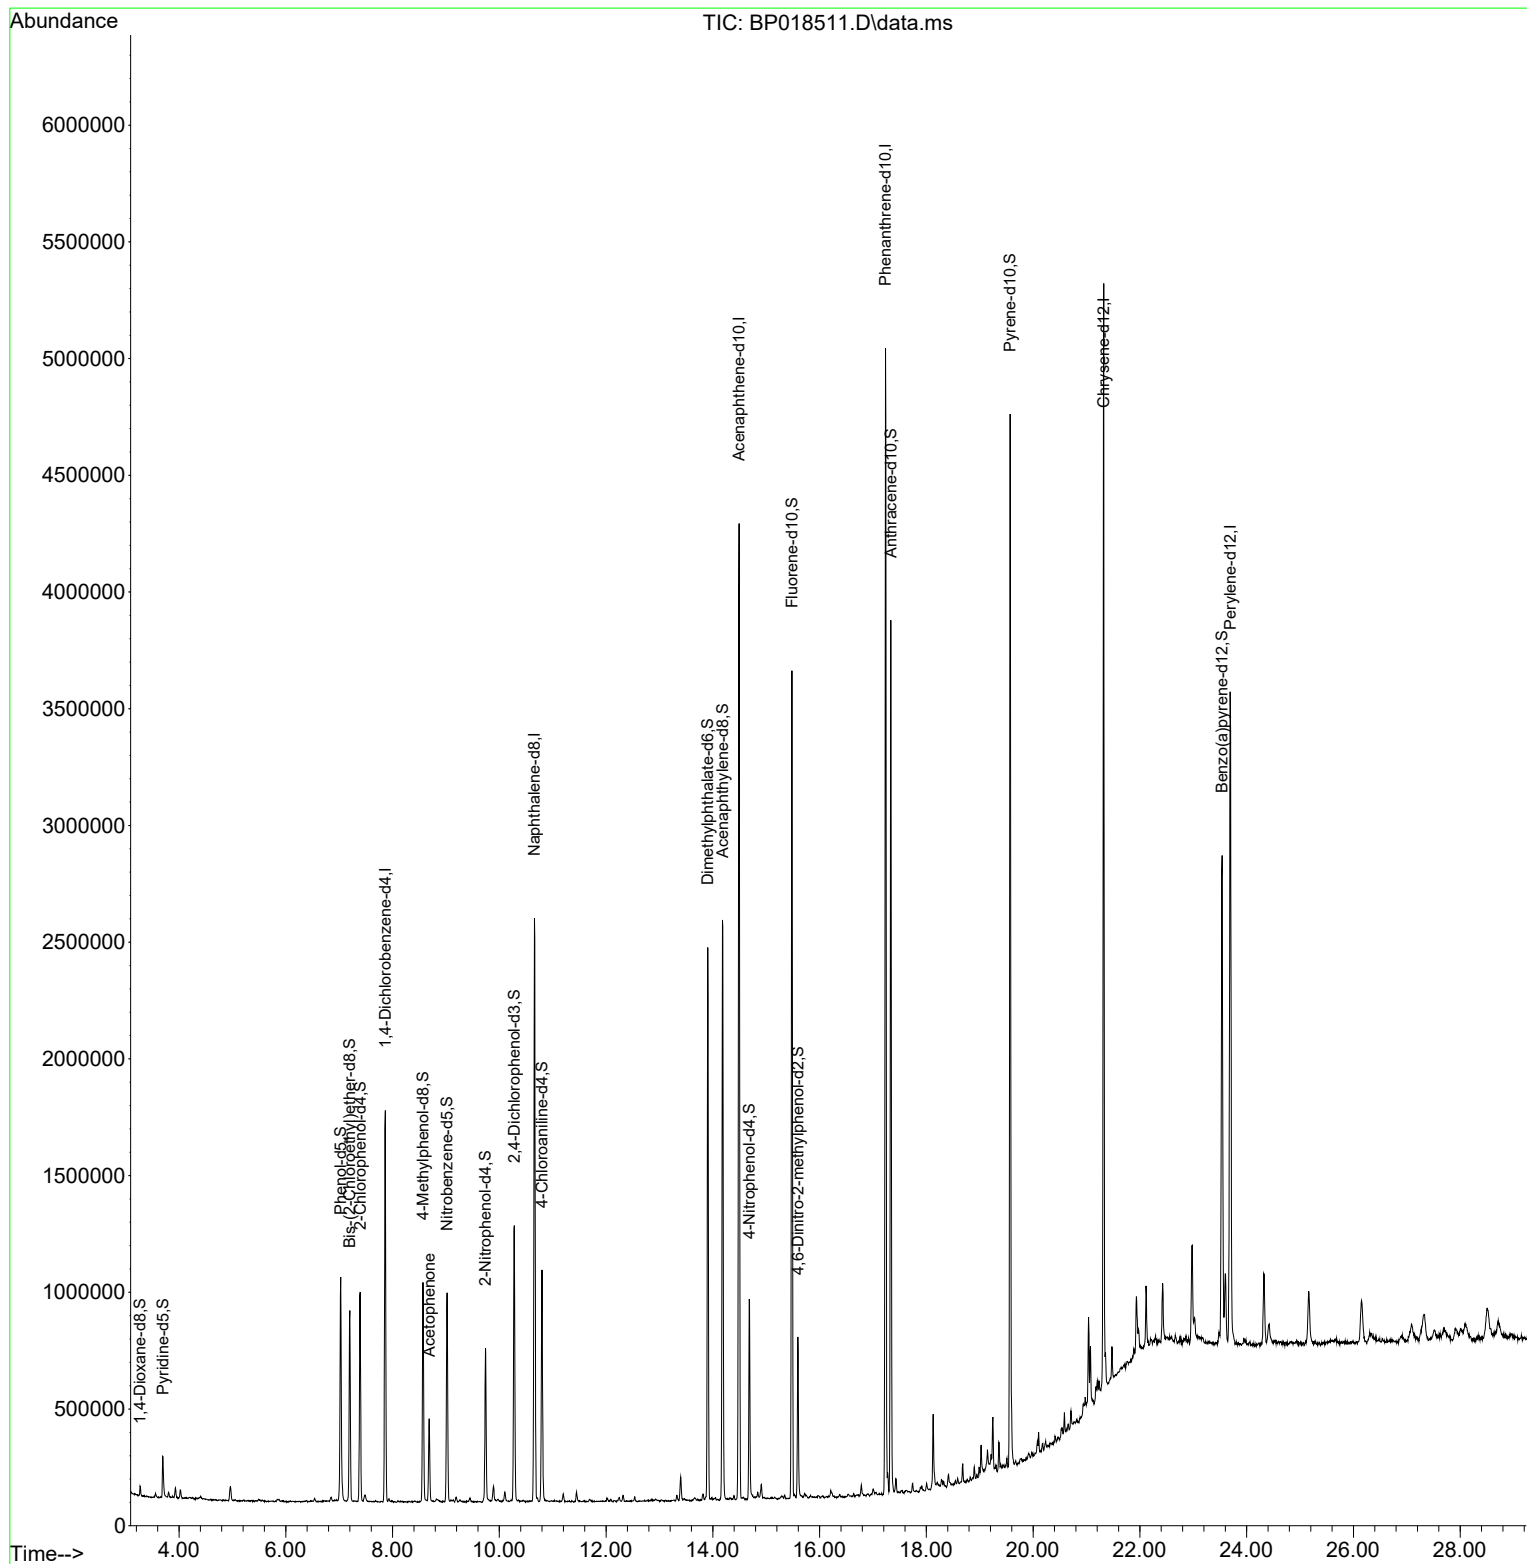

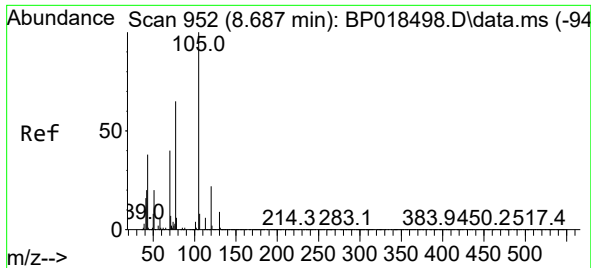

#16
 Acetophenone
 Concen: 3.299 ng/ul
 RT: 8.687 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP018511.D
 Acq: 02 Dec 2023 12:05

Instrument :
 BNA_P
 ClientSampleId :
 C0AH2

Tgt Ion:105 Resp: 186416
 Ion Ratio Lower Upper
 105 100
 77 77.4 59.4 89.0
 51 25.0 19.4 29.0

