

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018512.D
 Acq On : 02 Dec 2023 12:39
 Operator : MA/JU
 Sample : 05416-19
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ9

Quant Time: Dec 02 21:30:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 01 21:56:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	433097	20.000	ng/ul	0.00
20) Naphthalene-d8	10.657	136	1810300	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.487	164	1101788	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.234	188	2189771	20.000	ng/ul	0.00
79) Chrysene-d12	21.322	240	2039848	20.000	ng/ul	0.00
88) Perylene-d12	23.692	264	2418012	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	16216	1.276	ng/uL	0.00
4) Pyridine-d5	3.699	84	81651	2.398	ng/ul	0.00
7) Phenol-d5	7.028	99	434097	9.988	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	274903	10.672	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	327127	9.646	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	271136	7.708	ng/ul	-0.01
21) Nitrobenzene-d5	9.022	128	155003	9.620	ng/ul	0.00
24) 2-Nitrophenol-d4	9.746	143	151923	9.095	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	315842	9.247	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.799	131	346904	7.771	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	984566	10.012	ng/ul	0.00
49) Acenaphthylene-d8	14.181	160	1091149	10.077	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.681	143	108768	6.738	ng/ul	-0.01
60) Fluorene-d10	15.481	176	851049	10.310	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	69191	5.270	ng/ul	-0.01
73) Anthracene-d10	17.334	188	1191474	10.350	ng/ul	0.00
81) Pyrene-d10	19.569	212	1492320	9.398	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	1527101	10.831	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.687	105	168936	3.223	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018512.D
Acq On : 02 Dec 2023 12:39
Operator : MA/JU
Sample : 05416-19
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ9

Quant Time: Dec 02 21:30:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 01 21:56:43 2023
Response via : Initial Calibration

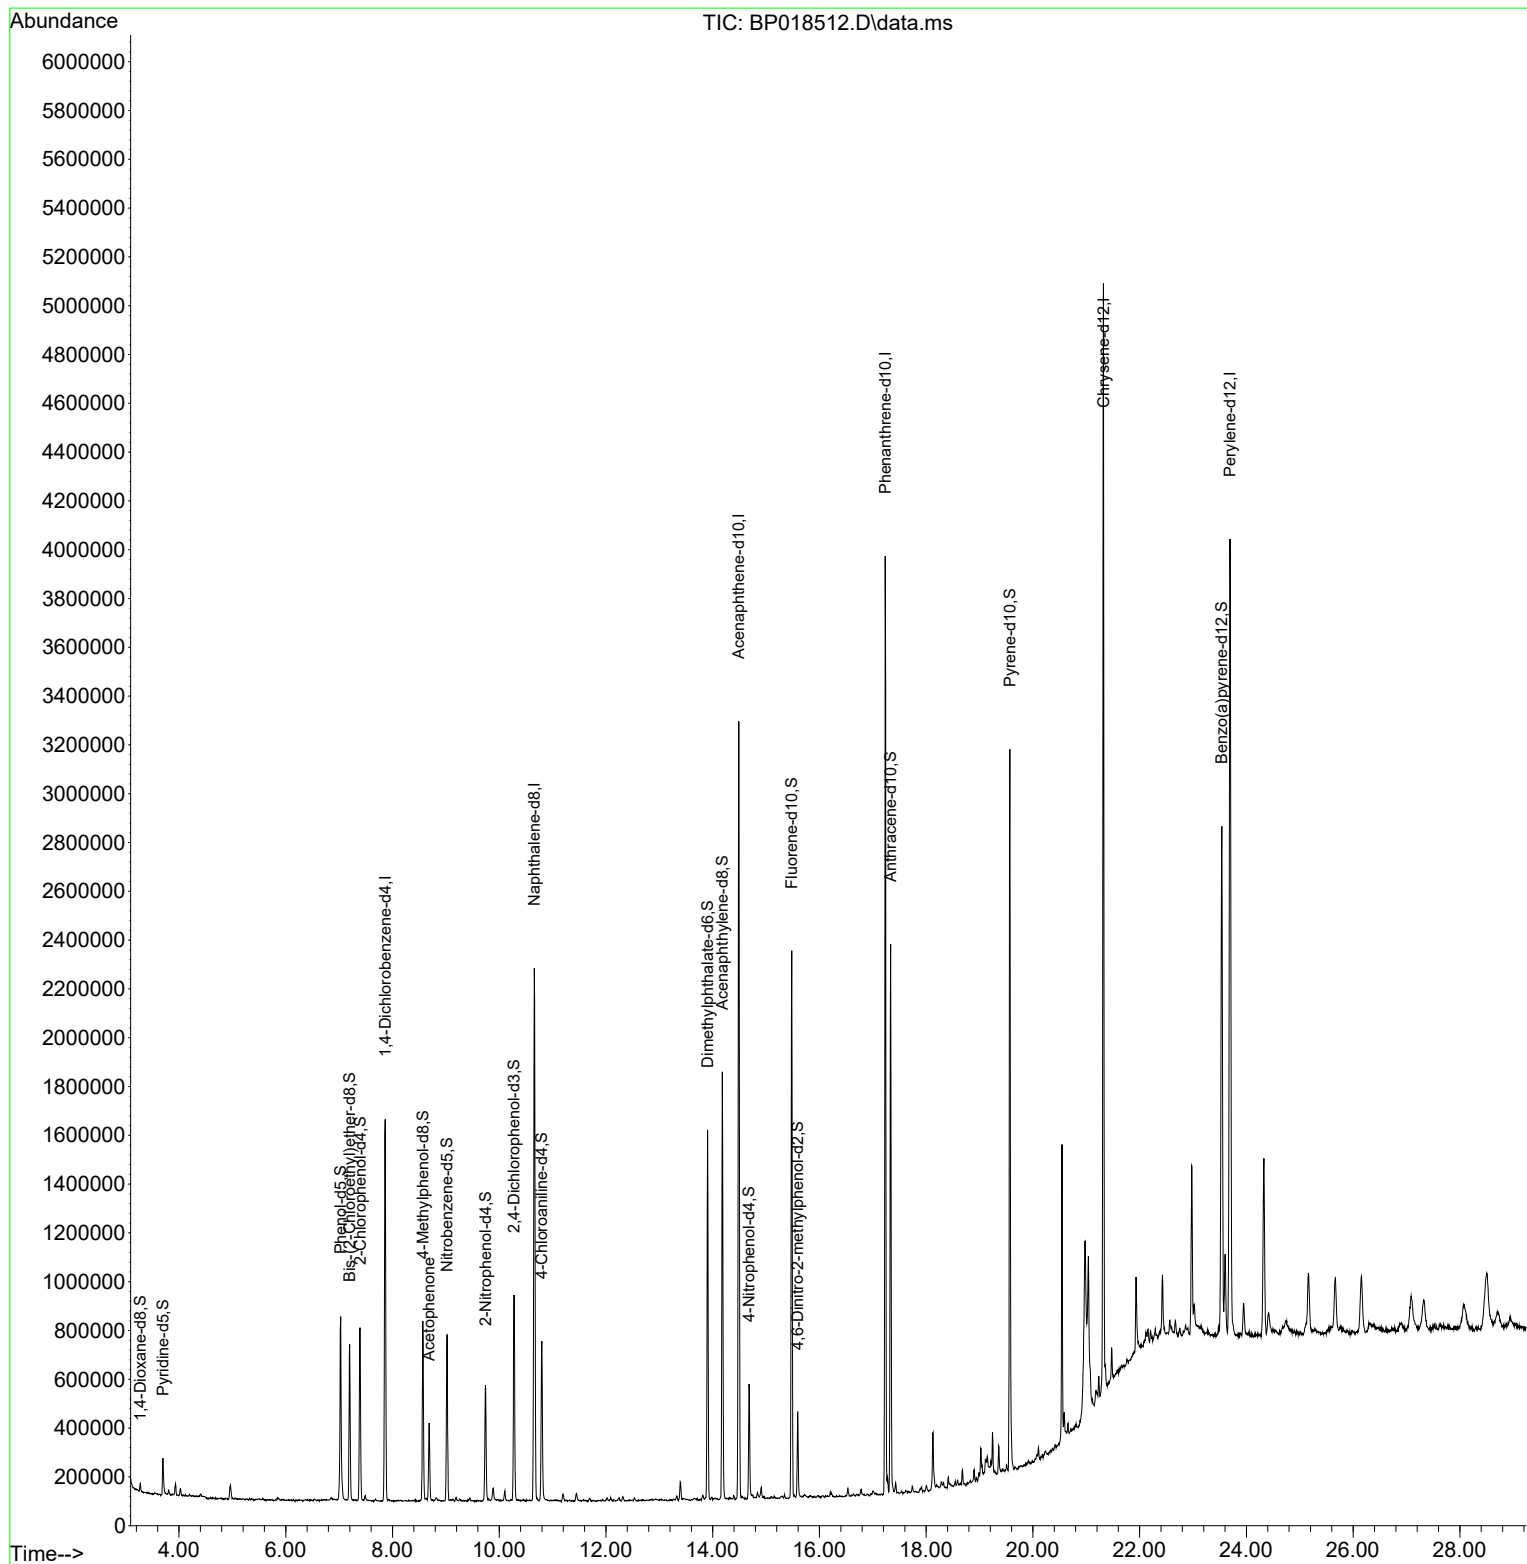

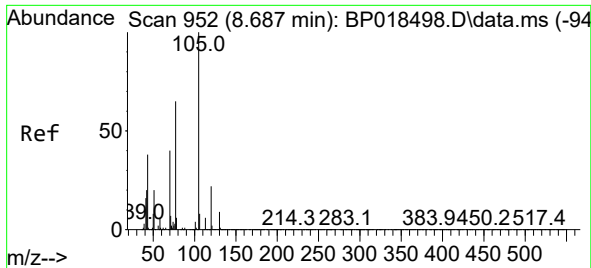

#16
 Acetophenone
 Concen: 3.223 ng/ul
 RT: 8.687 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP018512.D
 Acq: 02 Dec 2023 12:39

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ9

Tgt Ion:105 Resp: 168936
 Ion Ratio Lower Upper
 105 100
 77 76.4 59.4 89.0
 51 24.0 19.4 29.0

