

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018519.D
 Acq On : 02 Dec 2023 17:10
 Operator : MA/JU
 Sample : 05416-22
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH5

Quant Time: Dec 02 21:32:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 01 21:56:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.864	152	357783	20.000	ng/ul	0.00
20) Naphthalene-d8	10.657	136	1610797	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.487	164	1123564	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.234	188	2624330	20.000	ng/ul	0.00
79) Chrysene-d12	21.316	240	2368964	20.000	ng/ul	-0.01
88) Perylene-d12	23.692	264	2245008	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	16444	1.566	ng/uL	0.00
4) Pyridine-d5	3.699	84	67196	2.389	ng/ul	0.00
7) Phenol-d5	7.028	99	408544	11.379	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	270482	12.710	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	305508	10.905	ng/ul	-0.01
15) 4-Methylphenol-d8	8.569	113	276086	9.501	ng/ul	-0.01
21) Nitrobenzene-d5	9.022	128	155093	10.818	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143	128738	8.661	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.275	165	310052	10.201	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.799	131	414718	10.441	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	1212104	12.087	ng/ul	0.00
49) Acenaphthylene-d8	14.181	160	1289802	11.681	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.681	143	89504	5.438	ng/ul	-0.01
60) Fluorene-d10	15.481	176	1073632	12.755	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.593	200	47997	3.050	ng/ul	-0.01
73) Anthracene-d10	17.334	188	1703062	12.344	ng/ul	0.00
81) Pyrene-d10	19.569	212	2256037	12.234	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.533	264	1765991	13.491	ng/ul	-0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.687	105	173341	4.003	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018519.D
Acq On : 02 Dec 2023 17:10
Operator : MA/JU
Sample : 05416-22
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH5

Quant Time: Dec 02 21:32:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 01 21:56:43 2023
Response via : Initial Calibration

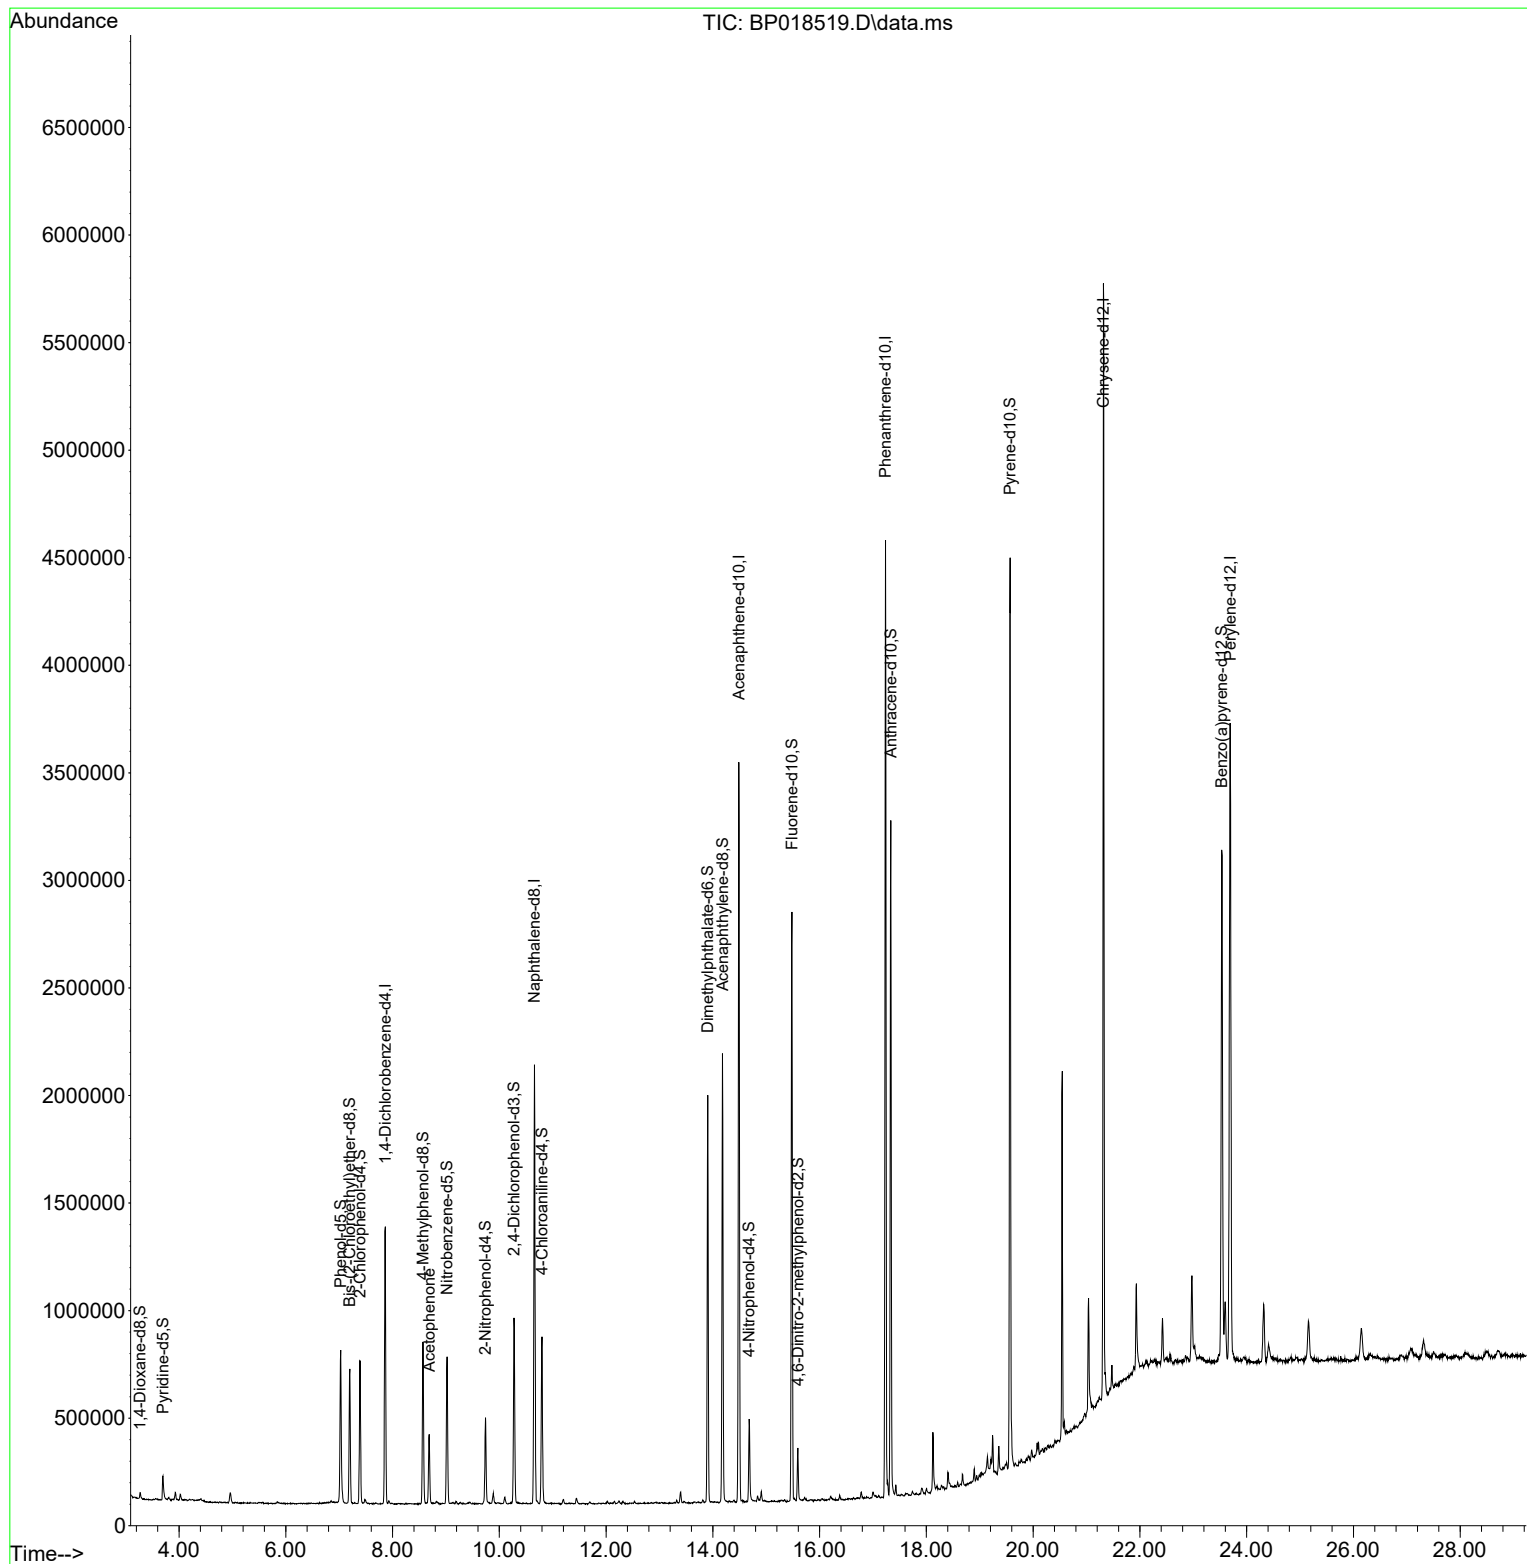

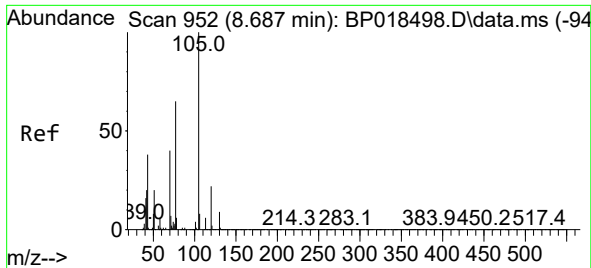

#16
 Acetophenone
 Concen: 4.003 ng/ul
 RT: 8.687 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP018519.D
 Acq: 02 Dec 2023 17:10

Instrument :
 BNA_P
 ClientSampleId :
 C0AH5

Tgt Ion:105 Resp: 173341
 Ion Ratio Lower Upper
 105 100
 77 75.7 59.4 89.0
 51 24.9 19.4 29.0

