

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018539.D
 Acq On : 03 Dec 2023 05:04
 Operator : MA/JU
 Sample : 05411-17
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK2

Quant Time: Dec 03 23:39:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 01 21:56:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	420358	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.657	136	1858105	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.487	164	1185175	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.234	188	2378859	20.000	ng/ul	0.00
79) Chrysene-d12	21.316	240	1578757	20.000	ng/ul	-0.01
88) Perylene-d12	23.692	264	1713428	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	43128	3.496	ng/uL	0.00
4) Pyridine-d5	3.693	84	166168	5.029	ng/ul	0.00
7) Phenol-d5	7.193	99	664971	15.763	ng/ul	0.16
9) Bis-(2-Chloroethyl)eth...	7.193	67	706099	28.241	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.387	132	549730	16.701	ng/ul	-0.01
15) 4-Methylphenol-d8	8.569	113	63323	1.855	ng/ul	-0.01
21) Nitrobenzene-d5	9.022	128	445332	26.928	ng/ul	0.00
24) 2-Nitrophenol-d4	9.740	143	389520	22.718	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.275	165	984865	28.091	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.810	131	9621	0.210	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	3156370	29.840	ng/ul	0.00
49) Acenaphthylene-d8	14.181	160	21329	0.183	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.681	143	56386	3.247	ng/ul	-0.01
60) Fluorene-d10	15.481	176	2418468	27.238	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	322369	22.601	ng/ul	-0.01
73) Anthracene-d10	17.234	188	2378859	19.022	ng/ul	-0.11
81) Pyrene-d10	19.563	212	113806	0.926	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.527	264	4790	0.048	ng/ul	-0.02
Target Compounds						
10) Bis(2-Chloroethyl)ether	7.269	93	1222172	35.973	ng/ul#	Qvalue 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018539.D
Acq On : 03 Dec 2023 05:04
Operator : MA/JU
Sample : 05411-17
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK2

Quant Time: Dec 03 23:39:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 01 21:56:43 2023
Response via : Initial Calibration

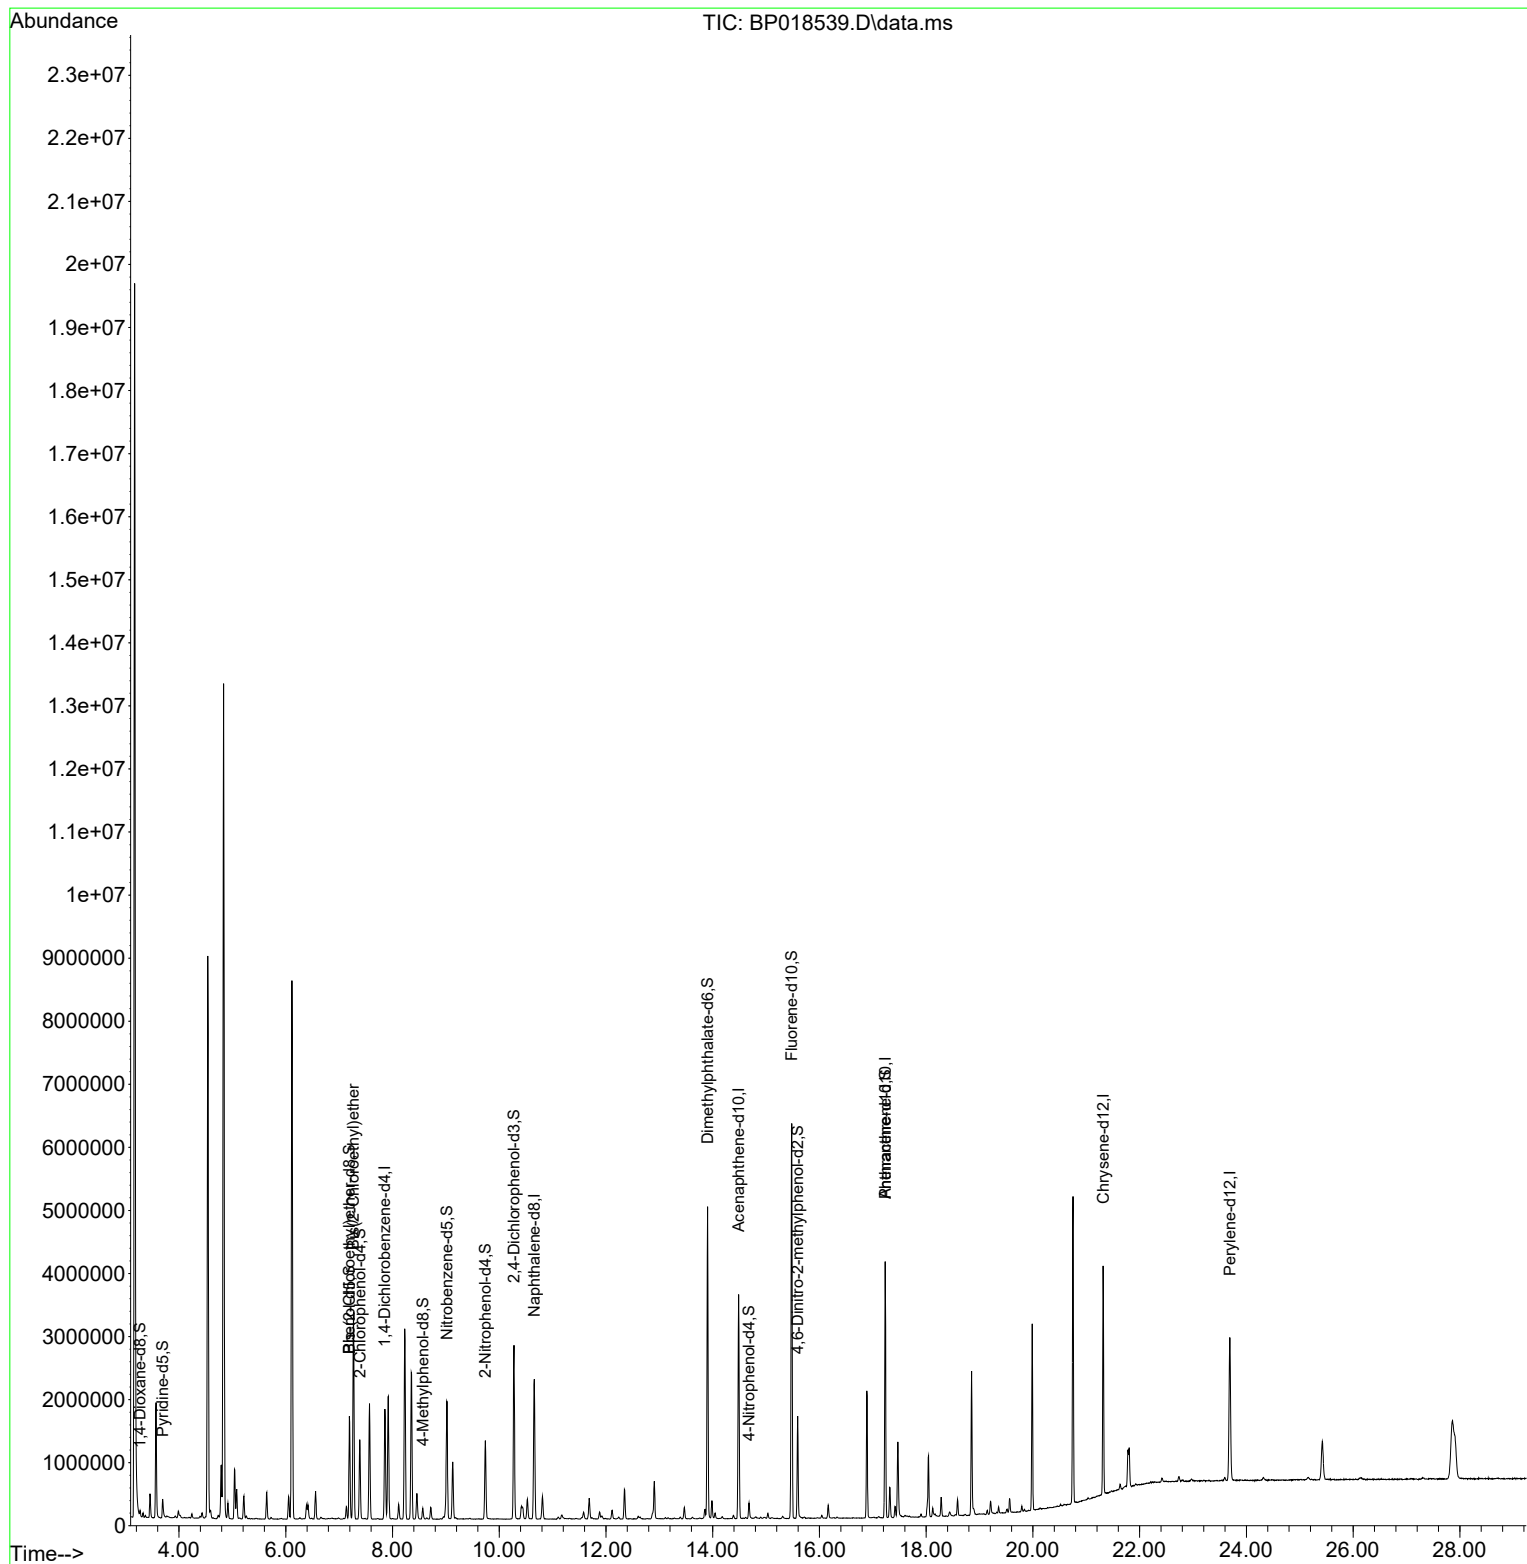

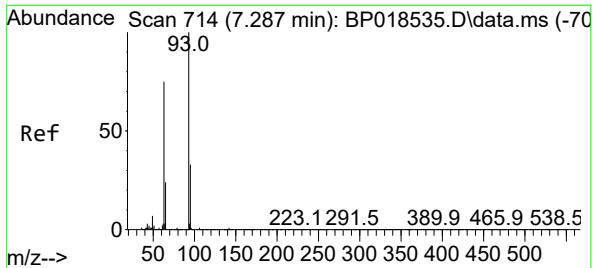

#10
 Bis(2-Chloroethyl)ether
 Concen: 35.973 ng/ul
 RT: 7.269 min Scan# 711
 Delta R.T. -0.029 min
 Lab File: BP018539.D
 Acq: 03 Dec 2023 05:04

Instrument :
 BNA_P
 ClientSampleId :
 C0QK2

Tgt Ion: 93 Resp: 1222172

Ion	Ratio	Lower	Upper
93	100		
63	5.8	58.3	87.5#
95	32.4	25.9	38.9

