

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018552.D
 Acq On : 03 Dec 2023 12:59
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020705

Quant Time: Dec 03 23:43:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 01 21:56:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	403025	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.657	136	1797483	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.487	164	1156087	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.234	188	2356729	20.000	ng/ul	0.00
79) Chrysene-d12	21.322	240	1555694	20.000	ng/ul	0.00
88) Perylene-d12	23.692	264	1620011	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.270	96	90414	7.645	ng/uL	0.00
4) Pyridine-d5	3.687	84	667340	21.066	ng/ul	0.00
7) Phenol-d5	7.022	99	834687	20.638	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.193	67	512655	21.386	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.387	132	623835	19.767	ng/ul	-0.01
15) 4-Methylphenol-d8	8.569	113	678901	20.742	ng/ul	-0.01
21) Nitrobenzene-d5	9.016	128	320839	20.055	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.740	143	326257	19.670	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.275	165	681147	20.084	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.793	131	950976	21.455	ng/ul	-0.01
46) Dimethylphthalate-d6	13.904	166	2049481	19.863	ng/ul	0.00
49) Acenaphthylene-d8	14.181	160	2322594	20.442	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.687	143	326591	19.283	ng/ul	0.00
60) Fluorene-d10	15.481	176	1725711	19.925	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	263883	18.674	ng/ul	0.00
73) Anthracene-d10	17.334	188	2501262	20.188	ng/ul	0.00
81) Pyrene-d10	19.569	212	2533895	20.924	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	1877012	19.871	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.305	88	98586	7.601	ng/uL	98
5) Pyridine	3.705	79	675167	21.105	ng/ul	99
6) Benzaldehyde	6.999	77	494988	23.704	ng/ul	97
8) Phenol	7.052	94	833189	21.007	ng/ul	98
10) Bis(2-Chloroethyl)ether	7.287	93	698673	21.449	ng/ul	99
12) 2-Chlorophenol	7.416	128	634729	19.872	ng/ul	99
13) 2-Methylphenol	8.305	108	635719	20.936	ng/ul	100
14) 2,2'-oxybis(1-Chloropr...	8.387	45	883205	21.369	ng/ul	98
16) Acetophenone	8.681	105	1076294	22.064	ng/ul	98
17) N-Nitroso-di-n-propyla...	8.675	70	538896	20.082	ng/ul	99
18) 4-Methylphenol	8.634	108	698211	21.057	ng/ul	100
19) Hexachloroethane	8.934	117	258797	19.764	ng/ul	99
22) Nitrobenzene	9.063	77	782465	20.116	ng/ul	97
23) Isophorone	9.593	82	1560192	19.673	ng/ul	99
25) 2-Nitrophenol	9.769	139	363378	20.462	ng/ul	99
26) 2,4-Dimethylphenol	9.834	107	686896	19.777	ng/ul	99
27) Bis(2-Chloroethoxy)met...	10.075	93	996352	19.900	ng/ul	99
29) 2,4-Dichlorophenol	10.305	162	656356	20.092	ng/ul	97
30) Naphthalene	10.704	128	2183026	20.020	ng/ul	100
32) 4-Chloroaniline	10.816	127	921953	21.824	ng/ul	100
33) Hexachlorobutadiene	10.993	225	434741	19.871	ng/ul	97
34) Caprolactam	11.593	113	185542	18.523	ng/ul	97
35) 4-Chloro-3-methylphenol	11.940	107	707743	19.339	ng/ul	99
36) 2-Methylnaphthalene	12.316	142	1534496	19.864	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018552.D
 Acq On : 03 Dec 2023 12:59
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020705

Quant Time: Dec 03 23:43:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 01 21:56:43 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.534	142	1551235	19.884	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.681	216	867366	20.679	ng/ul	99
40) Hexachlorocyclopentadiene	12.663	237	469779	18.896	ng/ul	100
41) 2,4,6-Trichlorophenol	12.922	196	545101	20.202	ng/ul	100
42) 2,4,5-Trichlorophenol	12.993	196	590558	20.188	ng/ul	100
43) 1,1'-Biphenyl	13.328	154	2054592	20.549	ng/ul	98
44) 2-Chloronaphthalene	13.363	162	1625490	20.584	ng/ul	99
45) 2-Nitroaniline	13.569	65	430145	20.093	ng/ul	97
47) Dimethylphthalate	13.951	163	2034311	20.029	ng/ul	99
48) 2,6-Dinitrotoluene	14.069	165	392389	20.448	ng/ul	94
50) Acenaphthylene	14.210	152	2621213	20.520	ng/ul	100
51) 3-Nitroaniline	14.393	138	397475	20.750	ng/ul	97
52) Acenaphthene	14.551	153	1717660	20.337	ng/ul	99
53) 2,4-Dinitrophenol	14.598	184	168751	16.593	ng/ul	99
55) 4-Nitrophenol	14.698	109	255839	19.994	ng/ul	99
56) Dibenzofuran	14.887	168	2373587	20.220	ng/ul	98
57) 2,4-Dinitrotoluene	14.851	165	545528	20.210	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.110	232	478851	19.515	ng/ul	97
59) Diethylphthalate	15.316	149	1932169	19.441	ng/ul	99
61) Fluorene	15.534	166	1890206	20.350	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.534	204	997182	20.469	ng/ul	95
63) 4-Nitroaniline	15.557	138	380555	20.854	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.610	198	284550	18.834	ng/ul	98
67) N-Nitrosodiphenylamine	15.745	169	1599733	20.485	ng/ul	99
68) 4-Bromophenyl-phenylether	16.428	248	590718	19.854	ng/ul	96
69) Hexachlorobenzene	16.534	284	676574	20.367	ng/ul	99
70) Atrazine	16.704	200	504623	21.734	ng/ul	97
71) Pentachlorophenol	16.881	266	365546	18.503	ng/ul	99
72) Phenanthrene	17.275	178	2878387	20.223	ng/ul	100
74) Anthracene	17.369	178	2921832	20.479	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.287	216	874695	21.465	ng/ul	99
76) Pentachlorobenzene	14.804	250	838749	20.954	ng/ul	99
77) Carbazole	17.639	167	2439694	21.455	ng/ul	99
78) Di-n-butylphthalate	18.198	149	2953692	19.508	ng/ul	100
80) Fluoranthene	19.245	202	2995102	20.924	ng/ul	99
82) Pyrene	19.598	202	3025339	20.950	ng/ul	98
83) Butylbenzylphthalate	20.475	149	983687	18.607	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.239	252	744931	19.705	ng/ul	99
85) Benzo(a)anthracene	21.304	228	2513937	19.909	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.239	149	1309048	18.016	ng/ul	99
87) Chrysene	21.357	228	2313225	19.893	ng/ul	100
89) Di-n-octyl phthalate	22.151	149	1934742	16.357	ng/ul	100
90) Benzo(b)fluoranthene	22.969	252	2307441	19.318	ng/ul	99
91) Benzo(k)fluoranthene	23.016	252	2242142	19.401	ng/ul	100
93) Benzo(a)pyrene	23.586	252	2202046	20.176	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.157	276	2810548	21.553	ng/ul	98
95) Dibenzo(a,h)anthracene	26.180	278	2343968	21.608	ng/ul	99
96) Benzo(g,h,i)perylene	26.921	276	2272782	21.657	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018552.D
 Acq On : 03 Dec 2023 12:59
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020705

Quant Time: Dec 03 23:43:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 01 21:56:43 2023
 Response via : Initial Calibration




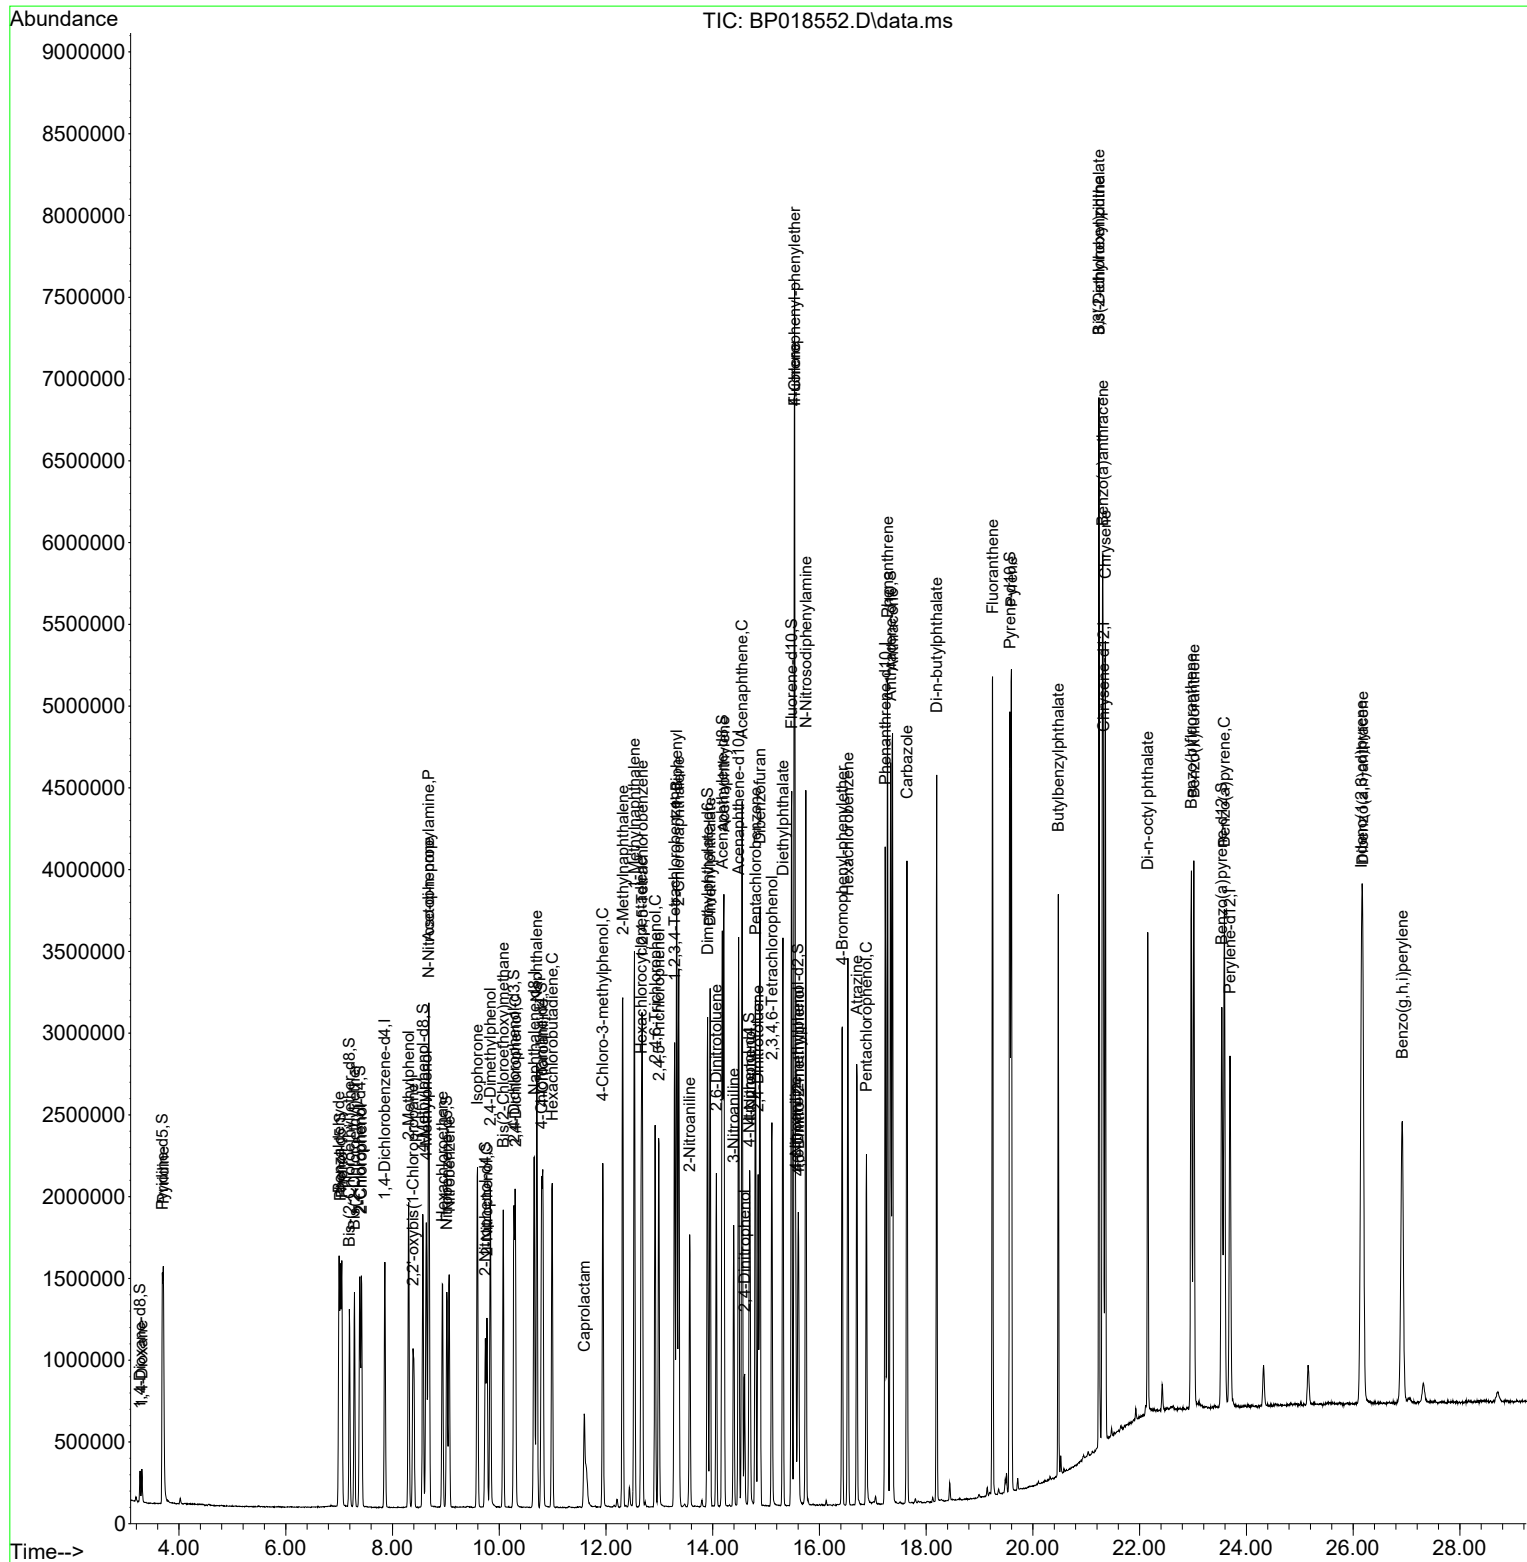


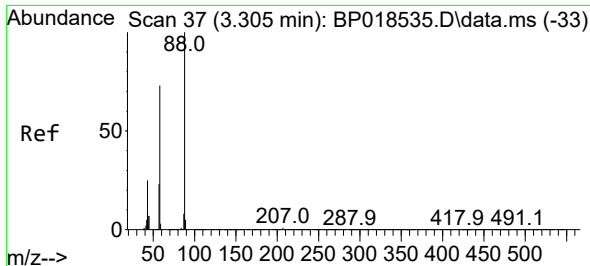

#2
1,4-Dioxane
Concen: 7.601 ng/uL
RT: 3.305 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:	88	Resp:	98586
Ion	Ratio	Lower	Upper
88	100		
43	24.9	21.8	32.6
58	70.0	56.5	84.7

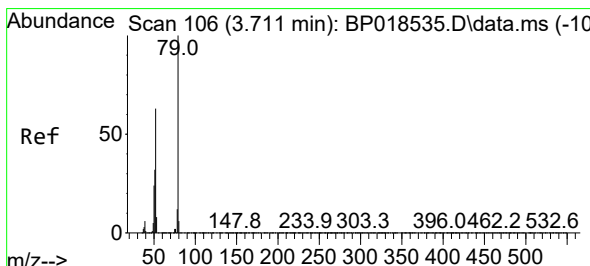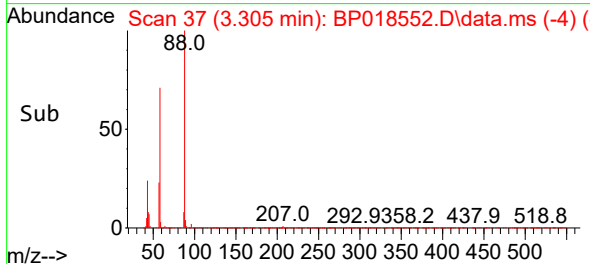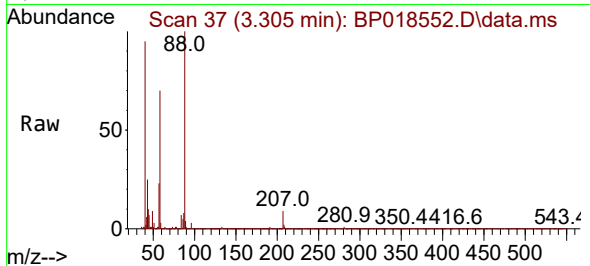

#5
Pyridine
Concen: 21.105 ng/uL
RT: 3.705 min Scan# 105
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:	79	Resp:	675167
Ion	Ratio	Lower	Upper
79	100		
52	71.1	57.4	86.0
51	32.8	26.2	39.4


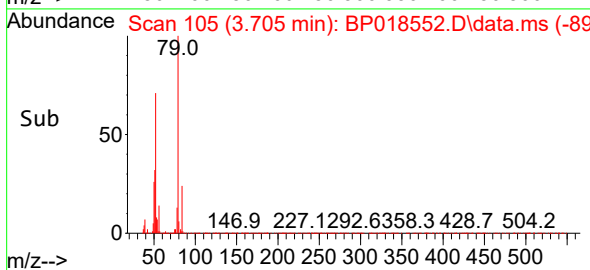

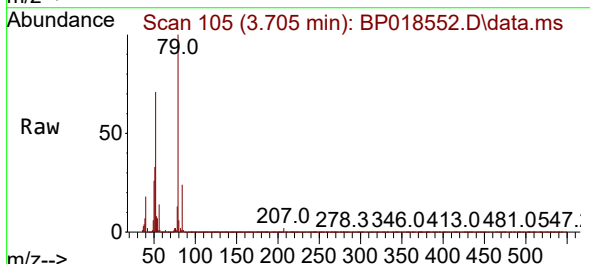




#6
Benzaldehyde
Concen: 23.704 ng/ul
RT: 6.999 min Scan# 601
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion: 77 Resp: 494988
Ion Ratio Lower Upper
77 100
105 101.7 77.9 116.9
106 94.5 74.6 111.8



#8
Phenol
Concen: 21.007 ng/ul
RT: 7.052 min Scan# 674
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion: 94 Resp: 833189
Ion Ratio Lower Upper
94 100
65 25.9 21.0 31.6
66 34.6 28.6 43.0









#10
Bis(2-Chloroethyl)ether
Concen: 21.449 ng/ul
RT: 7.287 min Scan# 714
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion: 93 Resp: 698673
Ion Ratio Lower Upper
93 100
63 73.5 58.3 87.5
95 32.5 25.9 38.9



#12
2-Chlorophenol
Concen: 19.872 ng/ul
RT: 7.416 min Scan# 736
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:128 Resp: 634729
Ion Ratio Lower Upper
128 100
64 46.3 37.0 55.4
130 32.0 26.8 40.2





#13

2-Methylphenol

Concen: 20.936 ng/ul

RT: 8.305 min Scan# 887

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :





SSTD020705

Tgt Ion:108 Resp: 635719

Ion Ratio Lower Upper

108 100

107 87.9 70.6 105.8

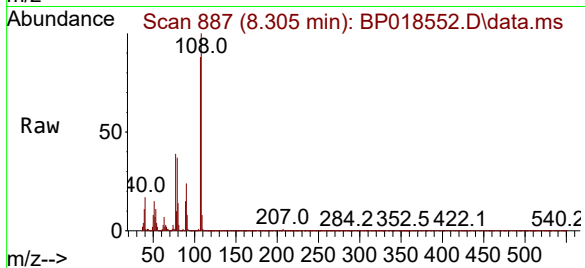

#14

2,2'-oxybis(1-Chloropropane)

Concen: 21.369 ng/ul

RT: 8.387 min Scan# 901

Delta R.T. -0.018 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion: 45 Resp: 883205


Ion Ratio Lower Upper

45 100

77 16.3 12.7 19.1

79 12.2 10.5 15.7




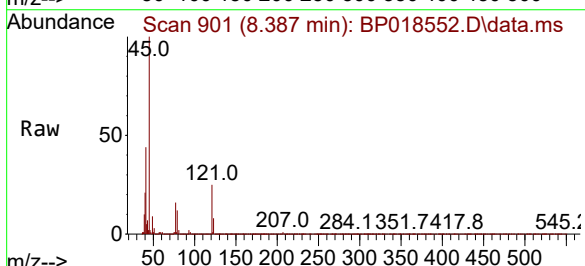




#16
Acetophenone
Concen: 22.064 ng/ul
RT: 8.681 min Scan# 91
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:105 Resp: 1076294
Ion Ratio Lower Upper
105 100
77 75.9 59.4 89.0
51 24.1 19.4 29.0



#17
N-Nitroso-di-n-propylamine
Concen: 20.082 ng/ul
RT: 8.675 min Scan# 950
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion: 70 Resp: 538896
Ion Ratio Lower Upper
70 100
42 50.4 41.0 61.4
101 10.5 7.8 11.8
130 21.1 16.9 25.3



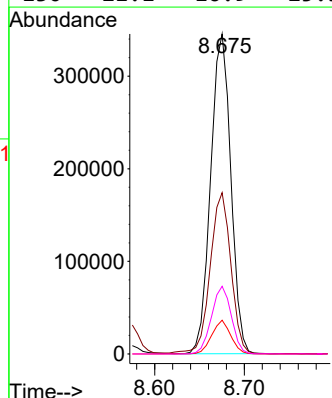





#18
4-Methylphenol
Concen: 21.057 ng/ul
RT: 8.634 min Scan# 943
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:108 Resp: 698211
Ion Ratio Lower Upper
108 100
107 113.0 90.6 136.0



#19
Hexachloroethane
Concen: 19.764 ng/ul
RT: 8.934 min Scan# 994
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:117 Resp: 258797
Ion Ratio Lower Upper
117 100
201 104.4 83.7 125.5
199 64.5 52.3 78.5









#22
Nitrobenzene
Concen: 20.116 ng/ul
RT: 9.063 min Scan# 1016
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion: 77 Resp: 782465
Ion Ratio Lower Upper
77 100
123 46.9 35.8 53.8
65 12.8 10.5 15.7



#23
Isophorone
Concen: 19.673 ng/ul
RT: 9.593 min Scan# 1106
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion: 82 Resp: 1560192
Ion Ratio Lower Upper
82 100
95 7.0 5.5 8.3
138 17.2 13.5 20.3









#25
2-Nitrophenol
Concen: 20.462 ng/ul
RT: 9.769 min Scan# 1136
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:139 Resp: 363378
Ion Ratio Lower Upper
139 100
65 49.6 39.1 58.7
109 29.8 23.8 35.6



#26
2,4-Dimethylphenol
Concen: 19.777 ng/ul
RT: 9.834 min Scan# 1147
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:107 Resp: 686896
Ion Ratio Lower Upper
107 100
121 50.4 40.0 60.0
122 85.2 69.1 103.7





#27

Bis(2-Chloroethoxy)methane

Concen: 19.900 ng/ul

RT: 10.075 min Scan# 1188

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion: 93 Resp: 996352

Ion Ratio Lower Upper

93 100

95 31.7 26.1 39.1

123 10.8 8.9 13.3

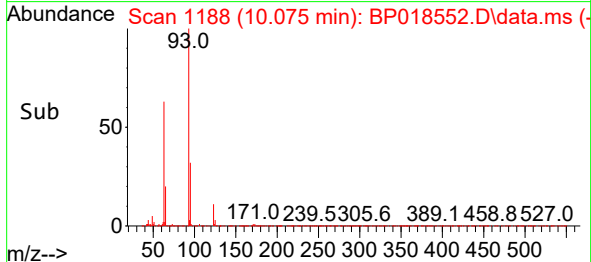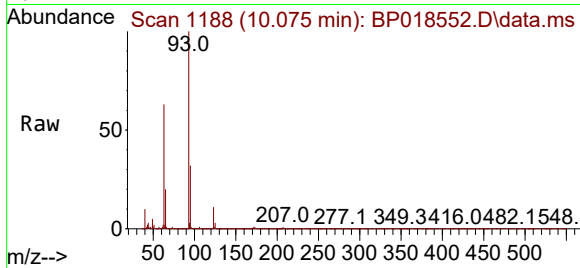

#29

2,4-Dichlorophenol

Concen: 20.092 ng/ul

RT: 10.305 min Scan# 1227

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:162 Resp: 656356


Ion Ratio Lower Upper

162 100

164 67.4 51.7 77.5

98 35.0 29.2 43.8


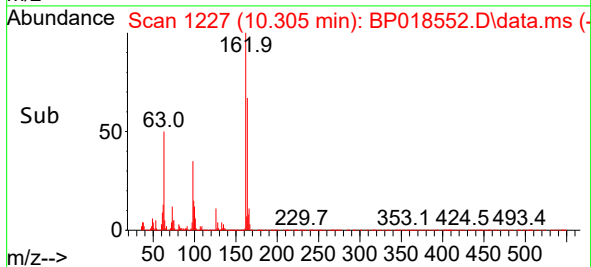

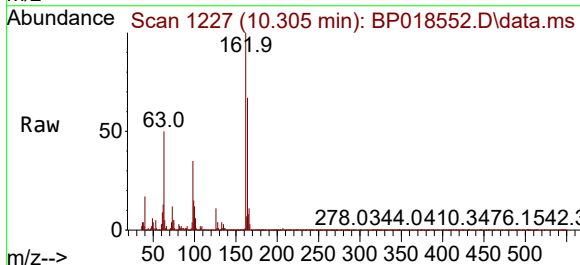




#30
Naphthalene
Concen: 20.020 ng/ul
RT: 10.704 min Scan# 1295
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:128 Resp: 2183026
Ion Ratio Lower Upper
128 100
129 10.9 8.9 13.3
127 13.3 10.5 15.7

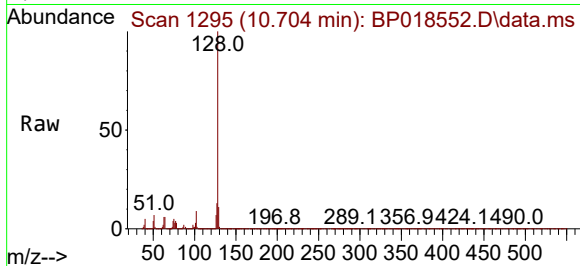

#32
4-Chloroaniline
Concen: 21.824 ng/ul
RT: 10.816 min Scan# 1314
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:127 Resp: 921953
Ion Ratio Lower Upper
127 100
129 32.2 25.6 38.4




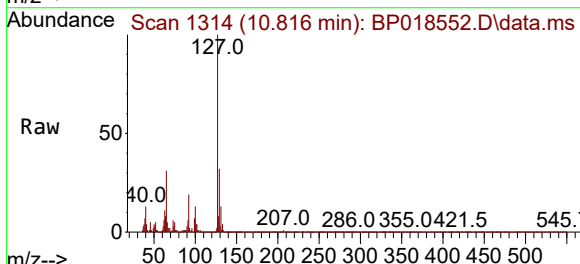




#33
Hexachlorobutadiene
Concen: 19.871 ng/ul
RT: 10.993 min Scan# 1344
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:225 Resp: 434741
Ion Ratio Lower Upper
225 100
223 64.0 49.5 74.3
227 65.9 50.9 76.3

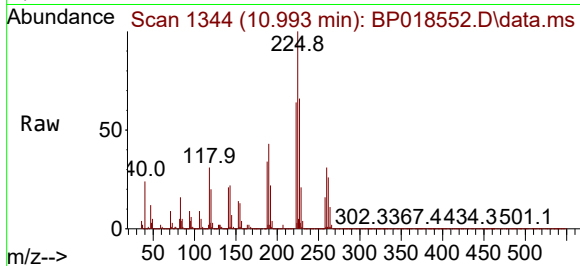

#34
Caprolactam
Concen: 18.523 ng/ul
RT: 11.593 min Scan# 1446
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:113 Resp: 185542
Ion Ratio Lower Upper
113 100
55 161.9 133.7 200.5
56 119.4 97.4 146.2



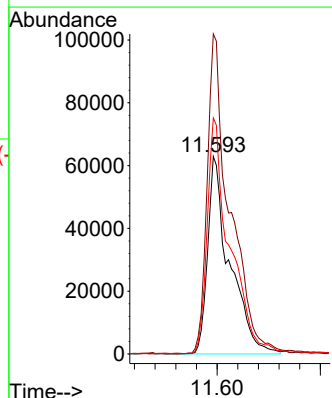
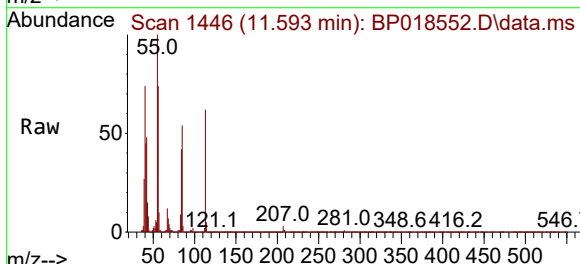




#35
4-Chloro-3-methylphenol
Concen: 19.339 ng/ul
RT: 11.940 min Scan# 1506
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:107 Resp: 707743
Ion Ratio Lower Upper
107 100
144 25.9 21.0 31.6
142 80.1 63.6 95.4

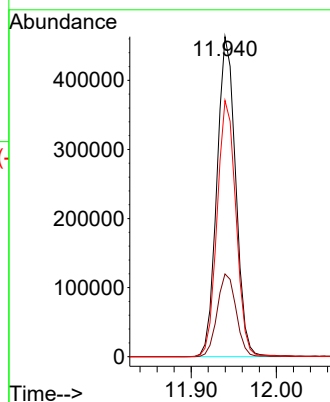

#36
2-Methylnaphthalene
Concen: 19.864 ng/ul
RT: 12.316 min Scan# 1569
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:142 Resp: 1534496
Ion Ratio Lower Upper
142 100
141 89.5 71.4 107.0


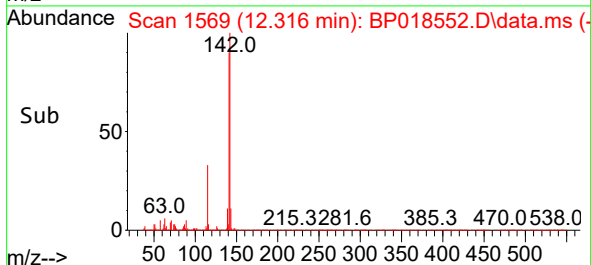

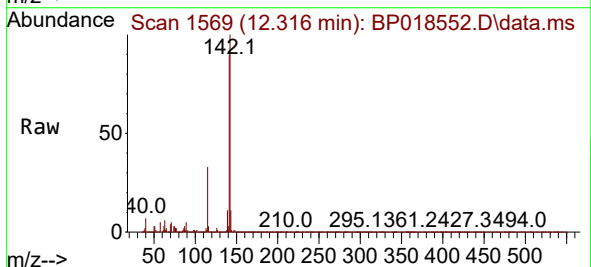


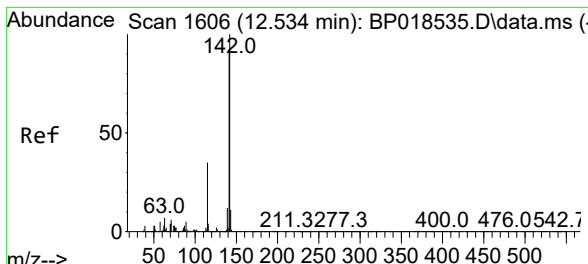

#37
 1-Methylnaphthalene
 Concen: 19.884 ng/ul
 RT: 12.534 min Scan# 1606
 Delta R.T. -0.012 min
 Lab File: BP018552.D
 Acq: 03 Dec 2023 12:59




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020705


Tgt Ion:142 Resp: 1551235
 Ion Ratio Lower Upper
 142 100
 141 91.7 73.5 110.3
 116 3.6 2.8 4.2

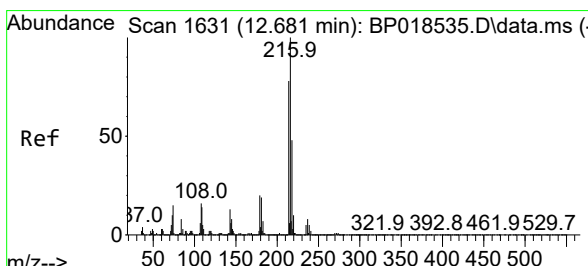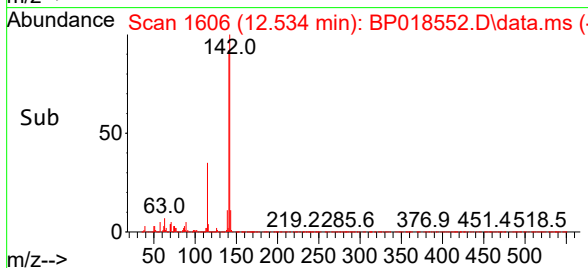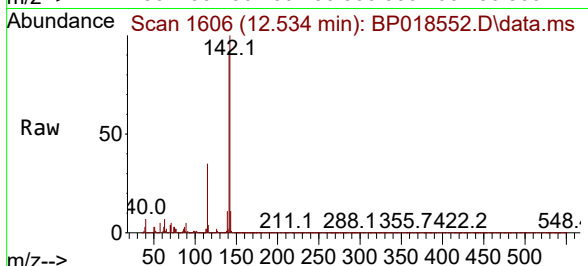

#39
 1,2,4,5-Tetrachlorobenzene
 Concen: 20.679 ng/ul
 RT: 12.681 min Scan# 1631
 Delta R.T. -0.012 min
 Lab File: BP018552.D
 Acq: 03 Dec 2023 12:59

Tgt Ion:216 Resp: 867366
 Ion Ratio Lower Upper
 216 100
 214 79.2 63.9 95.9
 179 20.2 16.3 24.5
 108 15.3 12.6 19.0

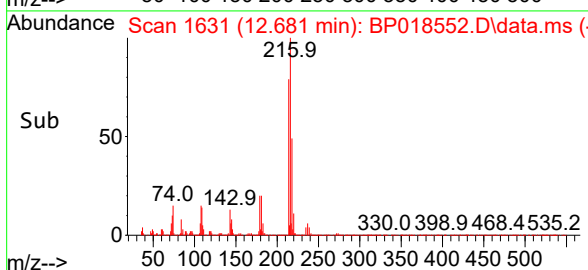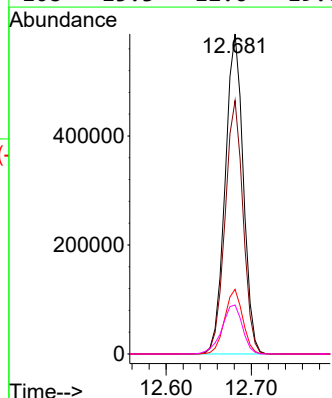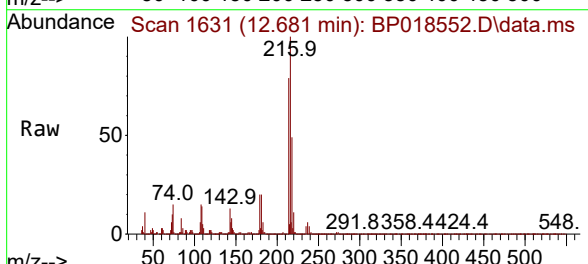



#40

Hexachlorocyclopentadiene

Concen: 18.896 ng/ul

RT: 12.663 min Scan# 1628

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:237 Resp: 469779

Ion Ratio Lower Upper

237 100

235 62.0 49.4 74.0

272 12.2 9.8 14.8



#41

2,4,6-Trichlorophenol

Concen: 20.202 ng/ul

RT: 12.922 min Scan# 1672

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:196 Resp: 545101


Ion Ratio Lower Upper

196 100

198 96.3 76.9 115.3

200 31.8 25.0 37.6





#42

2,4,5-Trichlorophenol

Concen: 20.188 ng/ul

RT: 12.993 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:196 Resp: 590558

Ion Ratio Lower Upper

196 100

198 97.4 77.9 116.9

200 31.1 25.2 37.8



#43

1,1'-Biphenyl

Concen: 20.549 ng/ul

RT: 13.328 min Scan# 1741

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:154 Resp: 2054592


Ion Ratio Lower Upper

154 100

153 39.6 32.8 49.2

76 12.8 10.7 16.1









#44
2-Chloronaphthalene
Concen: 20.584 ng/ul
RT: 13.363 min Scan# 1747
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:162 Resp: 1625490
Ion Ratio Lower Upper
162 100
164 32.7 25.7 38.5
127 37.7 30.3 45.5



#45
2-Nitroaniline
Concen: 20.093 ng/ul
RT: 13.569 min Scan# 1782
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion: 65 Resp: 430145
Ion Ratio Lower Upper
65 100
92 72.2 56.9 85.3
138 106.4 88.2 132.2


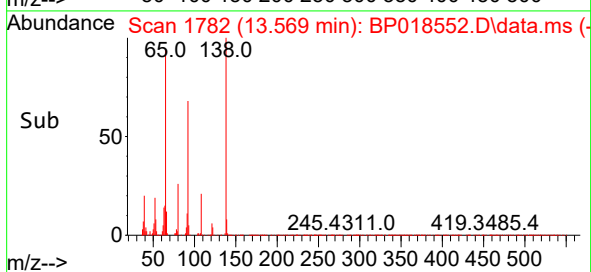






#47
Dimethylphthalate
Concen: 20.029 ng/ul
RT: 13.951 min Scan# 1847
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:163 Resp: 2034311
Ion Ratio Lower Upper
163 100
194 3.8 3.2 4.8
164 10.2 8.0 12.0

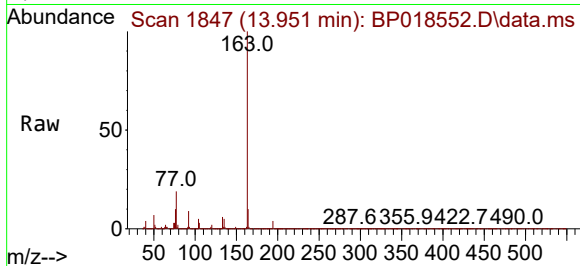

#48
2,6-Dinitrotoluene
Concen: 20.448 ng/ul
RT: 14.069 min Scan# 1867
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:165 Resp: 392389
Ion Ratio Lower Upper
165 100
89 53.2 46.6 70.0
121 20.4 17.3 25.9




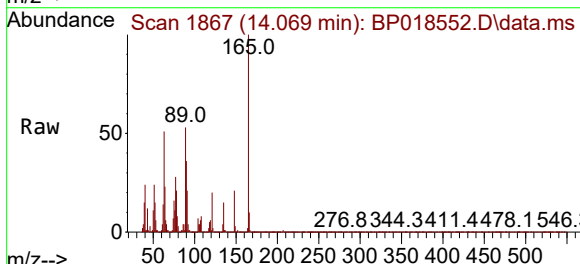




#50
Acenaphthylene
Concen: 20.520 ng/ul
RT: 14.210 min Scan# 1891
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:152 Resp: 2621213
Ion Ratio Lower Upper
152 100
151 19.8 15.9 23.9
153 13.0 10.6 16.0

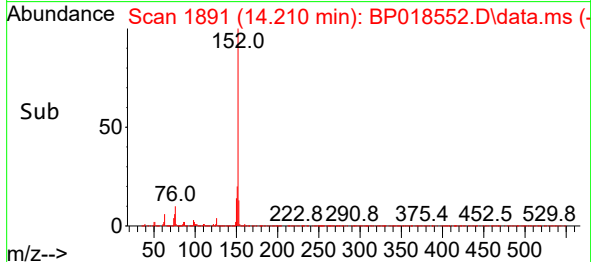

#51
3-Nitroaniline
Concen: 20.750 ng/ul
RT: 14.393 min Scan# 1922
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:138 Resp: 397475
Ion Ratio Lower Upper
138 100
108 11.9 9.5 14.3
92 120.2 93.1 139.7



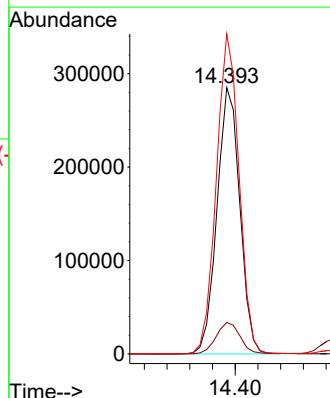





#52
Acenaphthene
Concen: 20.337 ng/ul
RT: 14.551 min Scan# 1949
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:153 Resp: 1717660
Ion Ratio Lower Upper
153 100
152 47.2 38.1 57.1
154 88.3 71.7 107.5



#53
2,4-Dinitrophenol
Concen: 16.593 ng/ul
RT: 14.598 min Scan# 1957
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:184 Resp: 168751
Ion Ratio Lower Upper
184 100
63 59.8 48.2 72.4
154 60.5 49.1 73.7



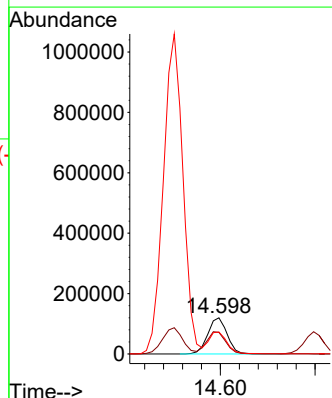





#55
4-Nitrophenol
Concen: 19.994 ng/ul
RT: 14.698 min Scan# 1974
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:109 Resp: 255839
Ion Ratio Lower Upper
109 100
139 137.4 109.0 163.4
65 131.0 106.2 159.4



#56
Dibenzofuran
Concen: 20.220 ng/ul
RT: 14.887 min Scan# 2006
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:168 Resp: 2373587
Ion Ratio Lower Upper
168 100
139 35.1 29.1 43.7









#57
2,4-Dinitrotoluene
Concen: 20.210 ng/ul
RT: 14.851 min Scan# 2000
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:165 Resp: 545528
Ion Ratio Lower Upper
165 100
63 39.9 32.7 49.1
182 2.7 2.1 3.1

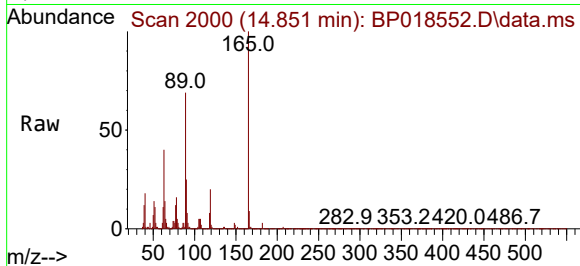

#58
2,3,4,6-Tetrachlorophenol
Concen: 19.515 ng/ul
RT: 15.110 min Scan# 2044
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:232 Resp: 478851
Ion Ratio Lower Upper
232 100
131 40.4 33.8 50.8
130 2.3 1.8 2.8
166 29.8 24.7 37.1



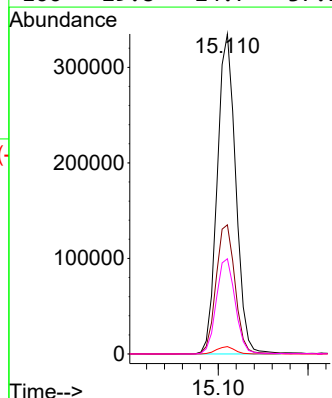
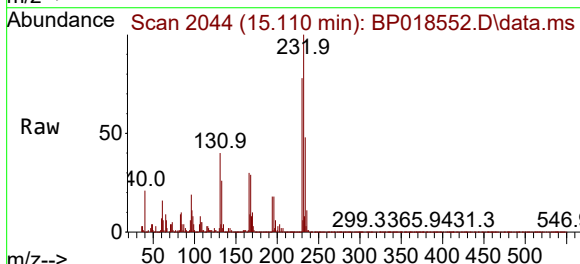




#59
Diethylphthalate
Concen: 19.441 ng/ul
RT: 15.316 min Scan# 2079
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:149 Resp: 1932169
Ion Ratio Lower Upper
149 100
177 23.1 18.2 27.4
150 12.2 9.9 14.9

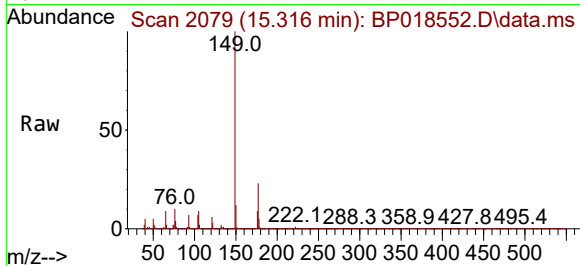

#61
Fluorene
Concen: 20.350 ng/ul
RT: 15.534 min Scan# 2116
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:166 Resp: 1890206
Ion Ratio Lower Upper
166 100
165 97.9 78.0 117.0
167 13.6 10.8 16.2



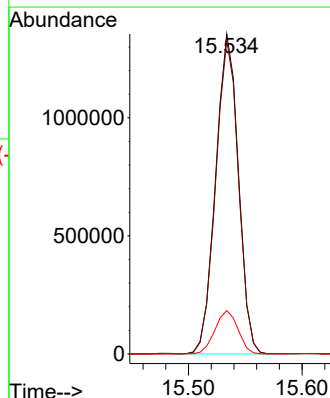
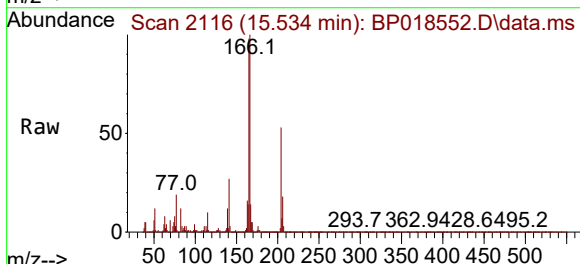




#62
4-Chlorophenyl-phenylether
Concen: 20.469 ng/ul
RT: 15.534 min Scan# 2116
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:204 Resp: 997182
Ion Ratio Lower Upper
204 100
206 33.6 27.1 40.7
141 51.1 45.8 68.8

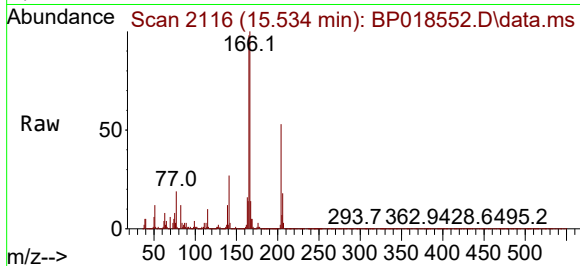

#63
4-Nitroaniline
Concen: 20.854 ng/ul
RT: 15.557 min Scan# 2120
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:138 Resp: 380555
Ion Ratio Lower Upper
138 100
92 51.9 42.3 63.5
108 76.2 62.0 93.0




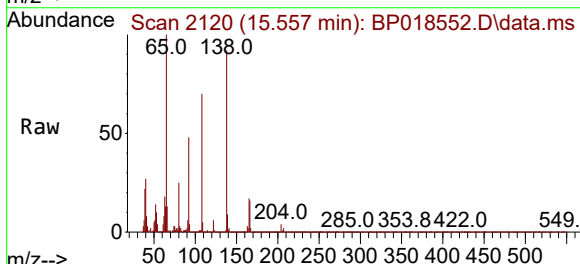




#66
4,6-Dinitro-2-methylphenol
Concen: 18.834 ng/ul
RT: 15.610 min Scan# 2129
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:198 Resp: 284550
Ion Ratio Lower Upper
198 100
182 4.3 3.4 5.2
77 24.6 20.6 30.8



#67
N-Nitrosodiphenylamine
Concen: 20.485 ng/ul
RT: 15.745 min Scan# 2152
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:169 Resp: 1599733
Ion Ratio Lower Upper
169 100
168 67.2 53.1 79.7
167 36.5 29.1 43.7







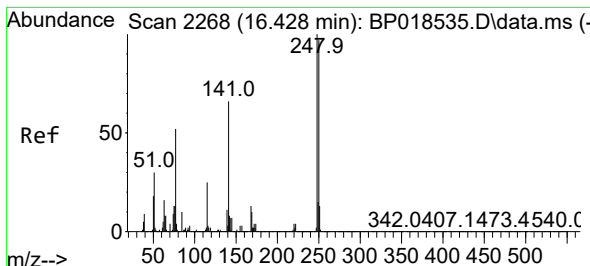

#68
4-Bromophenyl-phenylether
Concen: 19.854 ng/ul
RT: 16.428 min Scan# 2268
Delta R.T. -0.006 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:248 Resp: 590718
Ion Ratio Lower Upper
248 100
250 97.5 79.3 118.9
141 64.8 57.2 85.8

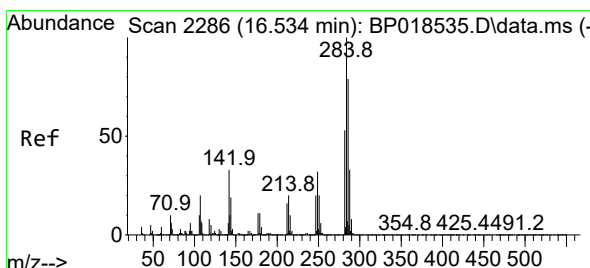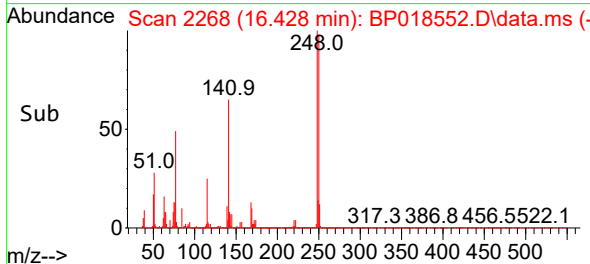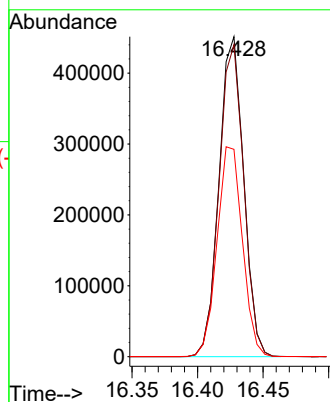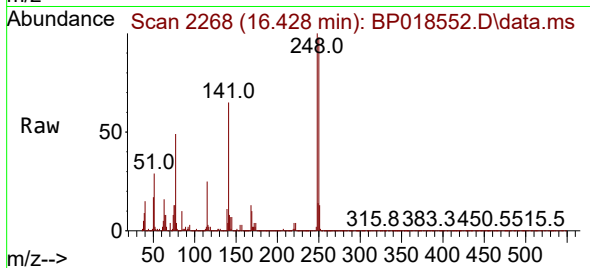

#69
Hexachlorobenzene
Concen: 20.367 ng/ul
RT: 16.534 min Scan# 2286
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:284 Resp: 676574
Ion Ratio Lower Upper
284 100
142 32.9 25.8 38.6
249 31.8 24.9 37.3

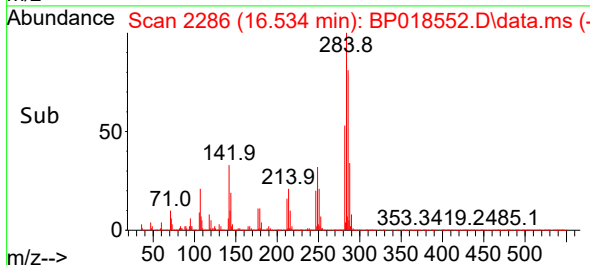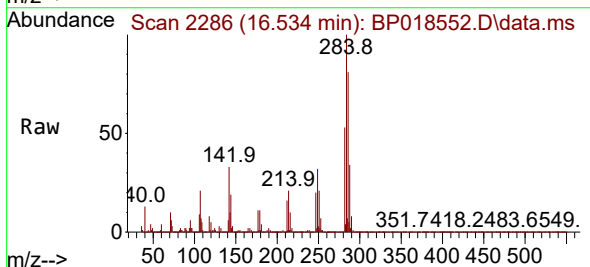



#70

Atrazine

Concen: 21.734 ng/ul

RT: 16.704 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:200 Resp: 504623

Ion Ratio Lower Upper

200 100

173 25.8 21.0 31.4

215 50.1 38.2 57.2



#71

Pentachlorophenol

Concen: 18.503 ng/ul

RT: 16.881 min Scan# 2345

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:266 Resp: 365546


Ion Ratio Lower Upper

266 100

264 63.7 50.2 75.2

268 63.1 50.5 75.7





#72

Phenanthrene

Concen: 20.223 ng/ul

RT: 17.275 min Scan# 2412

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:178 Resp: 2878387

Ion Ratio Lower Upper

178 100

179 15.4 12.3 18.5

176 19.0 15.4 23.2



#74

Anthracene

Concen: 20.479 ng/ul

RT: 17.369 min Scan# 2428

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:178 Resp: 2921832


Ion Ratio Lower Upper

178 100

179 15.3 12.5 18.7

176 18.5 15.0 22.6

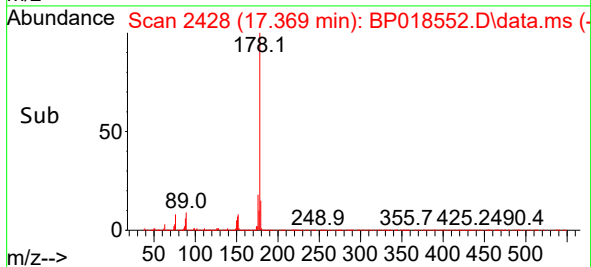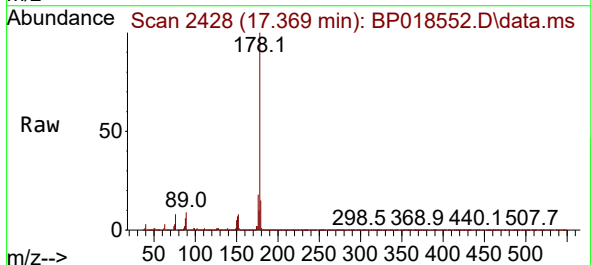



#75

1,2,3,4-Tetrachlorobenzene

Concen: 21.465 ng/uL

RT: 13.287 min Scan# 1734

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:216 Resp: 874695

Ion Ratio Lower Upper

216 100

214 76.8 61.4 92.2

218 47.2 39.2 58.8

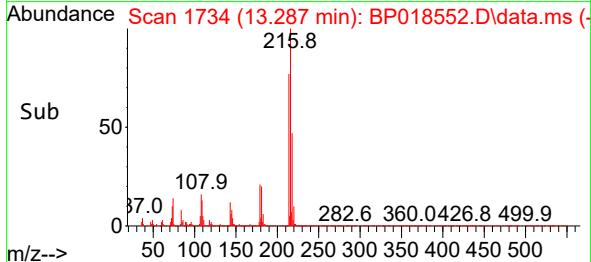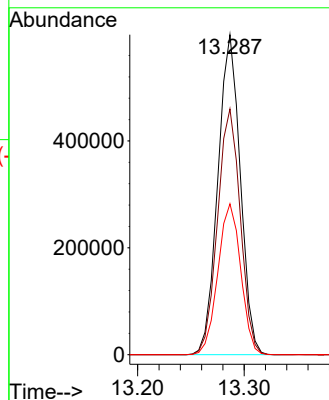

#76

Pentachlorobenzene

Concen: 20.954 ng/uL

RT: 14.804 min Scan# 1992

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:250 Resp: 838749


Ion Ratio Lower Upper

250 100

248 62.4 50.6 75.8

252 63.7 51.3 76.9


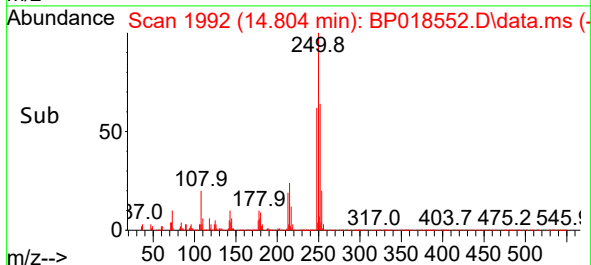
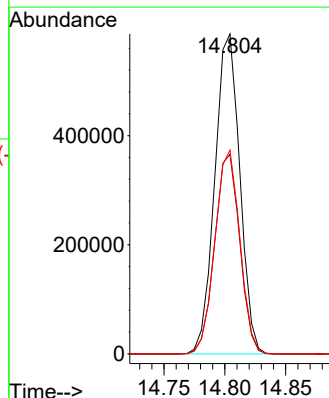
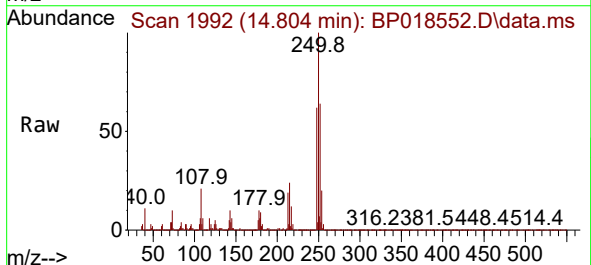




#77
Carbazole
Concen: 21.455 ng/ul
RT: 17.639 min Scan# 2474
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59




Instrument :
BNA_P
ClientSampleId :
SSTD020705


Tgt Ion:167 Resp: 2439694
Ion Ratio Lower Upper
167 100
166 21.5 17.1 25.7
139 12.3 10.2 15.4



#78
Di-n-butylphthalate
Concen: 19.508 ng/ul
RT: 18.198 min Scan# 2569
Delta R.T. -0.012 min
Lab File: BP018552.D
Acq: 03 Dec 2023 12:59

Tgt Ion:149 Resp: 2953692
Ion Ratio Lower Upper
149 100
150 9.2 7.4 11.2
104 4.8 3.9 5.9

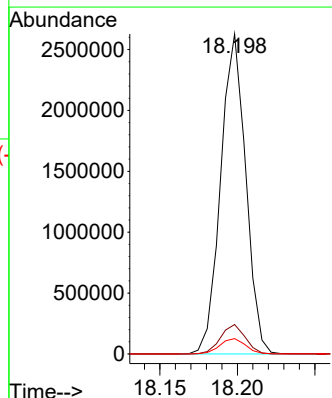



#80

Fluoranthene

Concen: 20.924 ng/ul

RT: 19.245 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:202 Resp: 2995102

Ion Ratio Lower Upper

202 100

101 10.9 9.1 13.7

100 8.3 7.1 10.7

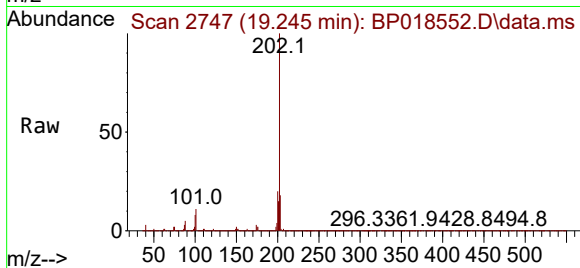

#82

Pyrene

Concen: 20.950 ng/ul

RT: 19.598 min Scan# 2807

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:202 Resp: 3025339


Ion Ratio Lower Upper

202 100

101 12.9 11.0 16.4

100 10.4 9.1 13.7

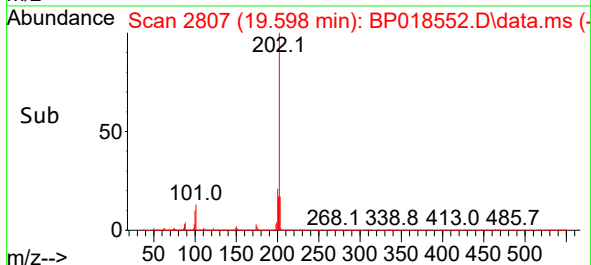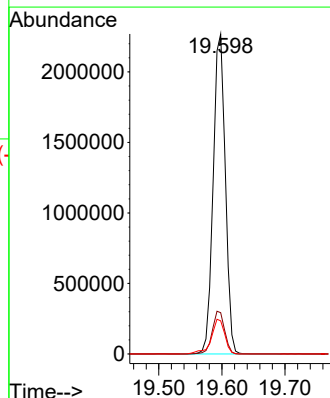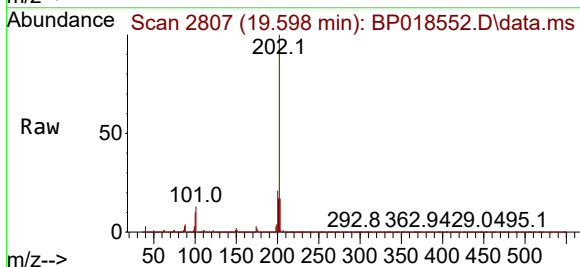



#83

Butylbenzylphthalate

Concen: 18.607 ng/ul

RT: 20.475 min Scan# 2956

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:149 Resp: 983687

Ion Ratio Lower Upper

149 100

91 70.6 56.6 85.0

206 21.6 17.4 26.0

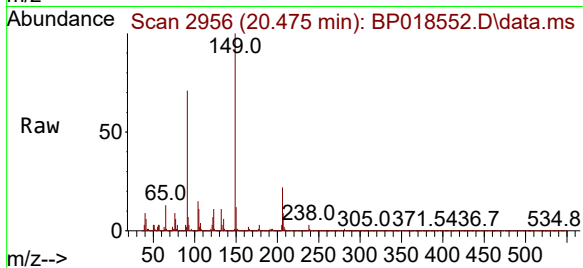

#84

3,3'-Dichlorobenzidine

Concen: 19.705 ng/ul

RT: 21.239 min Scan# 3086

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:252 Resp: 744931


Ion Ratio Lower Upper

252 100

254 63.6 51.0 76.4

126 11.1 7.8 11.6

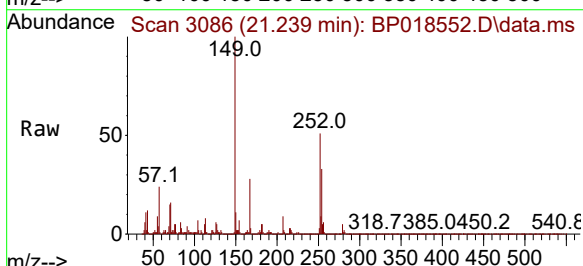



#85

Benzo(a)anthracene

Concen: 19.909 ng/ul

RT: 21.304 min Scan# 3097

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:228 Resp: 2513937

Ion Ratio Lower Upper

228 100

229 19.7 15.7 23.5

226 27.1 21.9 32.9

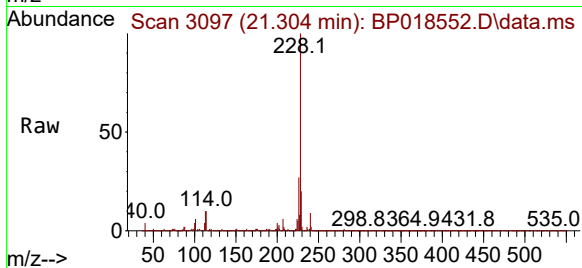

#86

Bis(2-ethylhexyl)phthalate

Concen: 18.016 ng/ul

RT: 21.239 min Scan# 3086

Delta R.T. -0.006 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:149 Resp: 1309048


Ion Ratio Lower Upper

149 100

167 27.9 22.2 33.2

279 4.5 3.3 4.9

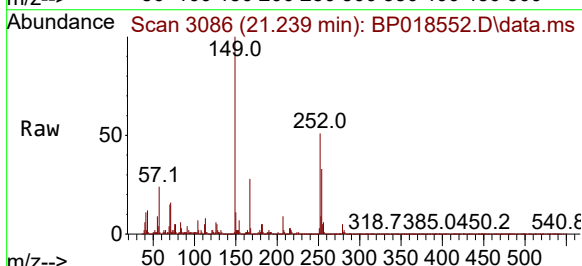



#87

Chrysene

Concen: 19.893 ng/ul

RT: 21.357 min Scan# 3106

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:228 Resp: 2313225

Ion Ratio Lower Upper

228 100

226 29.9 23.9 35.9

229 19.3 15.6 23.4



#89

Di-n-octyl phthalate

Concen: 16.357 ng/ul




RT: 22.151 min Scan# 3241


Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Tgt Ion:149 Resp: 1934742

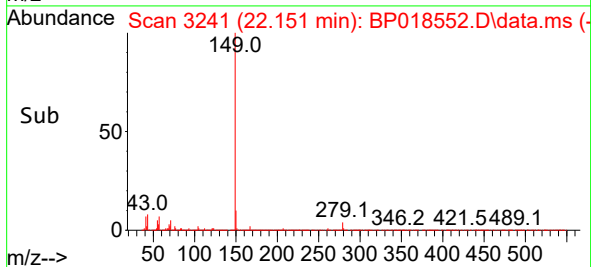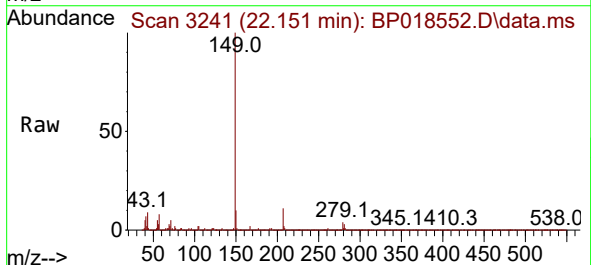



#90

Benzo(b)fluoranthene

Concen: 19.318 ng/ul

RT: 22.969 min Scan# 3380

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:252 Resp: 2307441

Ion Ratio Lower Upper

252 100

253 21.9 17.3 25.9

125 10.1 7.8 11.6



#91

Benzo(k)fluoranthene

Concen: 19.401 ng/ul

RT: 23.016 min Scan# 3388

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:252 Resp: 2242142


Ion Ratio Lower Upper

252 100

253 22.0 17.7 26.5

125 10.3 8.0 12.0





#93

Benzo(a)pyrene

Concen: 20.176 ng/ul

RT: 23.586 min Scan# 3485

Delta R.T. -0.012 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:252 Resp: 2202046

Ion Ratio Lower Upper

252 100

253 22.0 17.8 26.8

125 11.3 9.2 13.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 21.553 ng/ul

RT: 26.157 min Scan# 3922

Delta R.T. -0.023 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59




Tgt Ion:276 Resp: 2810548


Ion Ratio Lower Upper

276 100

138 22.6 19.4 29.2

277 24.5 19.8 29.6





#95

Dibenzo(a,h)anthracene

Concen: 21.608 ng/ul

RT: 26.180 min Scan# 3926

Delta R.T. -0.017 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Instrument :

BNA_P

ClientSampleId :

SSTD020705





Tgt Ion:278 Resp: 2343968

Ion Ratio Lower Upper

278 100

139 16.2 13.0 19.6

279 23.8 18.7 28.1



#96

Benzo(g,h,i)perylene

Concen: 21.657 ng/ul

RT: 26.921 min Scan# 4052

Delta R.T. -0.017 min

Lab File: BP018552.D

Acq: 03 Dec 2023 12:59

Tgt Ion:276 Resp: 2272782

Ion Ratio Lower Upper

276 100

138 21.2 18.1 27.1

277 24.4 19.4 29.0

