

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018513.D
 Acq On : 02 Dec 2023 13:12
 Operator : MA/JU
 Sample : 05416-21
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH4

Quant Time: Dec 02 21:58:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 01 21:56:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	492091	20.000	ng/u1	0.00
20) Naphthalene-d8	10.657	136	1992082	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.487	164	1211146	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.233	188	2537386	20.000	ng/u1	0.00
79) Chrysene-d12	21.322	240	2452425	20.000	ng/u1	0.00
88) Perylene-d12	23.692	264	2922792	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	15001	1.039	ng/uL	0.00
4) Pyridine-d5	3.699	84	65700	1.699	ng/u1	0.00
7) Phenol-d5	7.028	99	395667	8.012	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	294489	10.062	ng/u1	0.00
11) 2-Chlorophenol-d4	7.393	132	351839	9.131	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	299210	7.487	ng/u1	-0.01
21) Nitrobenzene-d5	9.022	128	168173	9.485	ng/u1	0.00
24) 2-Nitrophenol-d4	9.740	143	165687	9.014	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.275	165	326325	8.682	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.799	131	411668	8.380	ng/u1	0.00
46) Dimethylphthalate-d6	13.904	166	1056409	9.773	ng/u1	0.00
49) Acenaphthylene-d8	14.181	160	1180630	9.919	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.681	143	64320	3.625	ng/u1	-0.01
60) Fluorene-d10	15.481	176	918311	10.121	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	46802	3.076	ng/u1	-0.01
73) Anthracene-d10	17.333	188	1369214	10.264	ng/u1	0.00
81) Pyrene-d10	19.569	212	1757639	9.207	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.539	264	1811081	10.627	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.687	105	127163	2.135	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018513.D
Acq On : 02 Dec 2023 13:12
Operator : MA/JU
Sample : 05416-21
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH4


Quant Time: Dec 02 21:58:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 01 21:56:43 2023
Response via : Initial Calibration

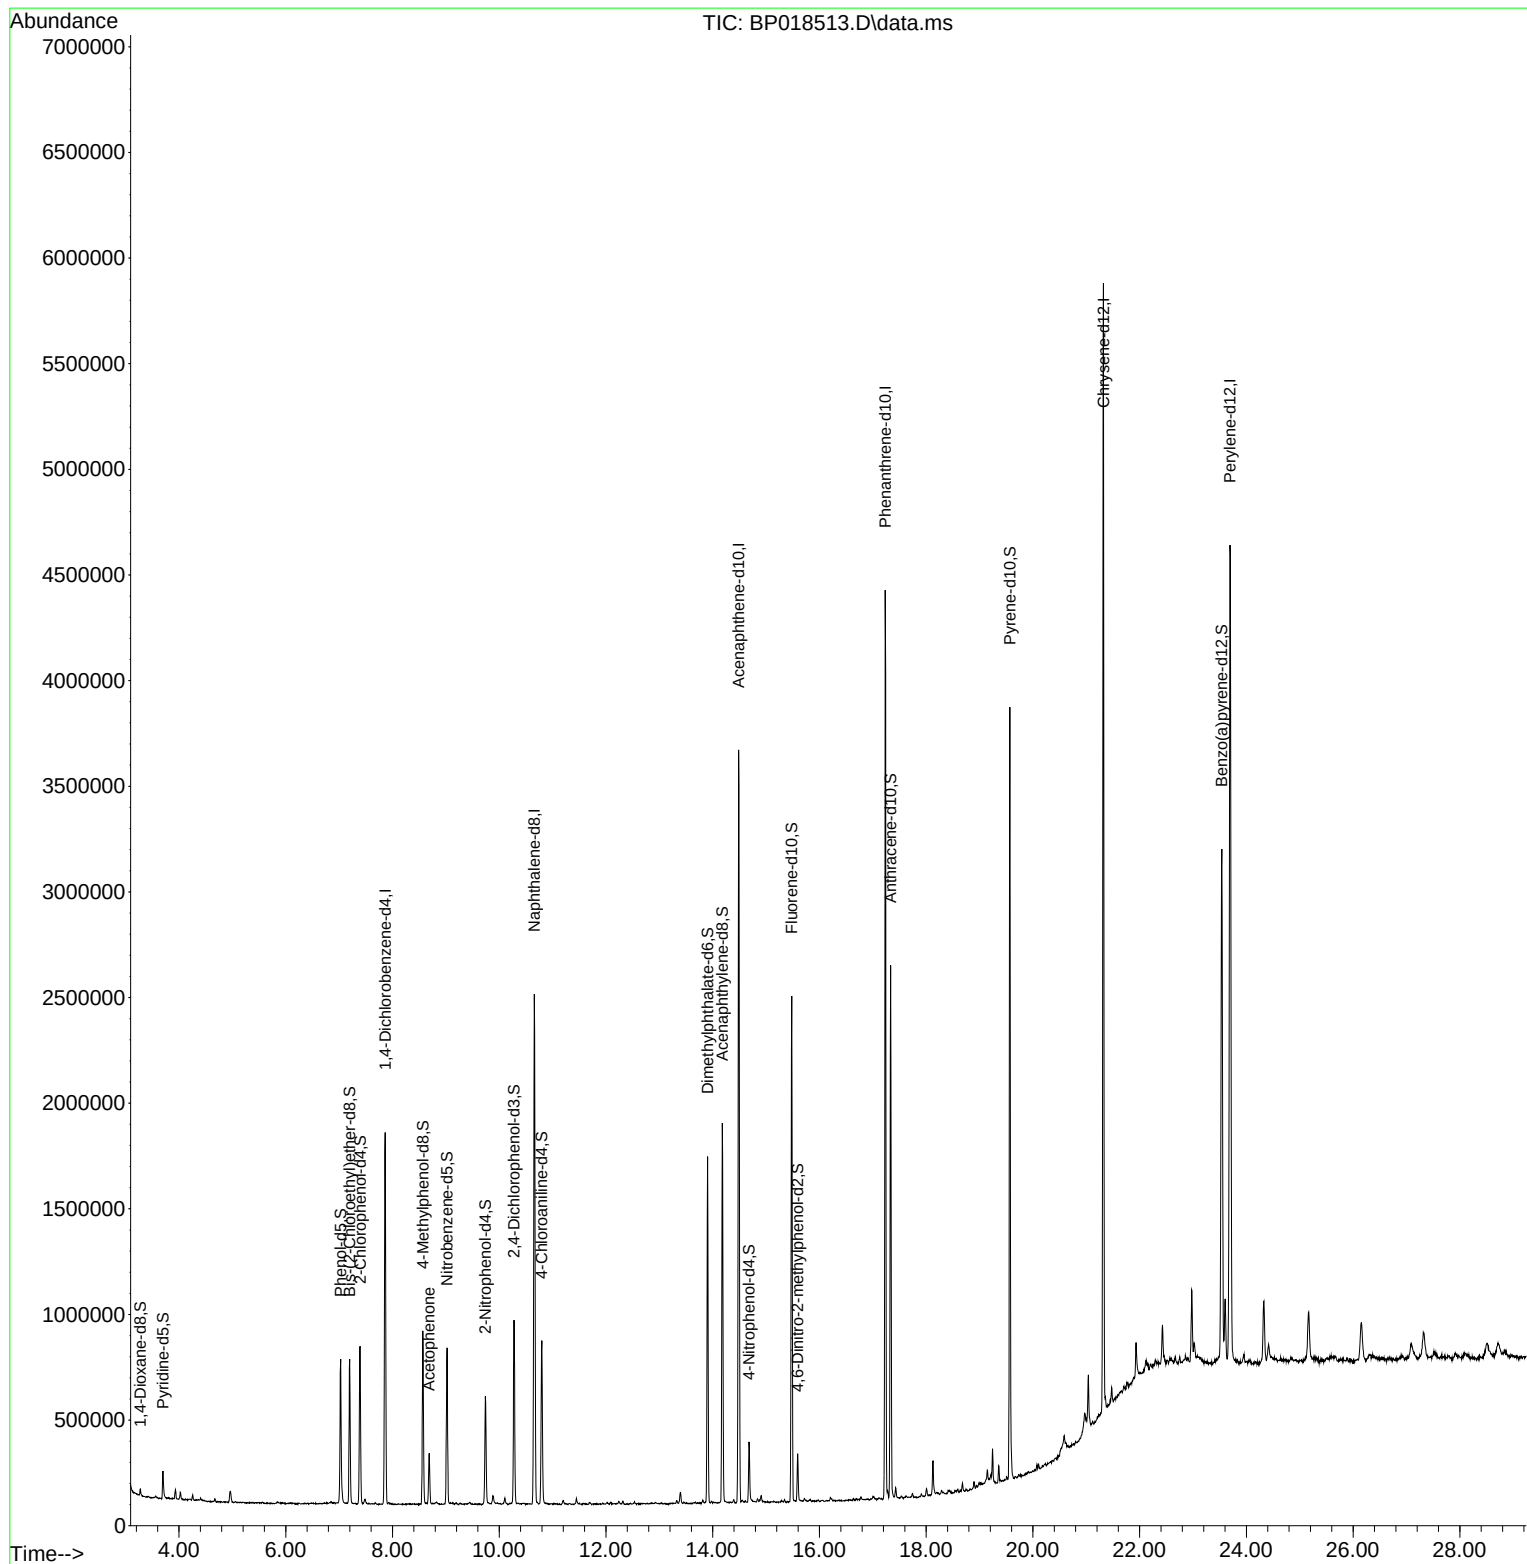

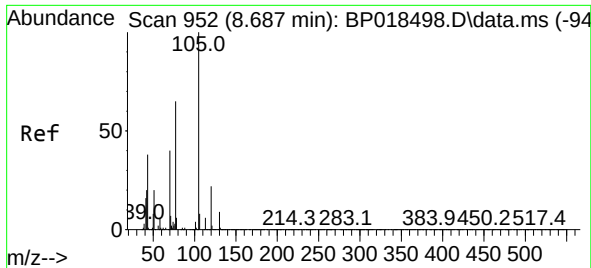

#16
 Acetophenone
 Concen: 2.135 ng/ul
 RT: 8.687 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BP018513.D
 Acq: 02 Dec 2023 13:12

Instrument :
 BNA_P
 ClientSampleId :
 C0AH4

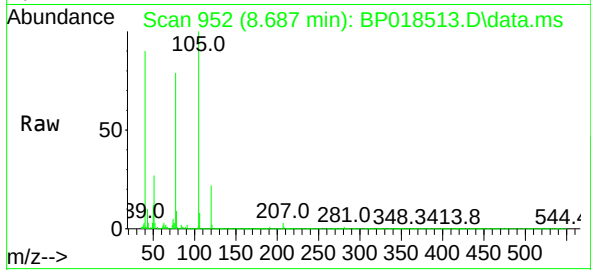

Tgt Ion:	105	Resp:	127163
Ion	Ratio	Lower	Upper
105	100		
77	78.5	59.4	89.0
51	27.1	19.4	29.0

