

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018482.D
 Acq On : 01 Dec 2023 18:29
 Operator : MA/JU
 Sample : PB157278BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK278

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	39	rVB	112394	149329	1.43%	0.148%
2	3.693	98	103	123	rBV	1433365	2090605	20.02%	2.071%
3	4.028	156	160	167	rVB	36502	52184	0.50%	0.052%
4	7.028	664	670	683	rVB	1581641	2467111	23.62%	2.444%
5	7.198	692	699	707	rBV	1346678	2054379	19.67%	2.035%
6	7.392	725	732	740	rBV	1582579	2459622	23.55%	2.436%
7	7.863	805	812	821	rVB	1229398	1924174	18.42%	1.906%
8	8.575	924	933	943	rBV	2020490	3188401	30.53%	3.158%
9	9.028	1001	1010	1019	rBV	1484822	2477756	23.72%	2.454%
10	9.745	1125	1132	1143	rBV	1226485	1950992	18.68%	1.932%
11	10.281	1216	1223	1231	rBV	1982196	3242857	31.05%	3.212%
12	10.663	1279	1288	1296	rBV	1757599	2899112	27.76%	2.871%
13	10.798	1303	1311	1324	rBV	2012572	3484185	33.36%	3.451%
14	12.251	1552	1558	1565	rVB3	40838	74675	0.71%	0.074%
15	13.398	1747	1753	1758	rBV2	34301	54090	0.52%	0.054%
16	13.910	1833	1840	1850	rBV	4151214	5564390	53.27%	5.511%
17	14.186	1880	1887	1896	rBV	4369777	6397770	61.25%	6.337%
18	14.492	1932	1939	1947	rBV	2991046	4341462	41.57%	4.300%
19	14.686	1965	1972	1983	rBV	1908911	2747339	26.30%	2.721%
20	14.910	2006	2010	2017	rVB4	12060	20802	0.20%	0.021%
21	15.486	2101	2108	2115	rBV	5510421	8158204	78.11%	8.080%
22	15.598	2118	2127	2143	rBV	1693483	2254148	21.58%	2.233%
23	15.721	2145	2148	2156	rVB3	28886	46624	0.45%	0.046%
24	16.268	2238	2241	2246	rVB6	9092	13788	0.13%	0.014%
25	16.915	2349	2351	2357	rVB4	11493	15330	0.15%	0.015%
26	17.027	2366	2370	2375	rBV2	11614	20108	0.19%	0.020%
27	17.239	2399	2406	2413	rBV	3819064	5423777	51.93%	5.372%
28	17.339	2416	2423	2434	rBV	6361738	9037213	86.52%	8.951%
29	17.615	2467	2470	2473	rBV3	10427	16359	0.16%	0.016%
30	18.127	2555	2557	2560	rBV4	17075	19881	0.19%	0.020%
31	19.151	2726	2731	2737	rBV3	88446	121026	1.16%	0.120%
32	19.215	2738	2742	2748	rVV	87799	115701	1.11%	0.115%
33	19.574	2797	2803	2810	rBV	8333786	10444873	100.00%	10.345%
34	21.327	3095	3101	3110	rBV	4216780	5398825	51.69%	5.347%
35	23.545	3471	3478	3486	rBV2	4143081	7772673	74.42%	7.699%
36	23.697	3498	3504	3516	rVB	2256309	4463429	42.73%	4.421%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018482.D
Acq On : 01 Dec 2023 18:29
Operator : MA/JU
Sample : PB157278BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK278

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 100963194

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018482.D
Acq On : 01 Dec 2023 18:29
Operator : MA/JU
Sample : PB157278BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK278

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

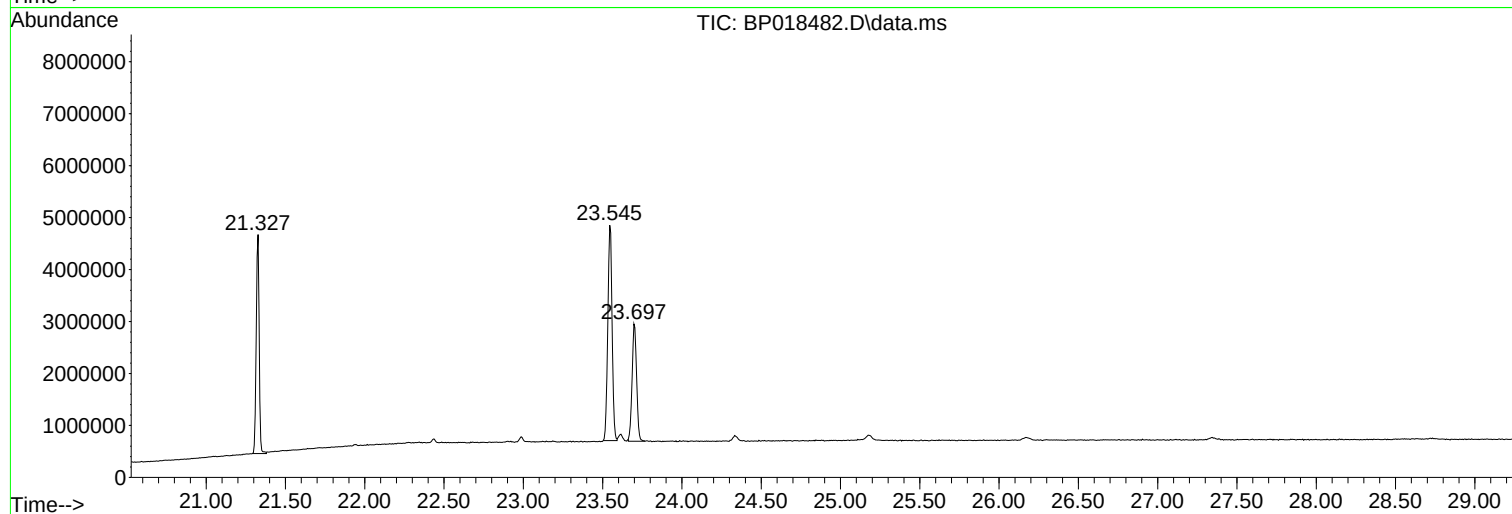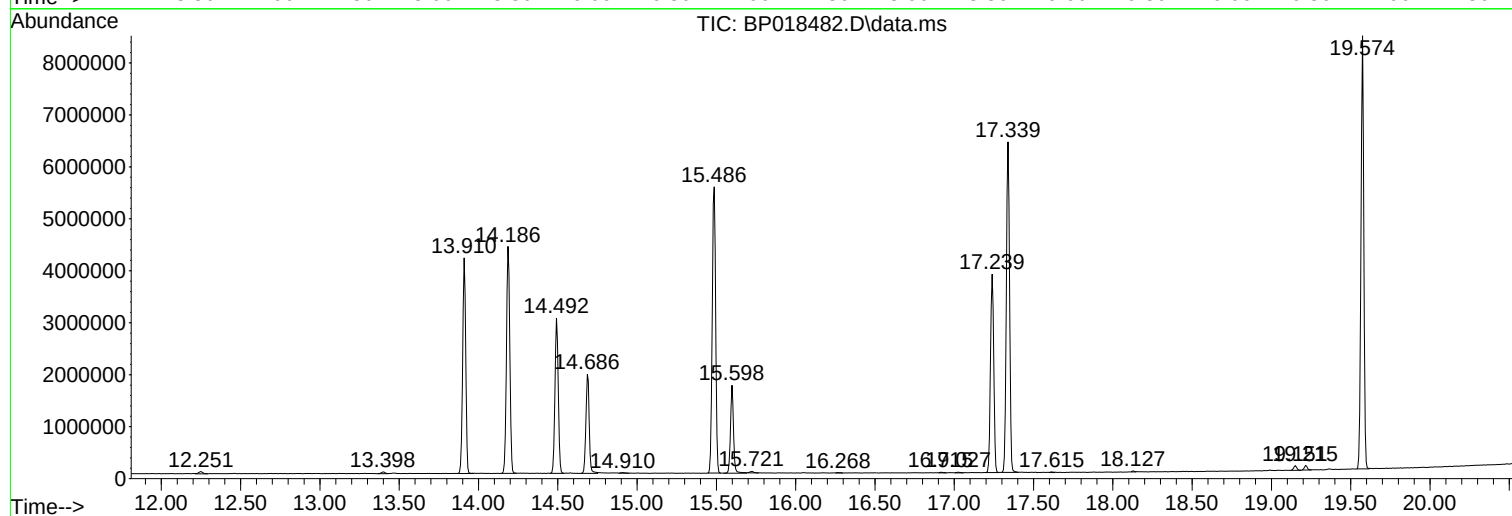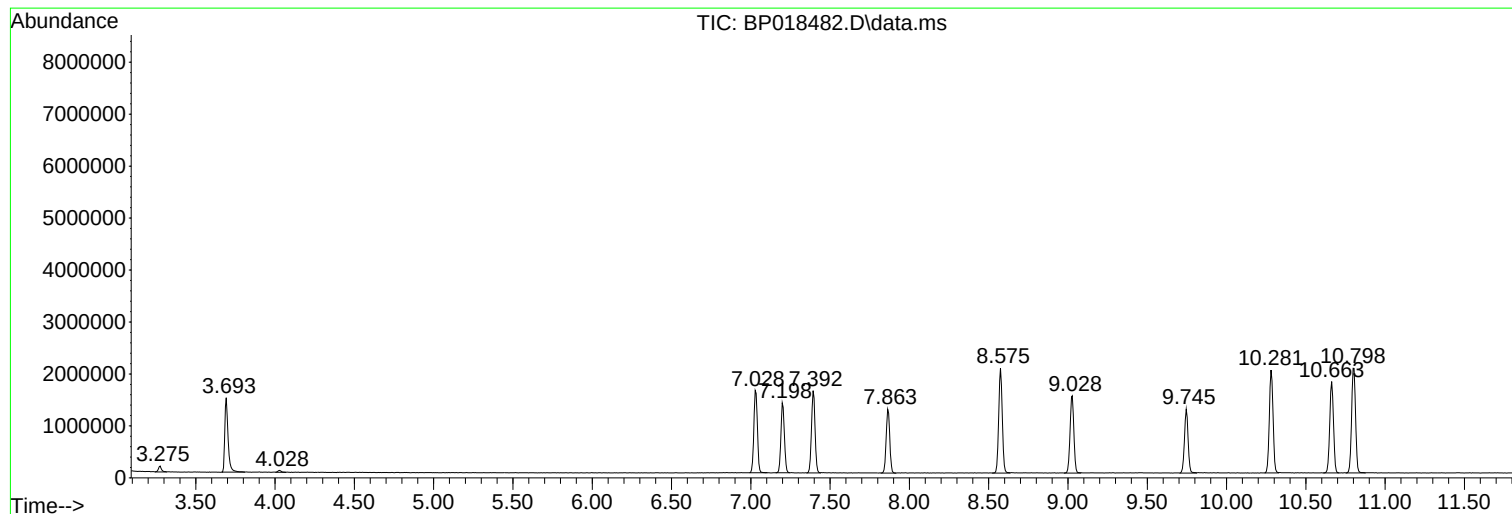

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018482.D
Acq On : 01 Dec 2023 18:29
Operator : MA/JU
Sample : PB157278BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK278

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018482.D
Acq On : 01 Dec 2023 18:29
Operator : MA/JU
Sample : PB157278BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK278

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc